
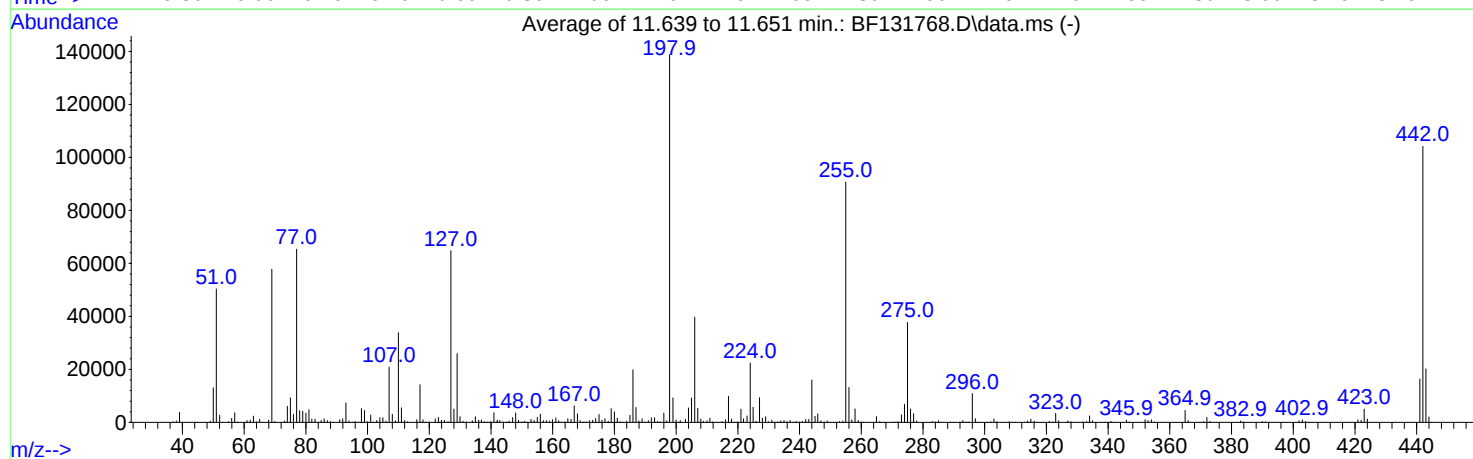


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
 Data File : BF131768.D
 Acq On : 22 Dec 2022 10:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 24 00:05:44 2022

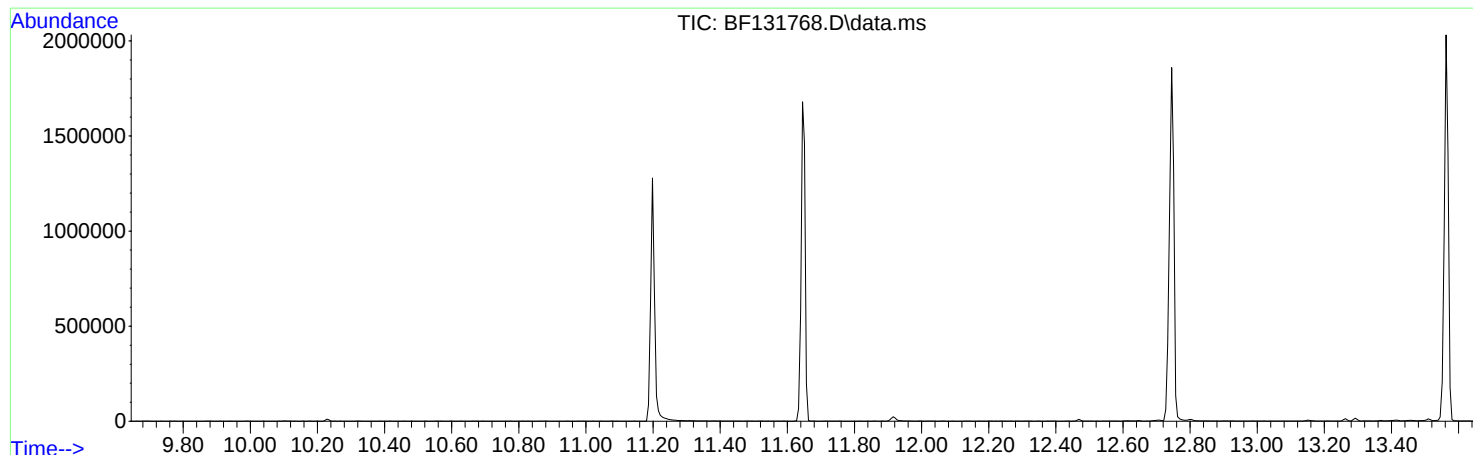




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	50379	PASS
68	69	0.00	2	1.5	876	PASS
69	198	0.00	100	41.6	57760	PASS
70	69	0.00	2	0.5	284	PASS
127	198	10	80	46.7	64784	PASS
197	198	0.00	2	0.5	637	PASS
198	198	100	100	100.0	138827	PASS
199	198	5	9	6.7	9267	PASS
275	198	10	60	27.2	37752	PASS
365	198	1	100	3.3	4550	PASS
441	198	0.01	100	11.8	16397	PASS
442	442	50	100	100.0	104197	PASS
443	442	15	24	19.4	20180	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131768.D
Acq On : 22 Dec 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 23 05:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

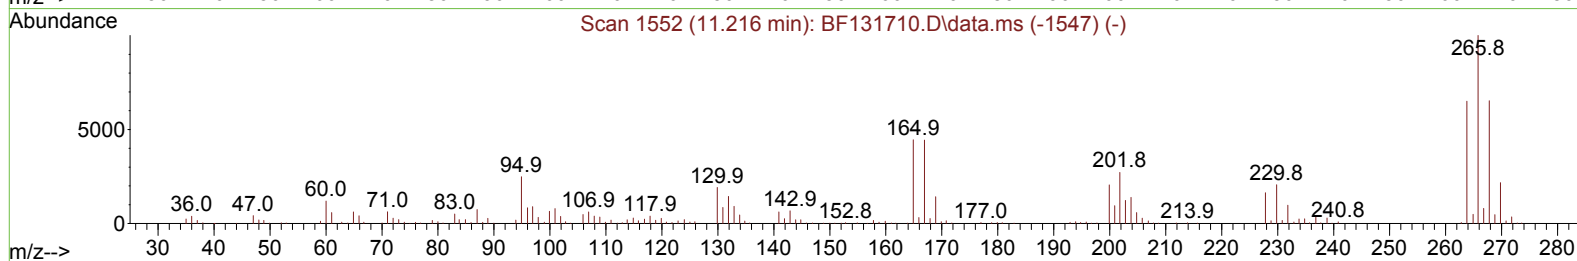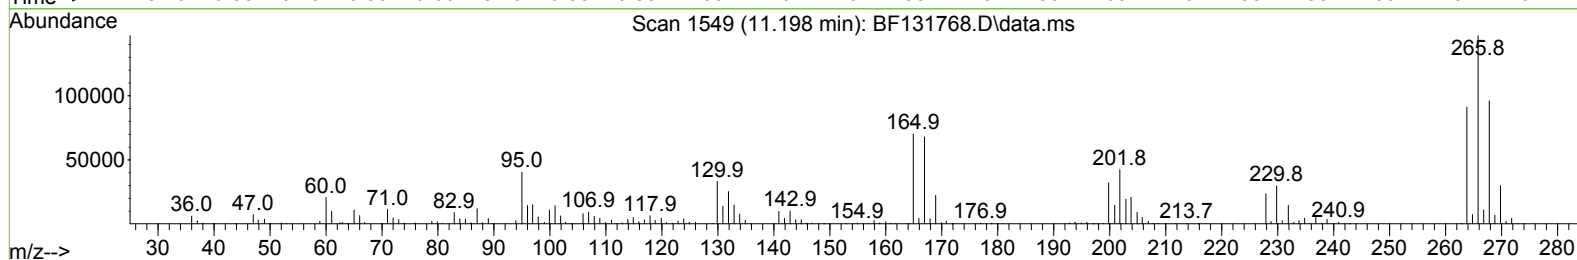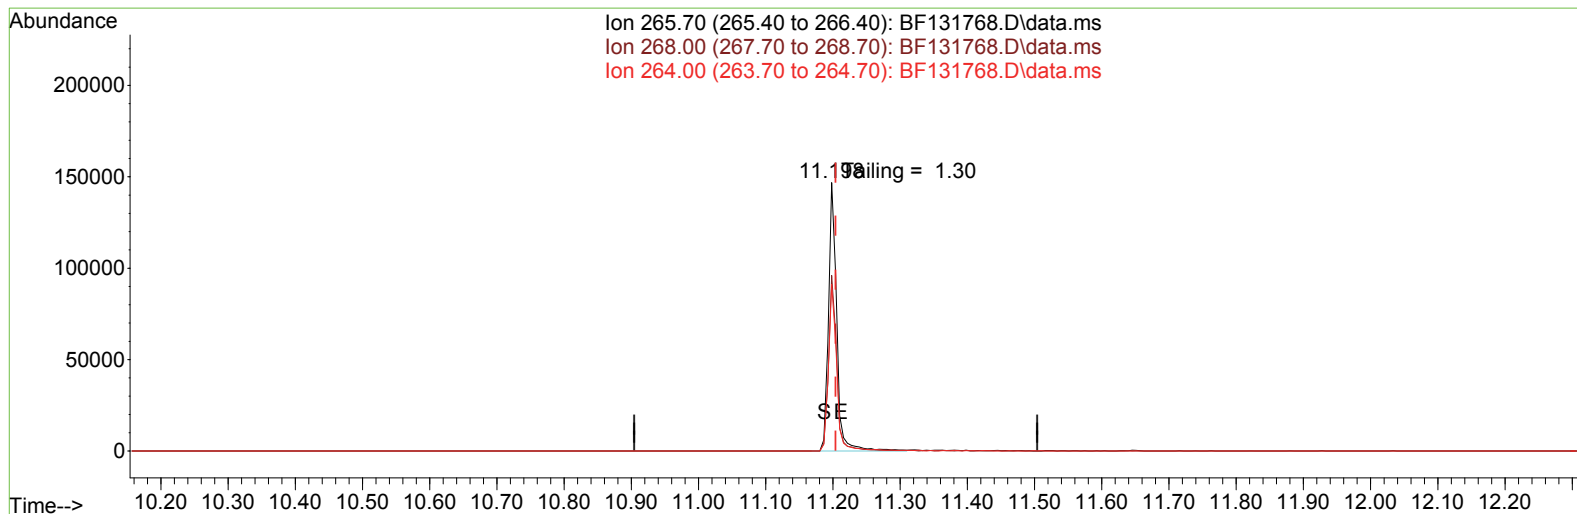

TIC: BF131768.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 31630.88 ng




response 126045

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.40
264.00	65.00	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131768.D
Acq On : 22 Dec 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 23 05:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

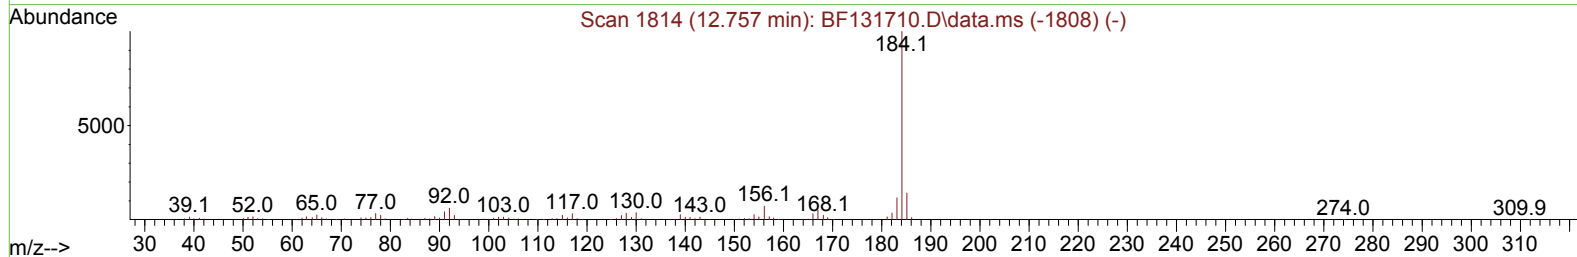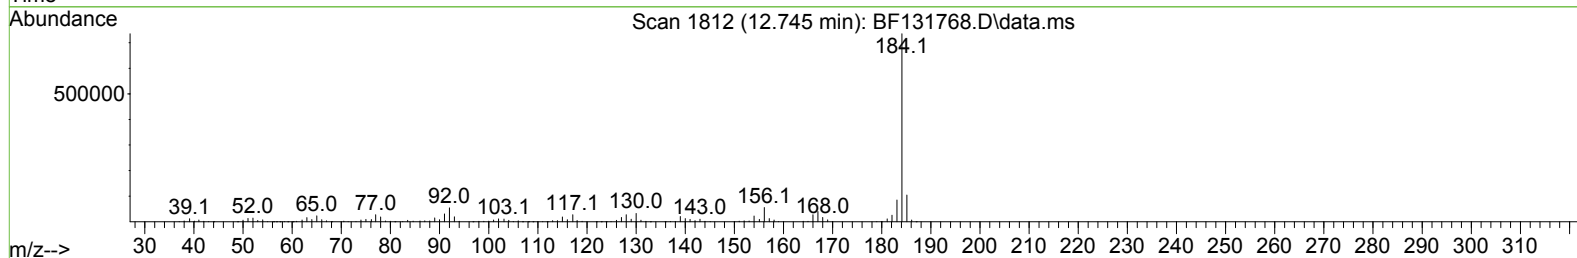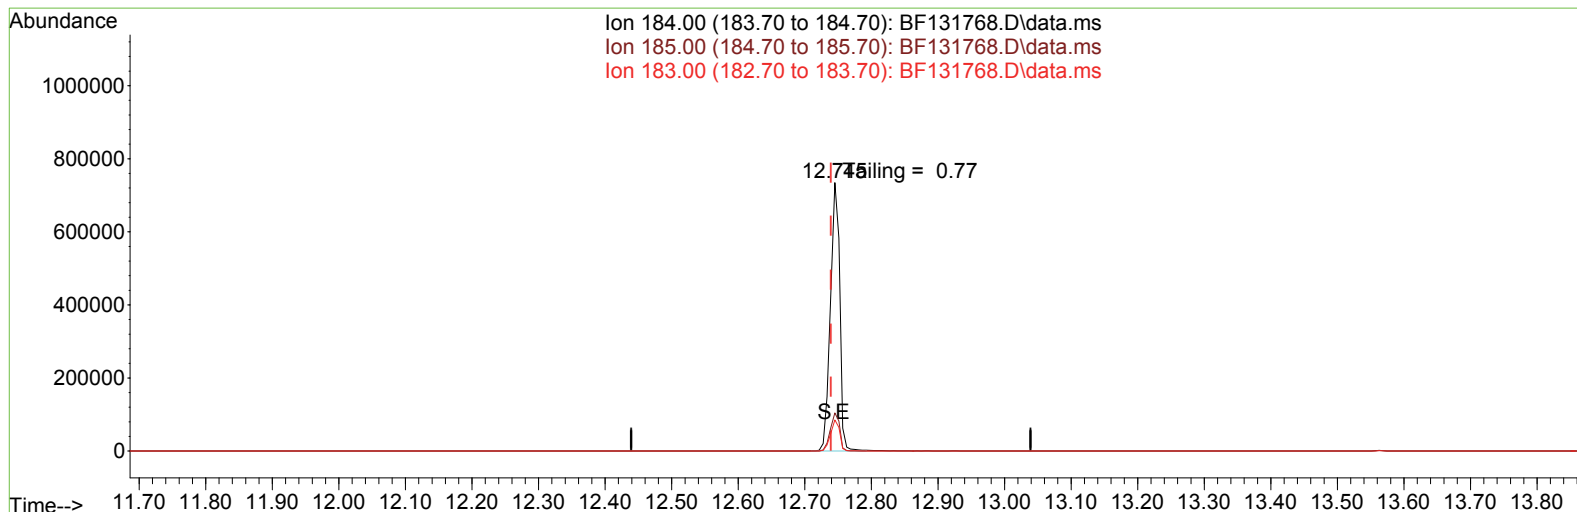

TIC: BF131768.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng

response 720501

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.60	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2022	BNA_F	<u>BF131768.D</u>
Compound Name	Response	Retention Time
DDT	339841	13.563
DDD	5529	13.263
DDE	200	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5729	345570	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP