


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
 Data File : BF131778.D
 Acq On : 22 Dec 2022 15:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 24 00:05:44 2022

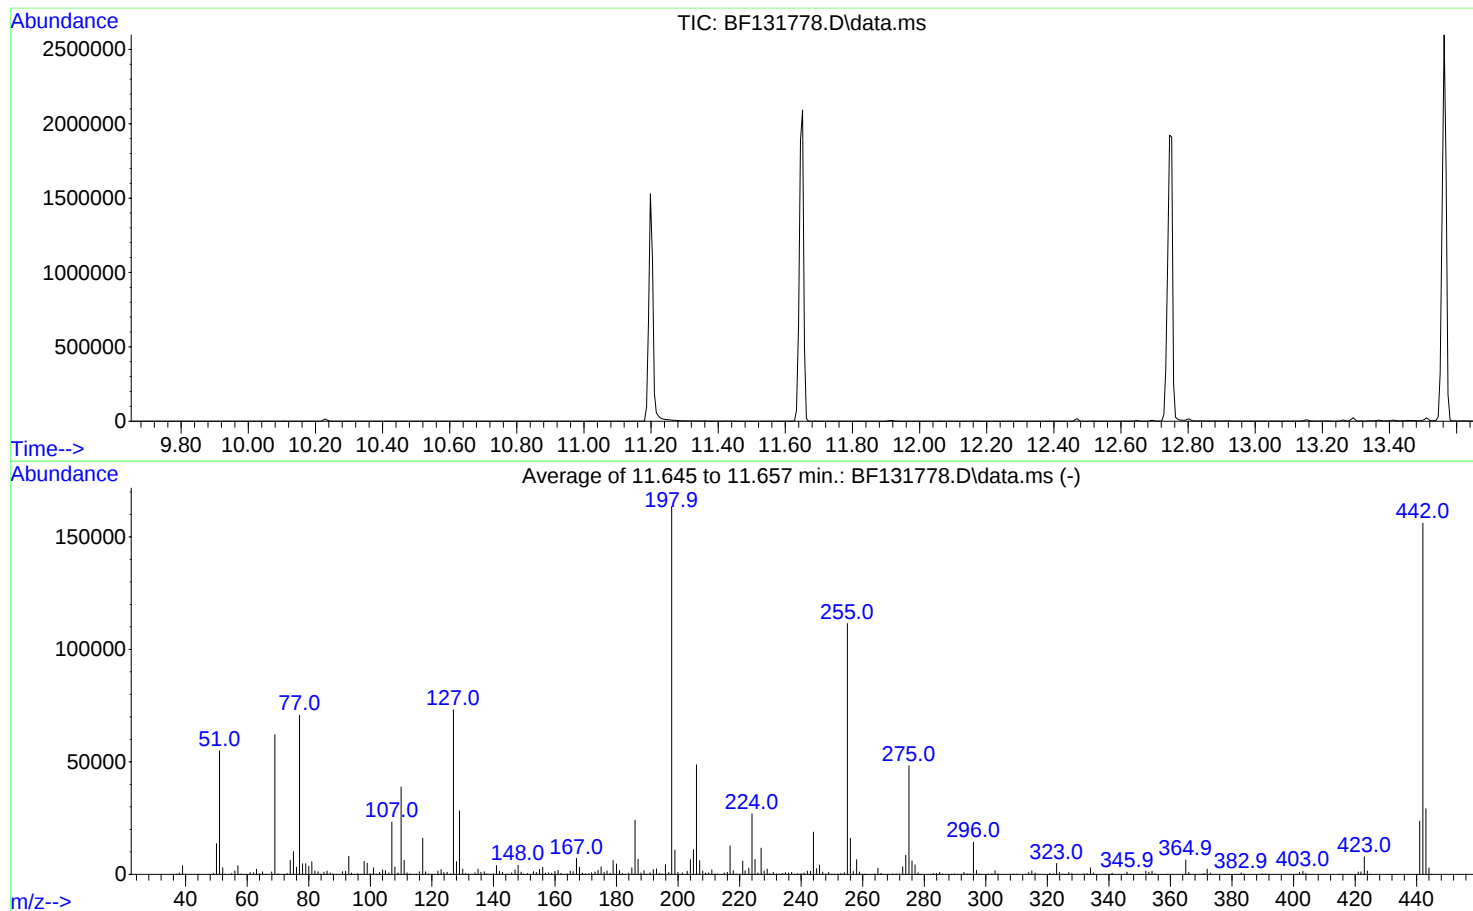




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	54953	PASS
68	69	0.00	2	1.7	1057	PASS
69	198	0.00	100	37.9	61997	PASS
70	69	0.00	2	0.5	323	PASS
127	198	10	80	44.8	73196	PASS
197	198	0.00	2	0.5	887	PASS
198	198	100	100	100.0	163504	PASS
199	198	5	9	6.6	10821	PASS
275	198	10	60	29.5	48216	PASS
365	198	1	100	3.9	6374	PASS
441	198	0.01	100	14.4	23599	PASS
442	442	50	100	100.0	156080	PASS
443	442	15	24	18.7	29171	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131778.D
Acq On : 22 Dec 2022 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 23 05:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

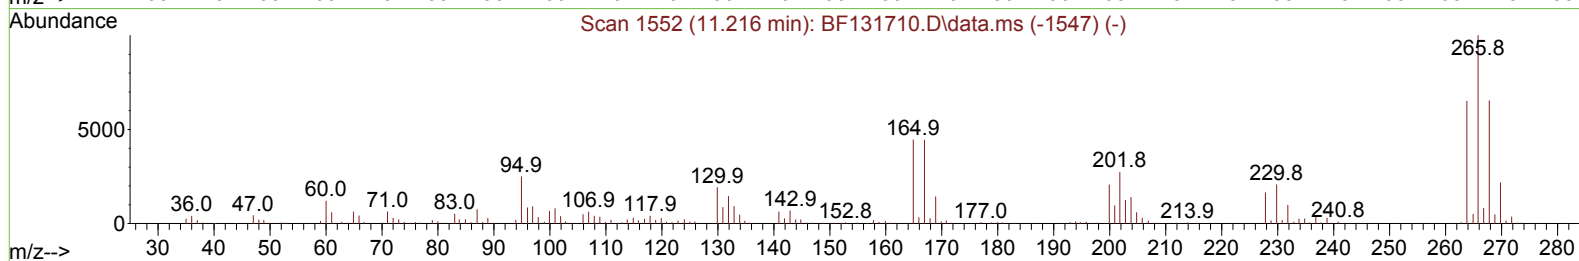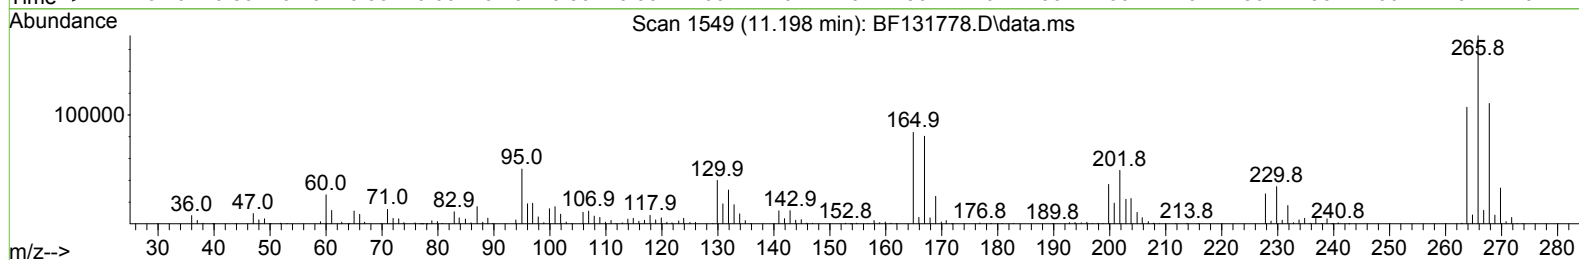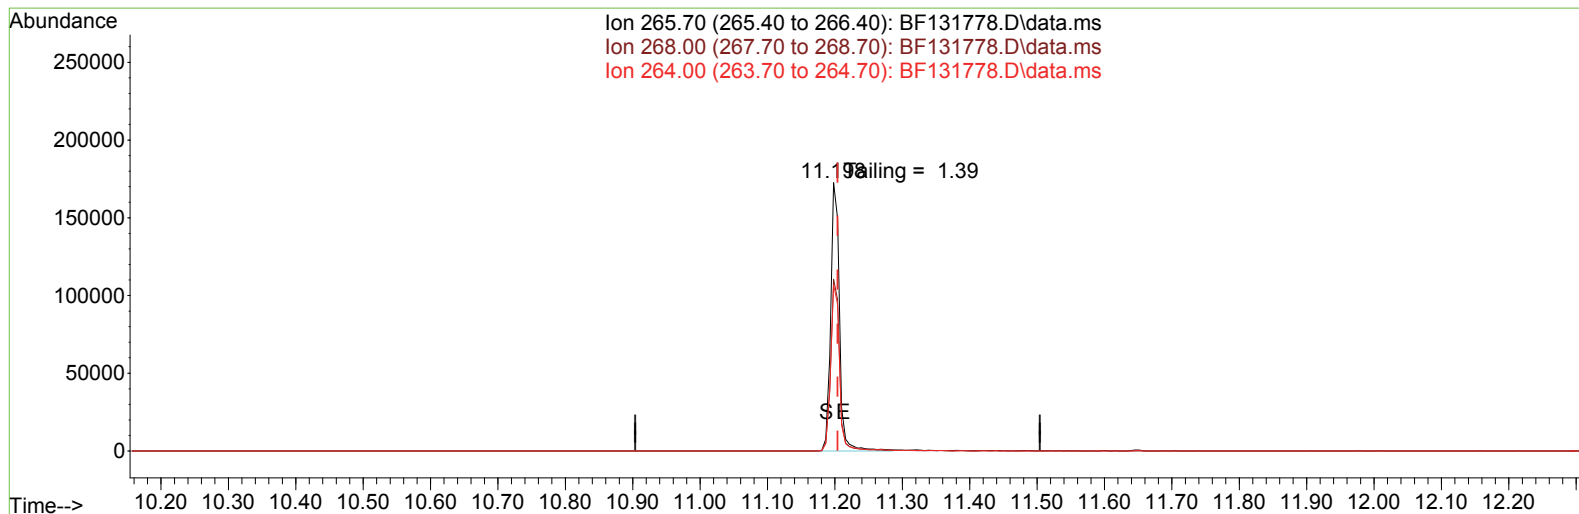

TIC: BF131778.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 27000.22 ng




response 158038

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.02
264.00	65.00	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131778.D
Acq On : 22 Dec 2022 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 23 05:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

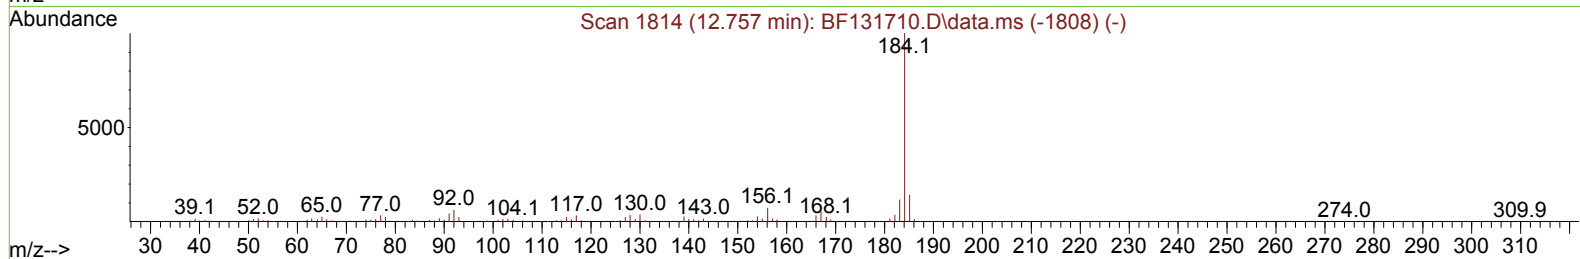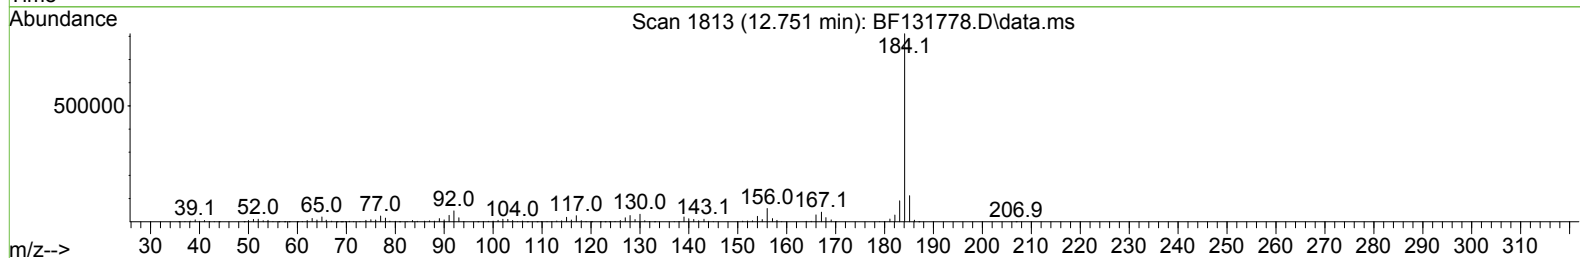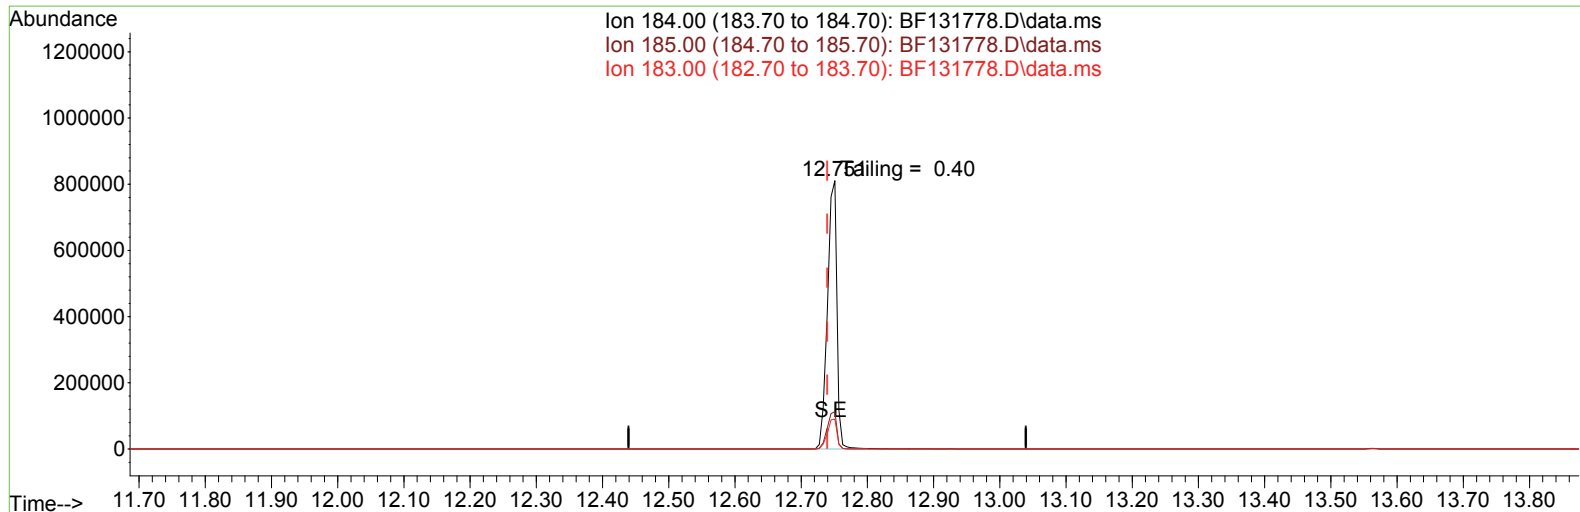

TIC: BF131778.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 0.00 ng

response 805819

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.90
183.00	11.60	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2022	BNA_F	<u>BF131778.D</u>
Compound Name	Response	Retention Time
DDT	435043	13.563
DDD	5332	13.292
DDE	181	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5513	440556	1.25

Instrument :
BNA_F
ClientSampleId :
DFTPP