
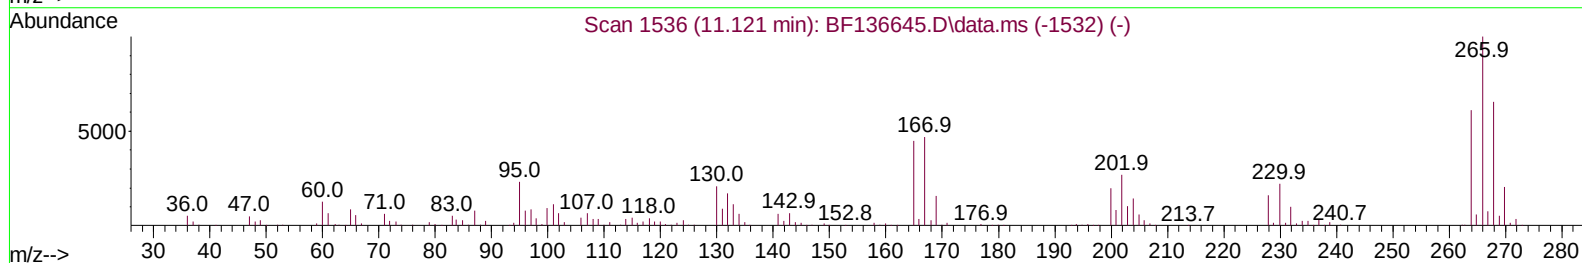
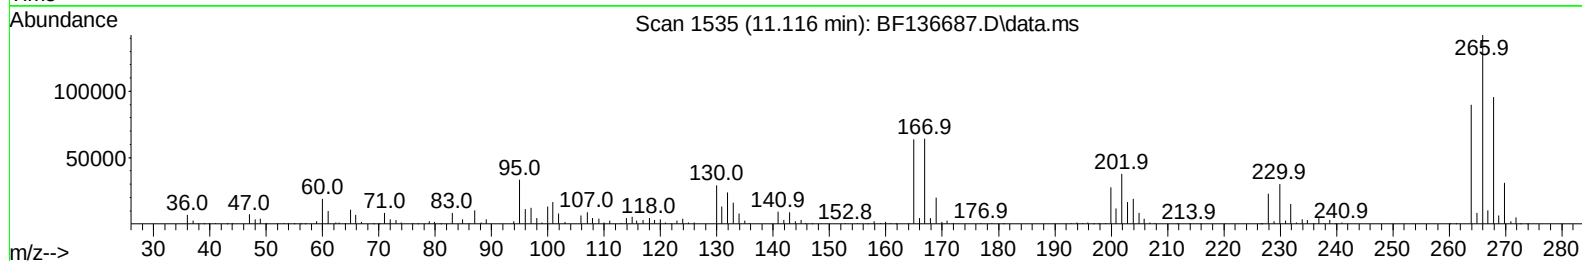


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136687.D
Acq On : 22 Dec 2023 15:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 01:02:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

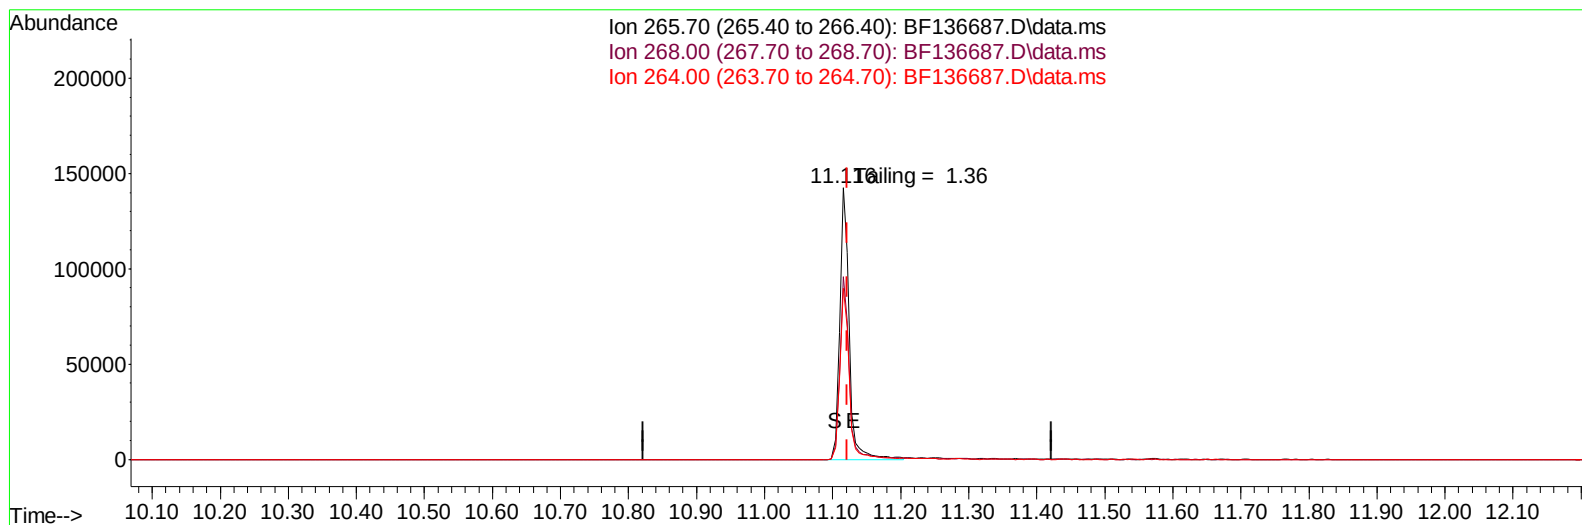




TIC: BF136687.D\data.ms

(70) Pentachlorophenol (C)**11.116min (-0.006) 36116.37 ng****response 136884**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.22
264.00	61.20	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136687.D
Acq On : 22 Dec 2023 15:57
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 01:02:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

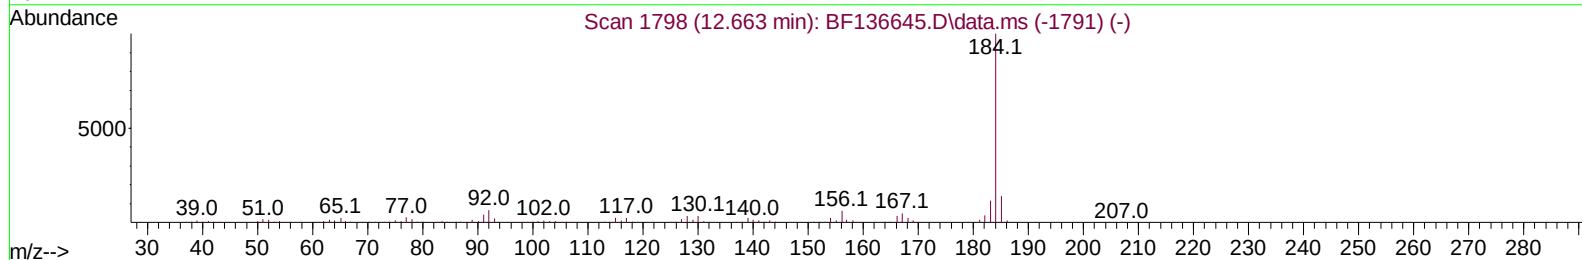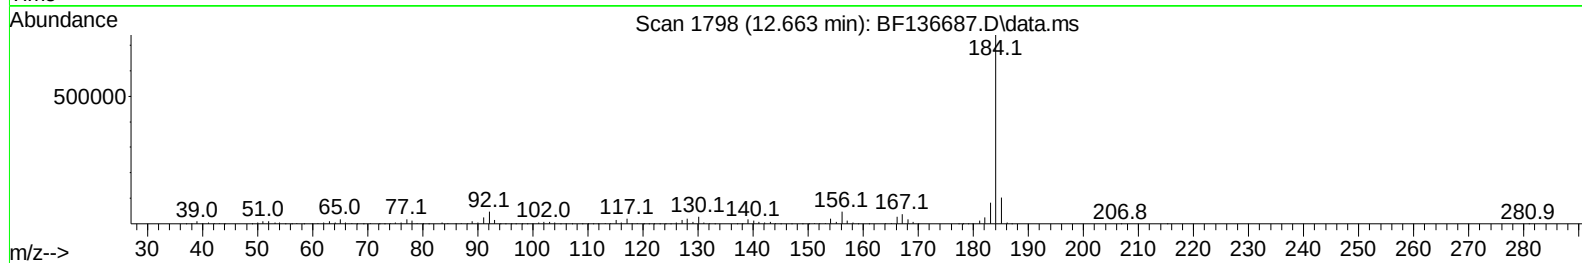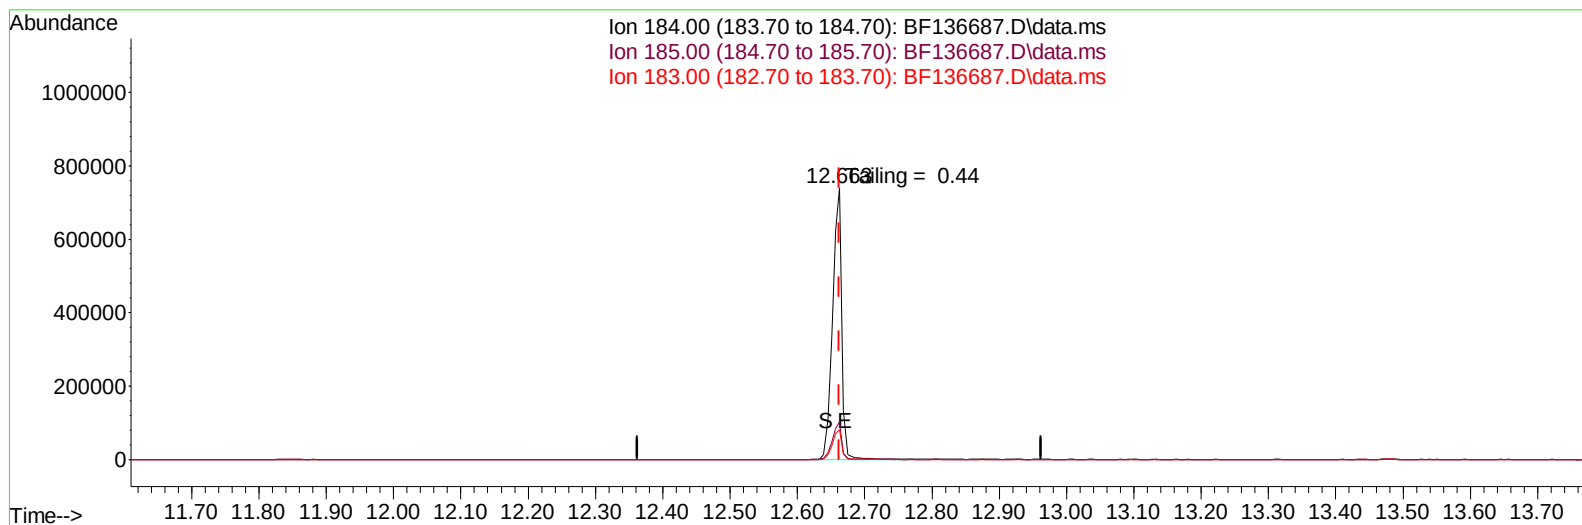

TIC: BF136687.D\data.ms

(77) Benzidine**12.663min (+ 0.000) 0.00 ng****response 708927**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.89
183.00	11.60	11.08
0.00	0.00	0.00