

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
 Data File : BF136678.D
 Acq On : 22 Dec 2023 10:34
 Operator : CG\JU
 Sample : PB157642BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157642BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	496	503	511	rBV	38385	52027	1.85%	0.326%
2	5.434	564	569	572	rBV	2137739	2043334	72.83%	12.817%
3	6.428	733	738	741	rBV	1818772	2104515	75.01%	13.201%
4	6.781	795	798	802	rBV	512841	431848	15.39%	2.709%
5	7.345	888	894	897	rBV	1306758	1364619	48.64%	8.560%
6	8.057	1010	1015	1019	rBV	639291	577712	20.59%	3.624%
7	9.139	1193	1199	1202	rBV	2815381	2601344	92.72%	16.318%
8	9.816	1309	1314	1317	rBV	819500	661845	23.59%	4.152%
9	10.610	1445	1449	1453	rBV	1565504	1525031	54.36%	9.566%
10	11.310	1564	1568	1571	rBV	817337	729979	26.02%	4.579%
11	12.910	1835	1840	1843	rBV	2929794	2805671	100.00%	17.599%
12	13.963	2014	2019	2027	rVB	601796	582693	20.77%	3.655%
13	15.439	2264	2270	2283	rVB	336984	461294	16.44%	2.894%




Sum of corrected areas: 15941912

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136678.D
Acq On : 22 Dec 2023 10:34
Operator : CG\JU
Sample : PB157642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157642BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

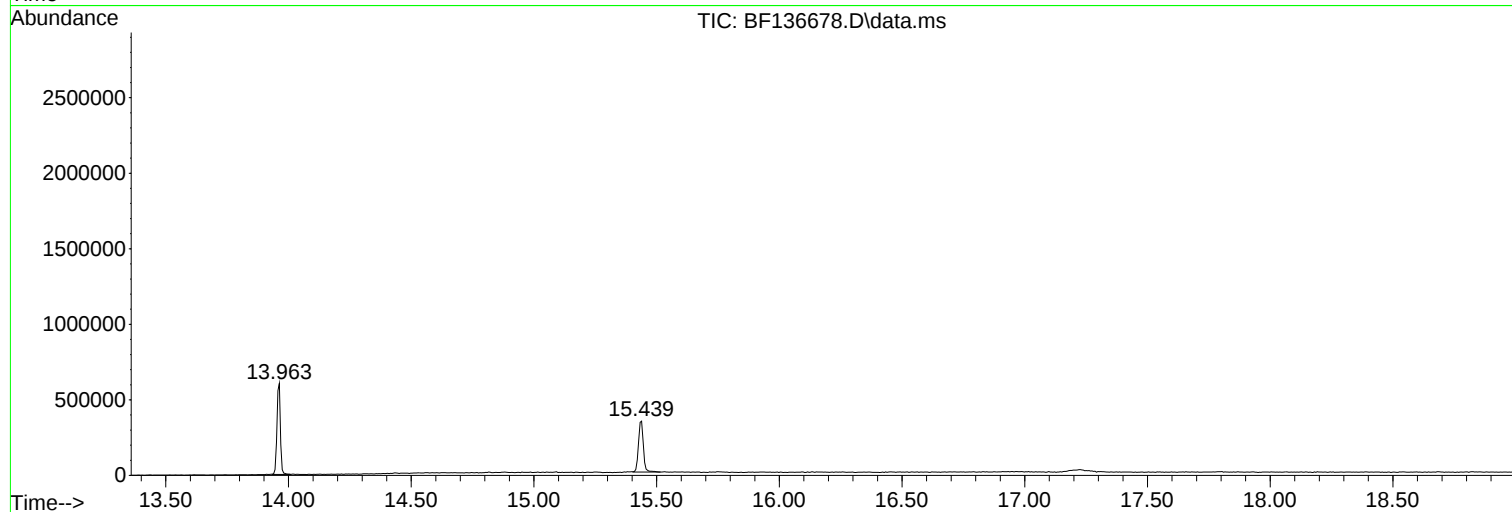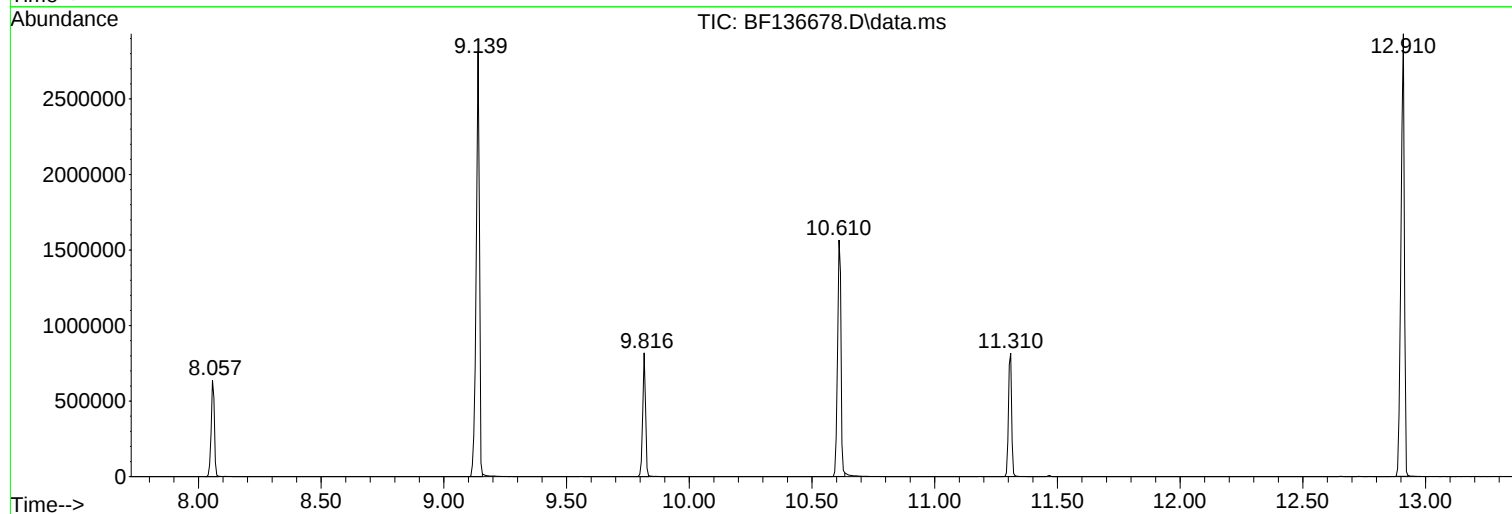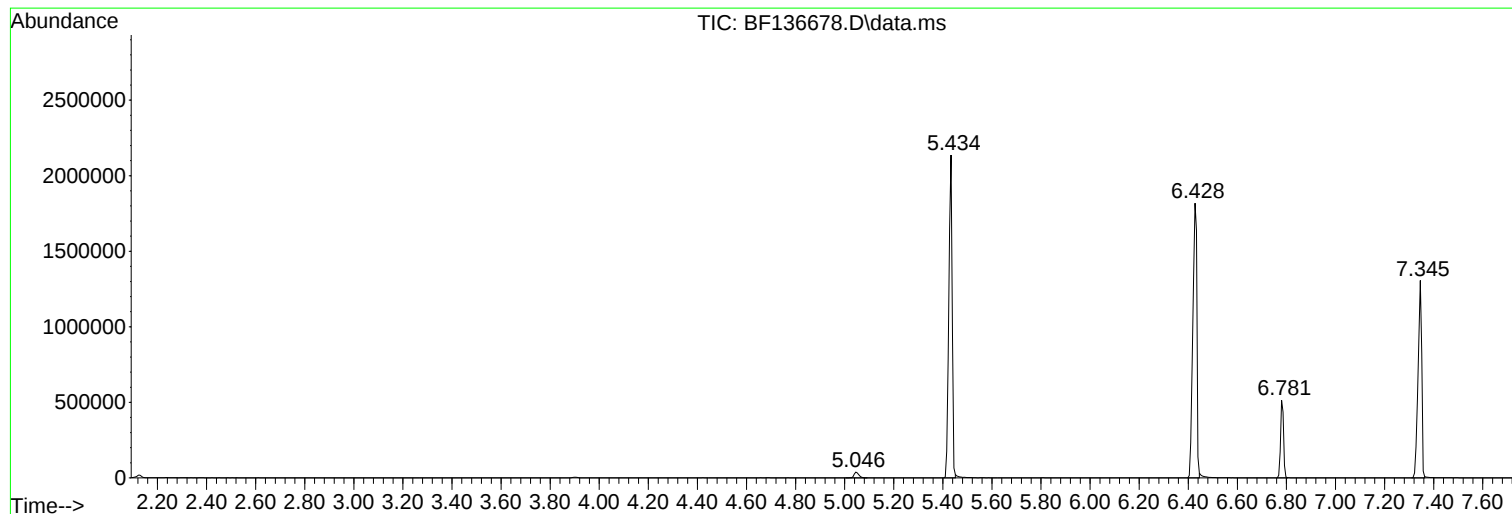

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136678.D
Acq On : 22 Dec 2023 10:34
Operator : CG\JU
Sample : PB157642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB157642BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.046	2.41 ng	52027	1,4-Dichlorobenzene-d4			6.781
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	59
2	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
3	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9
4	Butane, 1-ethoxy-		102	C6H14O	000628-81-9	9
5	4-Penten-2-one, 4-methyl-		98	C6H10O	003744-02-3	9

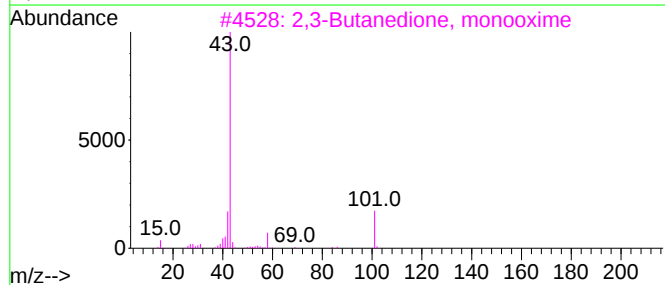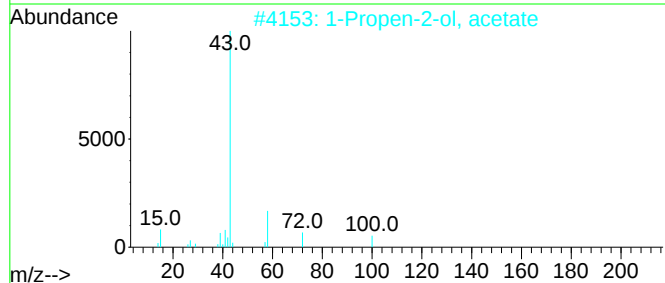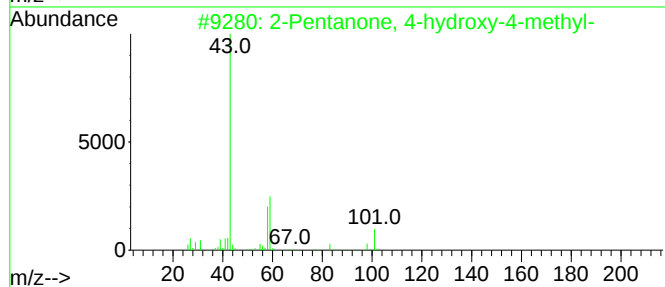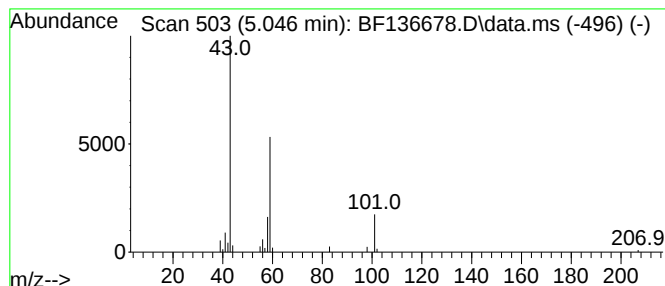

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136678.D
Acq On : 22 Dec 2023 10:34
Operator : CG\JU
Sample : PB157642BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157642BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.046	2.4	ng	52027	1	6.781	431848	20.0