
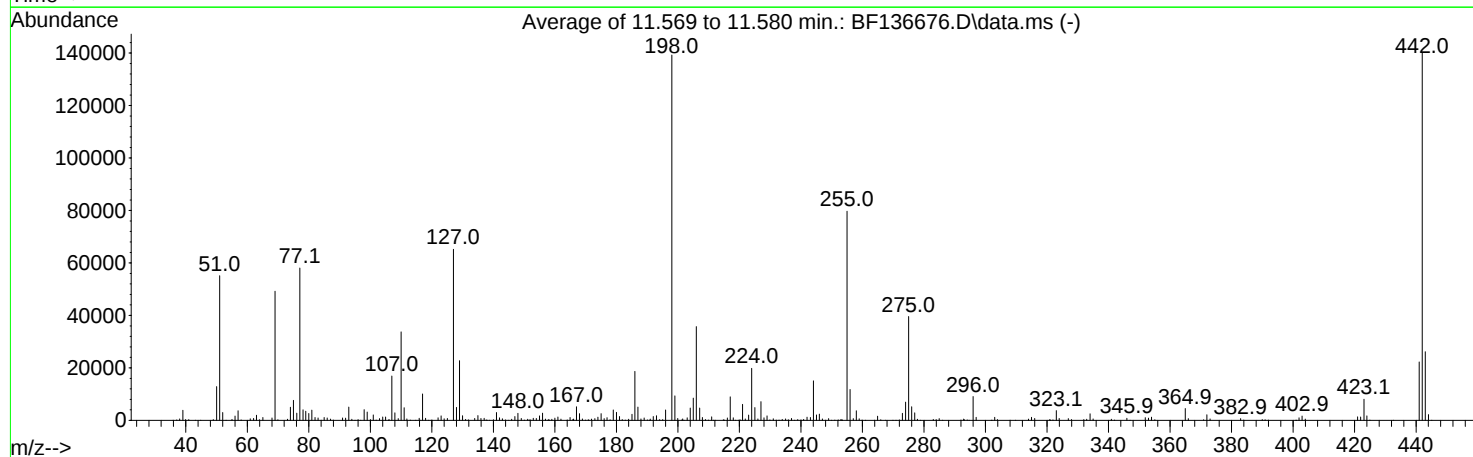


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136676.D
Acq On : 22 Dec 2023 08:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

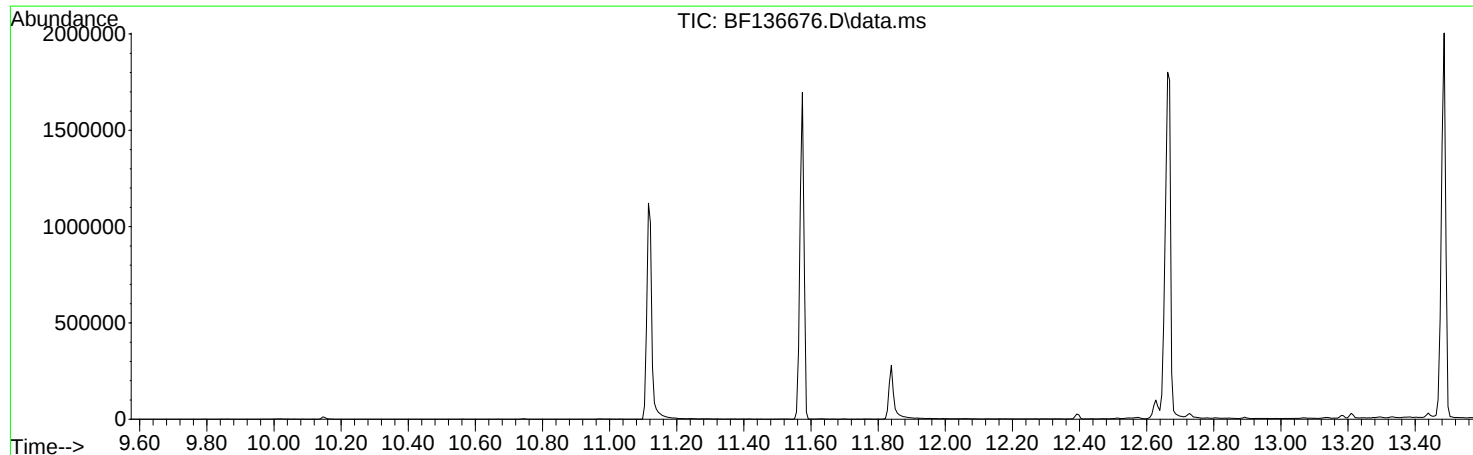




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	55128	PASS
68	69	0.00	2	1.9	922	PASS
69	198	0.00	100	35.4	49235	PASS
70	69	0.00	2	0.5	223	PASS
127	198	10	80	46.8	65195	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139208	PASS
199	198	5	9	6.7	9349	PASS
275	198	10	60	28.4	39603	PASS
365	198	1	100	3.2	4513	PASS
441	198	0.01	100	16.0	22238	PASS
442	442	50	100	100.0	140205	PASS
443	442	15	24	18.7	26175	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136676.D
Acq On : 22 Dec 2023 08:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 11:08:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

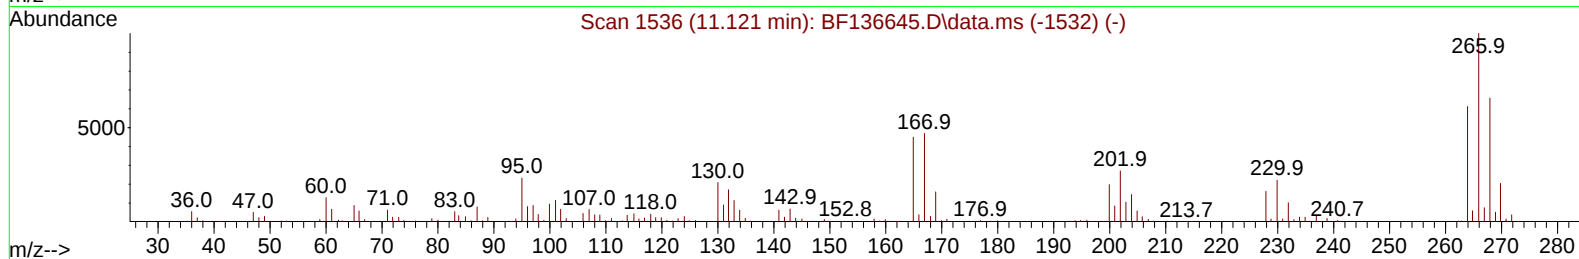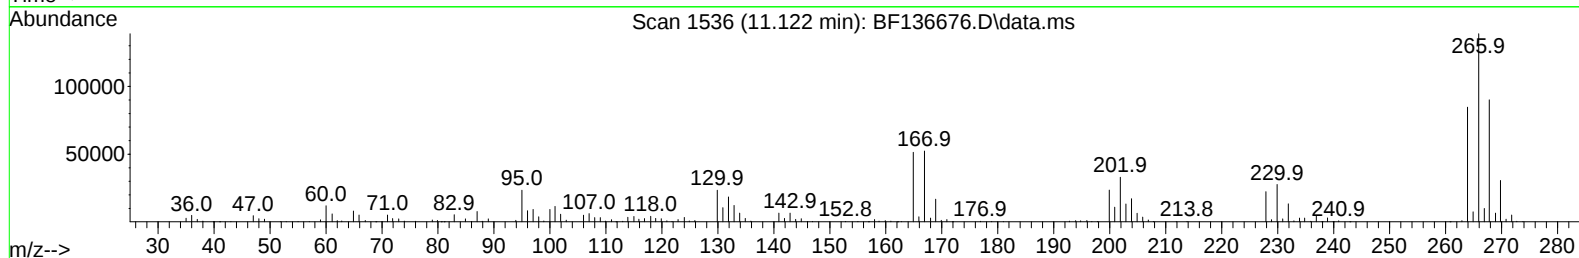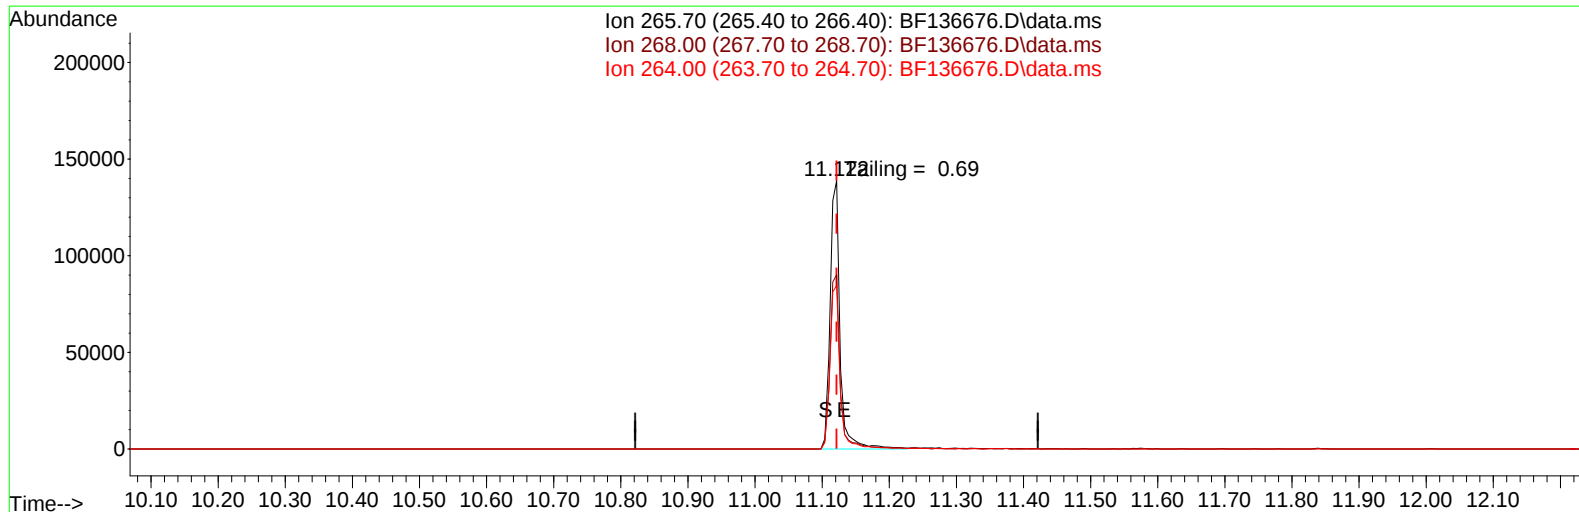

TIC: BF136676.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 195113.88 ng




response 142947

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	64.91
264.00	61.20	60.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136676.D
Acq On : 22 Dec 2023 08:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 11:08:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

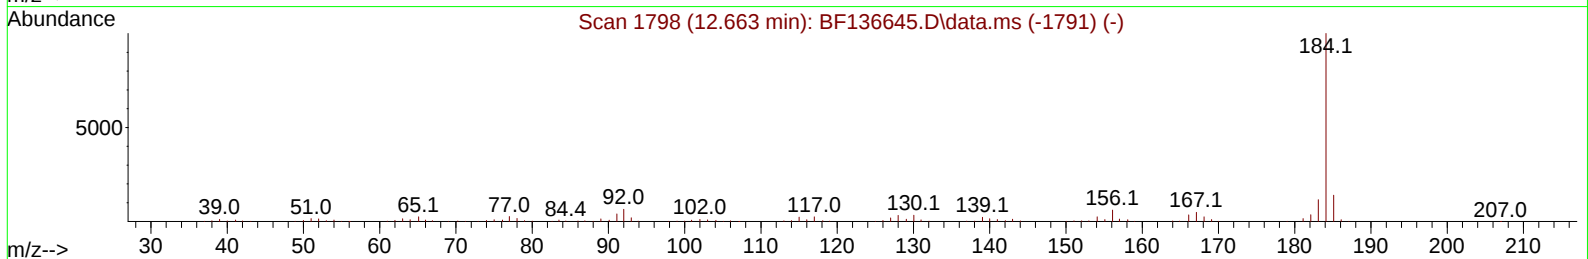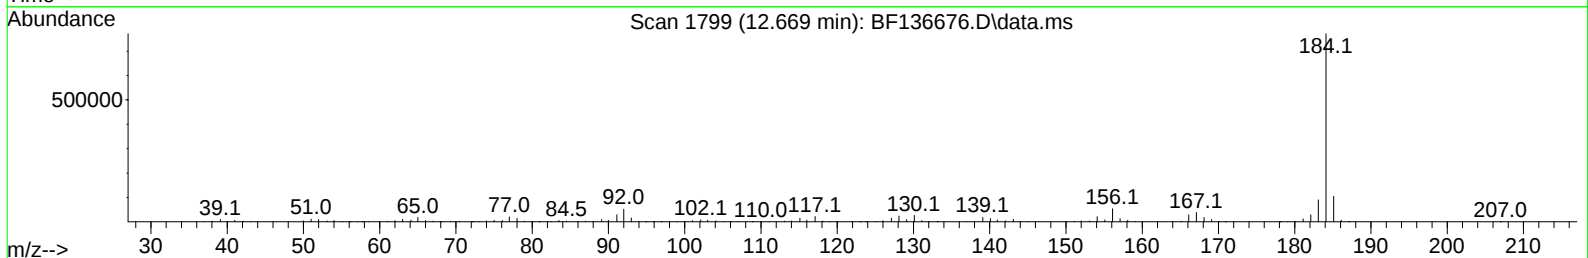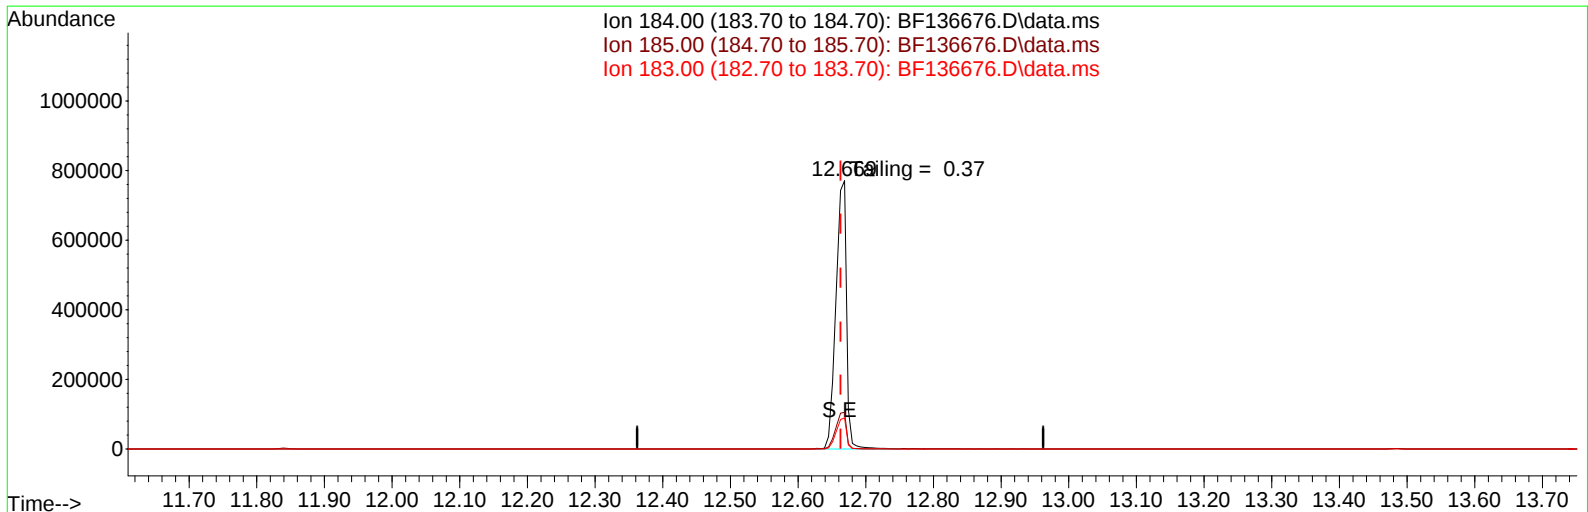

TIC: BF136676.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 40964.46 ng

response 841883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.67
183.00	11.60	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2023	BNA_F	<u>BF136676.D</u>
Compound Name	Response	Retention Time
DDT	363591	13.486
DDD	7063	13.21
DDE	446	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7509	371100	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP