


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
Data File : BF136687.D
Acq On : 22 Dec 2023 15:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

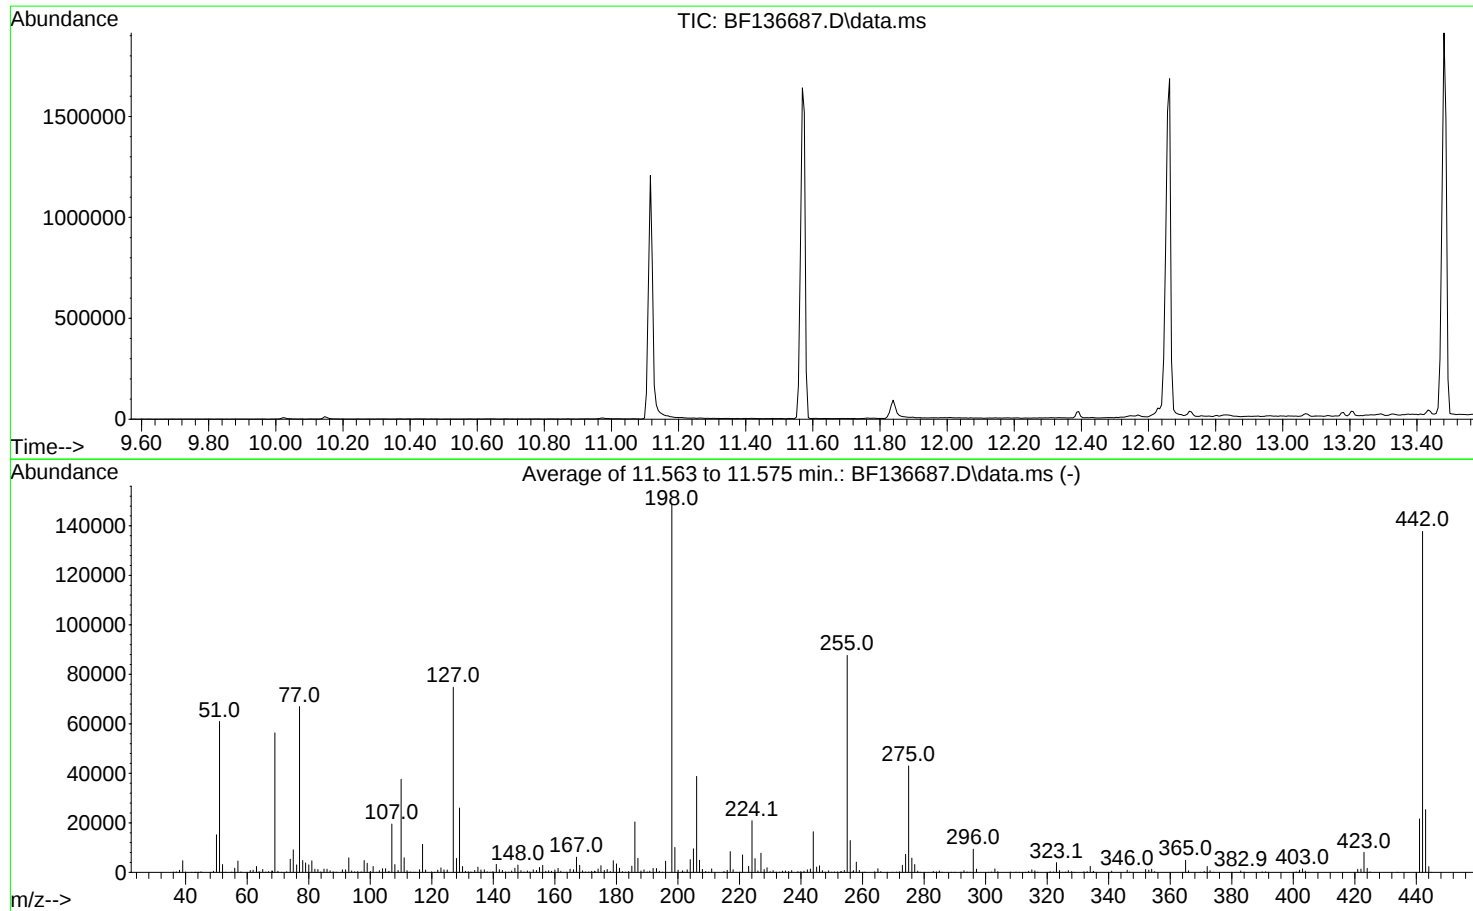




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	60944	PASS
68	69	0.00	2	1.1	595	PASS
69	198	0.00	100	37.9	56368	PASS
70	69	0.00	2	0.8	445	PASS
127	198	10	80	50.3	74813	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148619	PASS
199	198	5	9	6.8	10085	PASS
275	198	10	60	28.9	43000	PASS
365	198	1	100	3.3	4897	PASS
441	198	0.01	100	14.5	21624	PASS
442	442	50	100	100.0	137787	PASS
443	442	15	24	18.4	25344	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
 Data File : BF136687.D
 Acq On : 22 Dec 2023 15:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 23 01:02:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

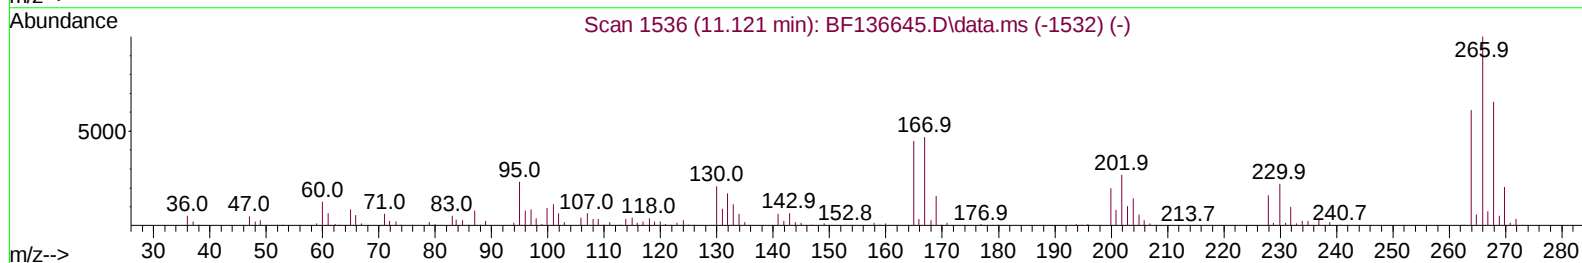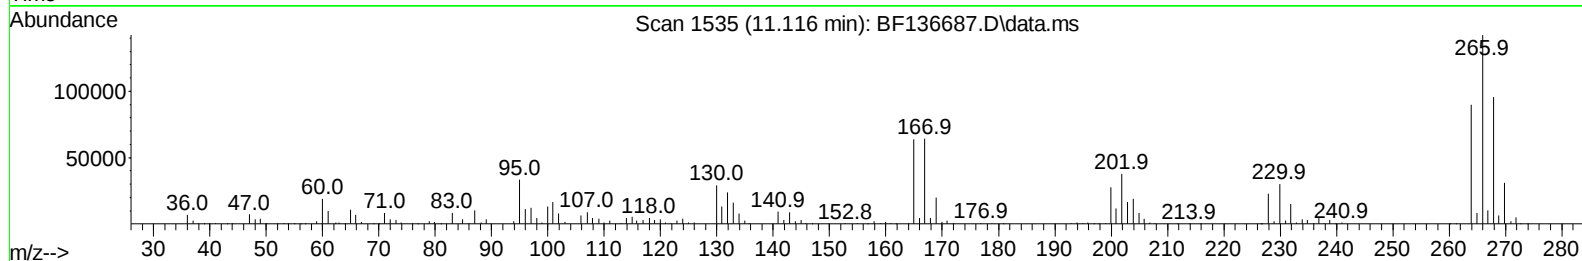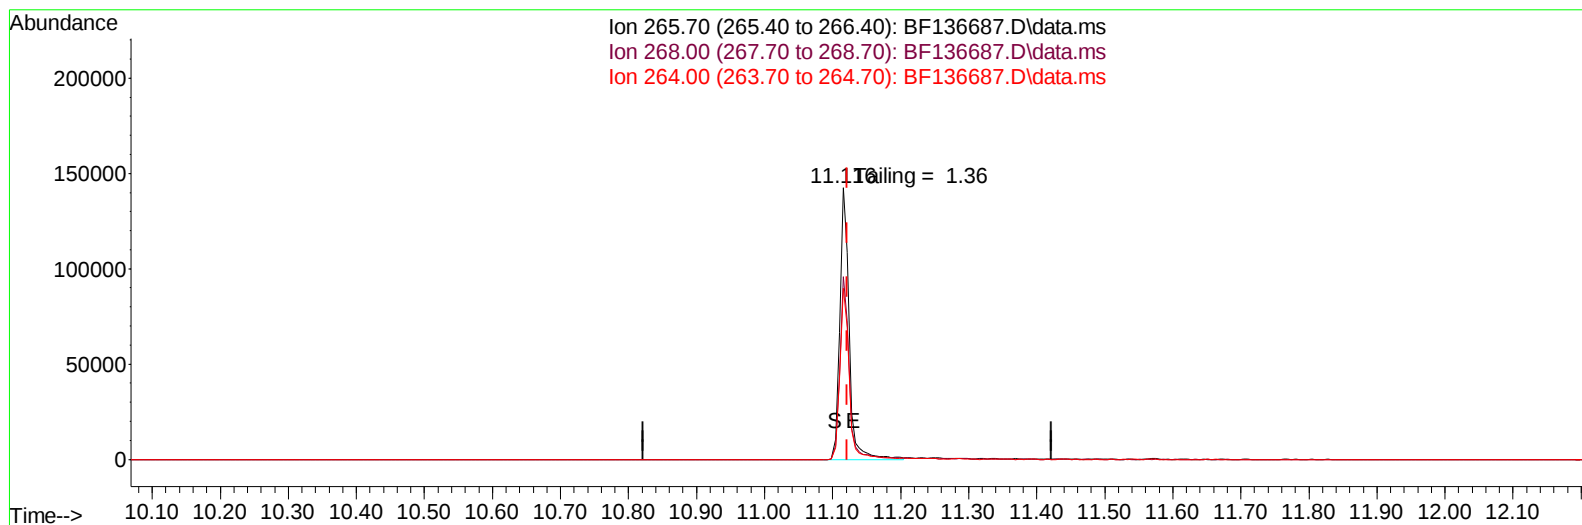

TIC: BF136687.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 36116.37 ng




response 136884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.22
264.00	61.20	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122223\
 Data File : BF136687.D
 Acq On : 22 Dec 2023 15:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 23 01:02:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

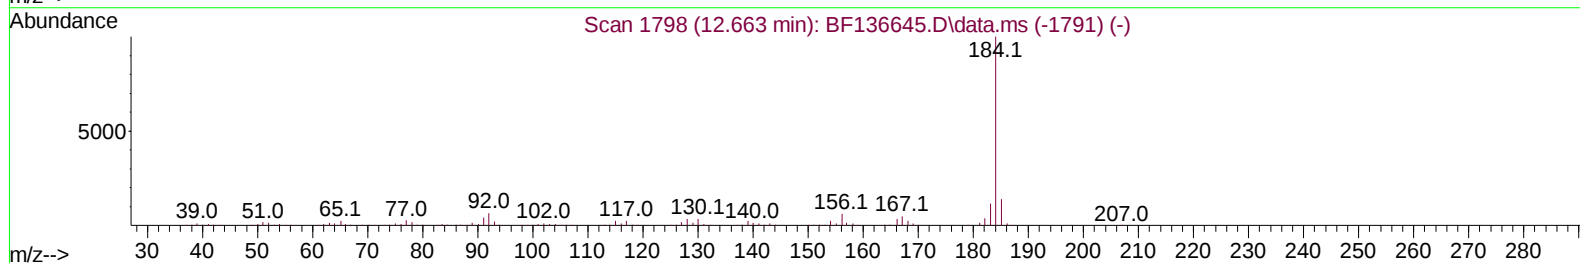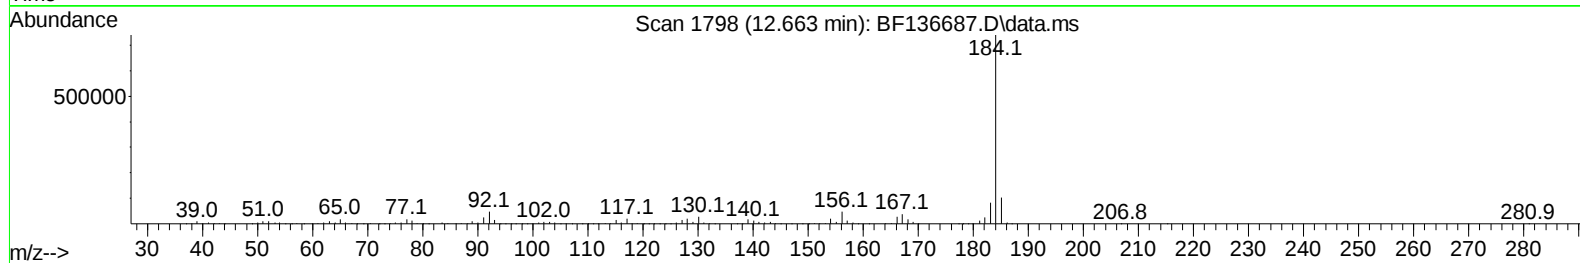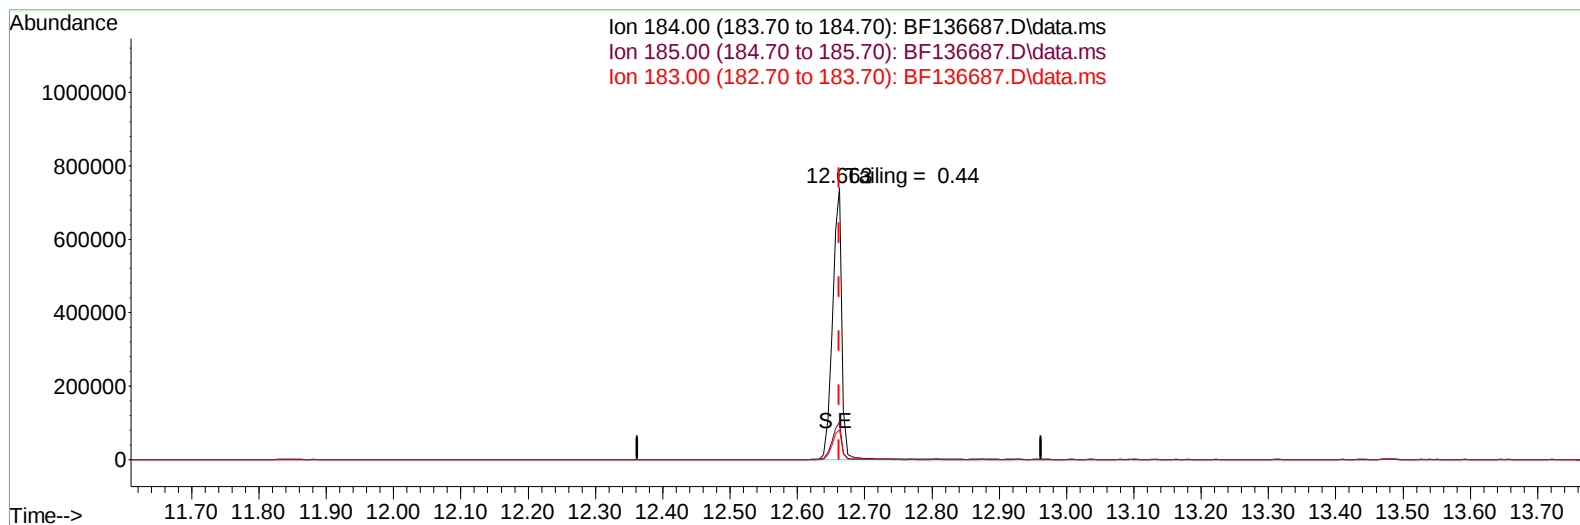

TIC: BF136687.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 0.00 ng

response 708927

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.89
183.00	11.60	11.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2023	BNA_F	<u>BF136687.D</u>
Compound Name	Response	Retention Time
DDT	355038	13.48
DDD	7529	13.21
DDE	809	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8338	363376	2.29

Instrument :
BNA_F
ClientSampleId :
DFTPP