


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122315\
 Data File : BF084061.D
 Acq On : 24 Dec 2015 4:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 22 18:54:09 2015

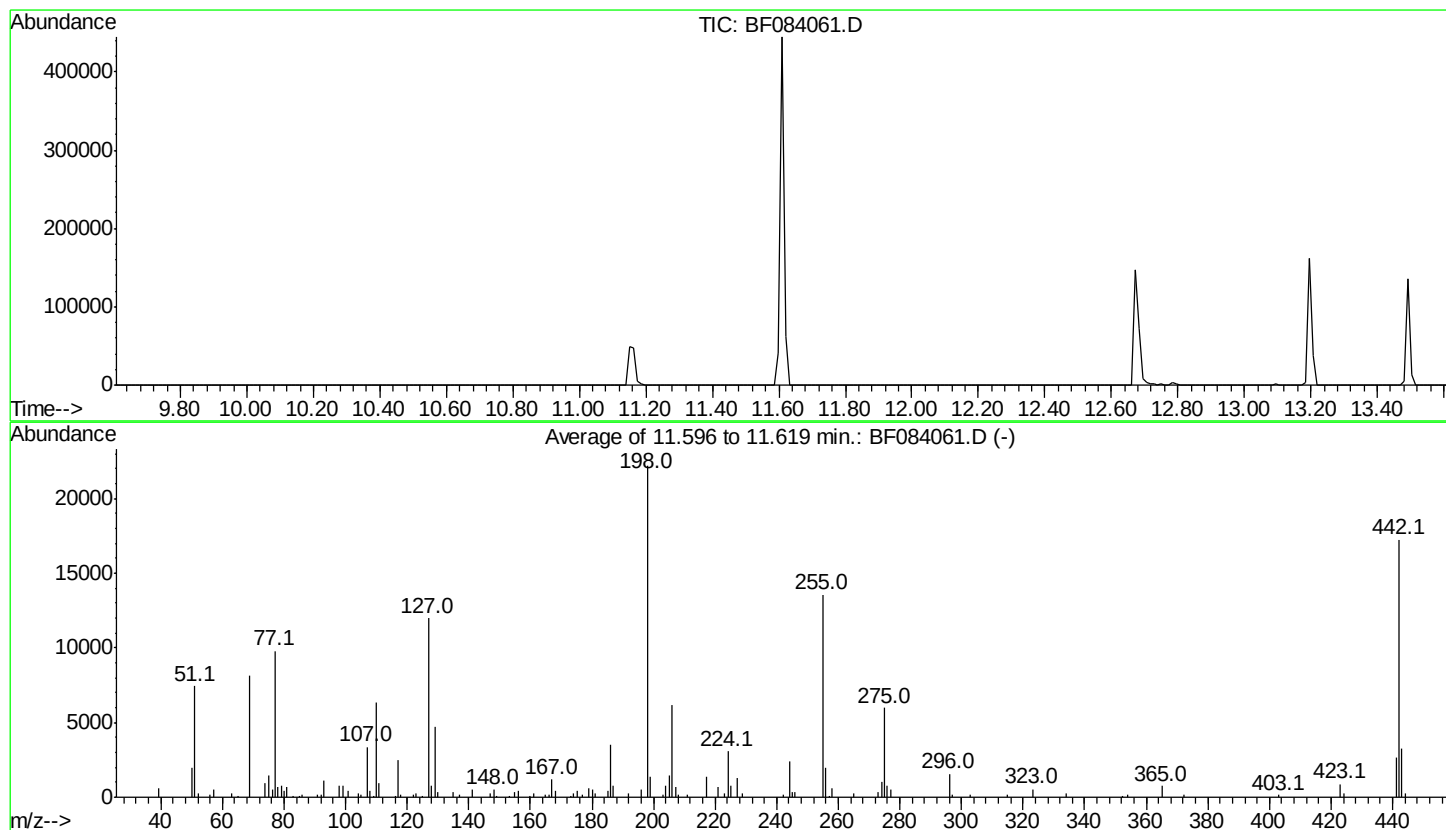

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	7423	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.7	8143	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.0	11992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22206	PASS
199	198	5	9	6.2	1366	PASS
275	198	10	60	26.9	5970	PASS
365	198	1	100	3.3	736	PASS
441	442	0.01	24	15.3	2638	PASS
442	198	50	100	77.7	17261	PASS
443	442	15	24	19.1	3294	PASS