

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122316\
 Data File : BF091921.D
 Acq On : 23 Dec 2016 14:08
 Operator : UM/SJ
 Sample : H6156-24DL 50X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-201612DL

Quant Time: Dec 23 17:06:19 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 17:02:35 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	264436	20.00	ng	-0.01
21) Naphthalene-d8	8.03	136	898276	20.00	ng	-0.01
38) Acenaphthene-d10	9.78	164	495614	20.00	ng	-0.01
63) Phenanthrene-d10	11.25	188	770885	20.00	ng	-0.01
75) Chrysene-d12	13.88	240	609833	20.00	ng	-0.02
86) Perylene-d12	15.28	264	492438	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	16626	1.05	ng	0.03
7) Phenol-d6	6.43	99	16465	0.85	ng	0.02
23) Nitrobenzene-d5	7.30	82	36771	2.28	ng	-0.02
41) 2,4,6-Tribromophenol	10.57	330	13247	3.23	ng	-0.01
44) 2-Fluorobiphenyl	9.10	172	62788	2.43	ng	-0.01
78) Terphenyl-d14	12.84	244	52450	2.09	ng	-0.01
Target Compounds						
31) Naphthalene	8.05	128	1905878	46.36	ng	99
37) 2-Methylnaphthalene	8.74	142	92347	2.43	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122316\
Data File : BF091921.D
Acq On : 23 Dec 2016 14:08
Operator : UM/SJ
Sample : H6156-24DL 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-201612DL

Quant Time: Dec 23 17:06:19 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 17:02:35 2016
Response via : Initial Calibration

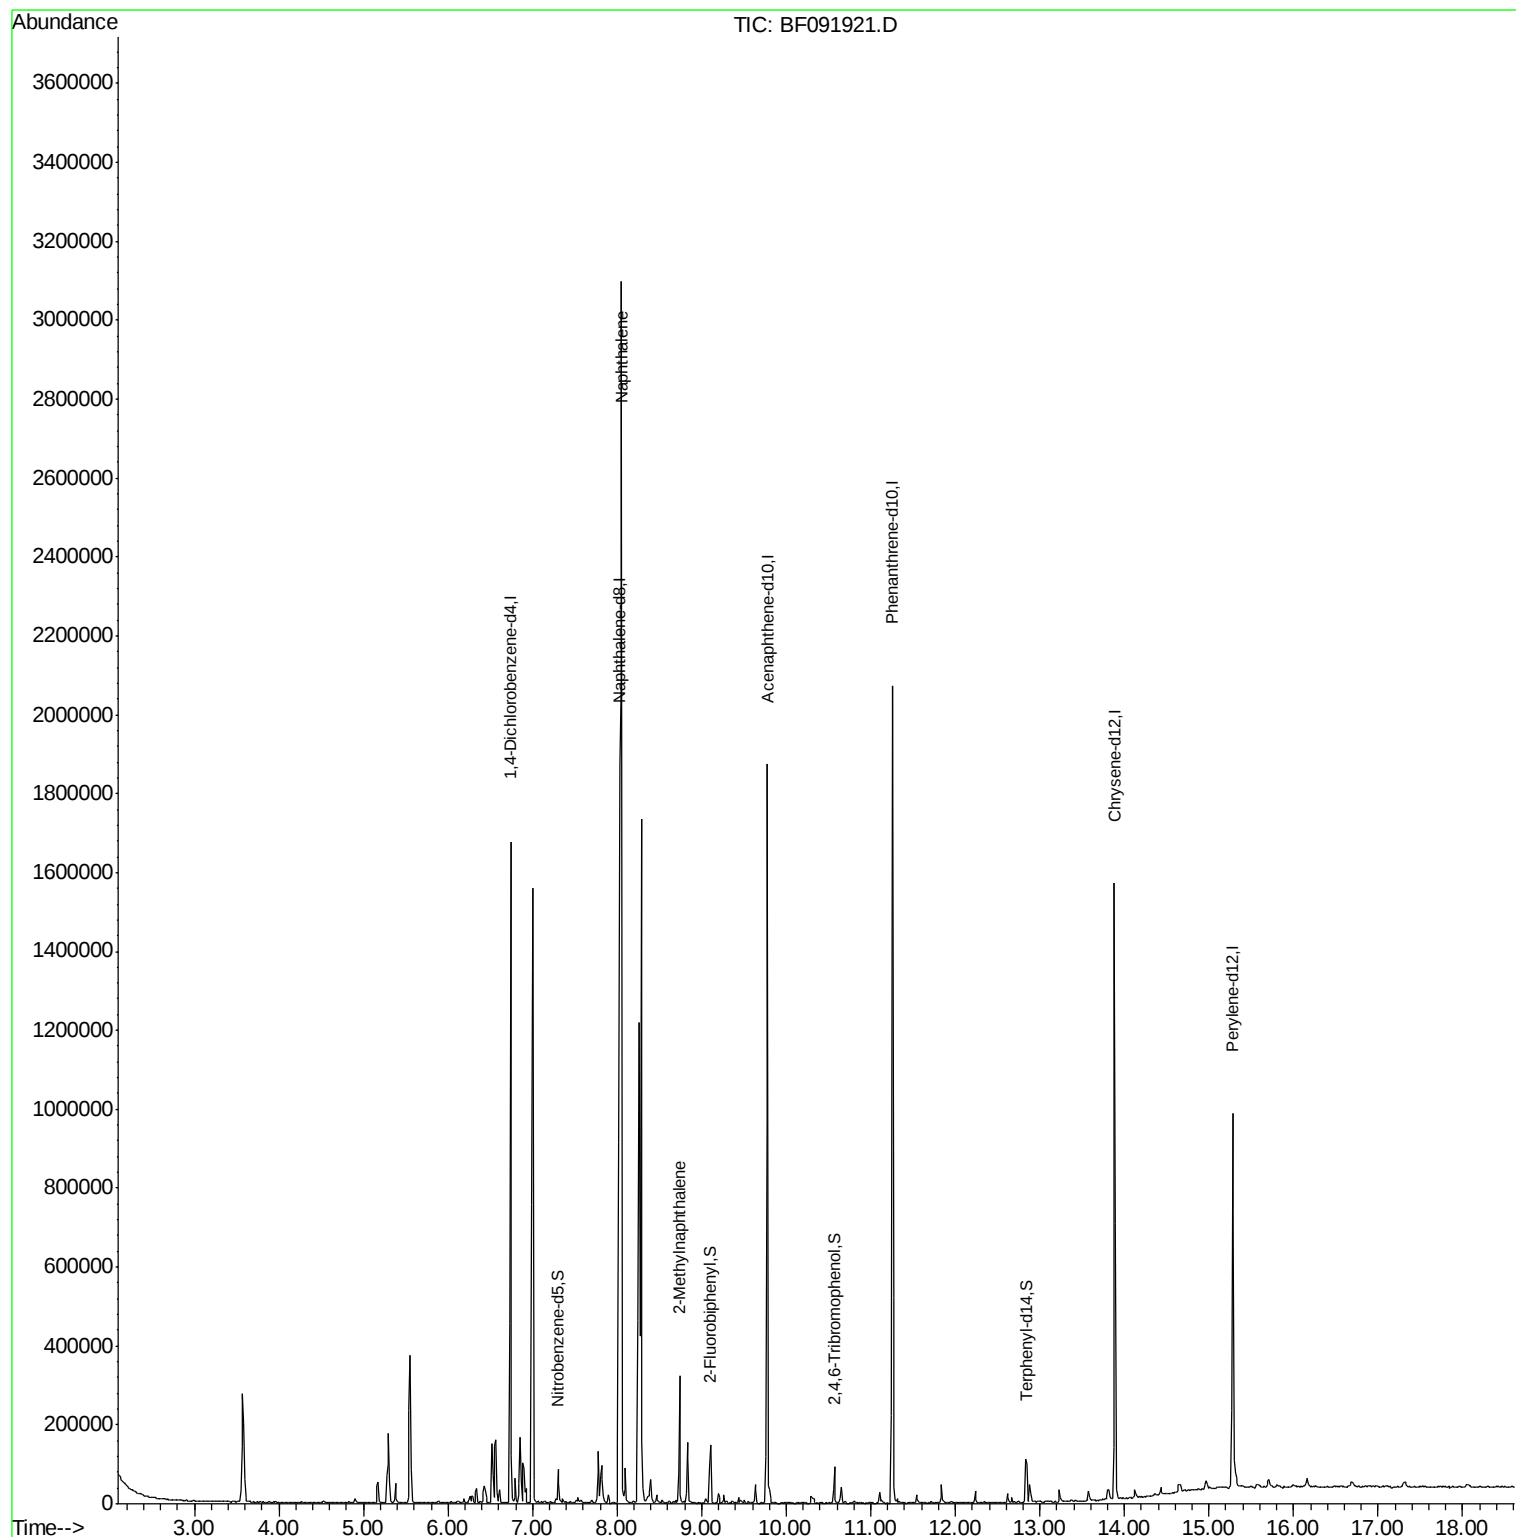



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 407

Delta R.T. -0.01 min

Lab File: BF091921.D

Acq: 23 Dec 2016 14:08

Instrument :

BNA_F

ClientSampleId :

WC-201612DL


Tot Ion:152 Resp: 264436

Ion Ratio Lower Upper

152 100

150 153.3 124.9 187.3




115 59.4 46.0 69.0

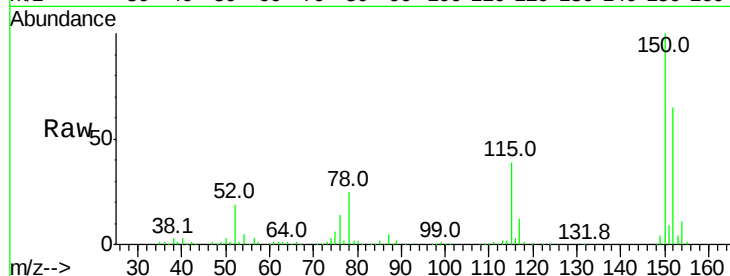

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

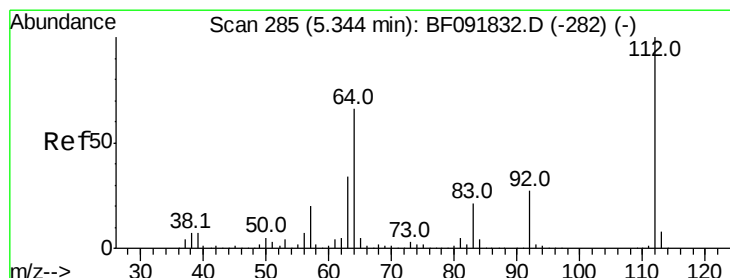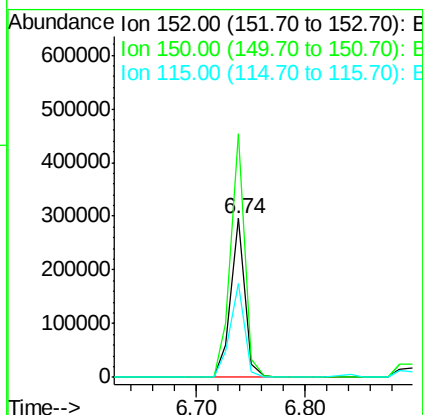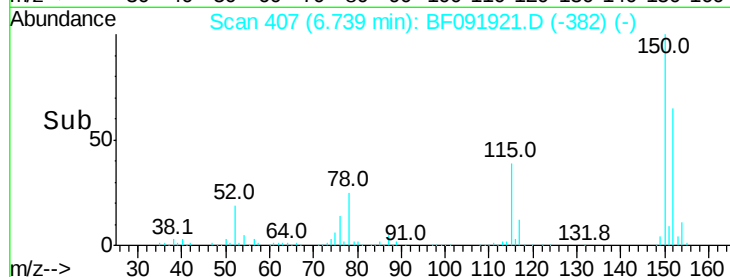

#5

2-Fluorophenol

Concen: 1.05 ng

RT: 5.38 min Scan# 288

Delta R.T. 0.03 min

Lab File: BF091921.D

Acq: 23 Dec 2016 14:08


Tgt Ion:112 Resp: 16626

Ion Ratio Lower Upper

112 100

64 56.4 46.1 69.1



63 30.2 23.8 35.6

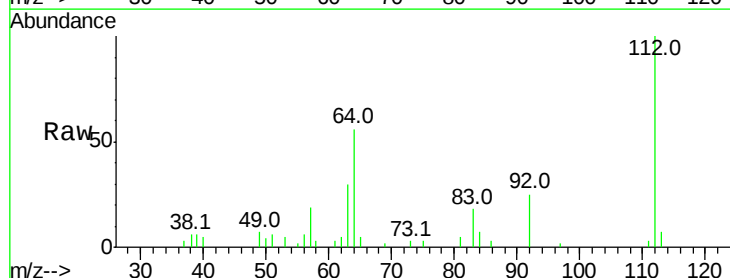


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

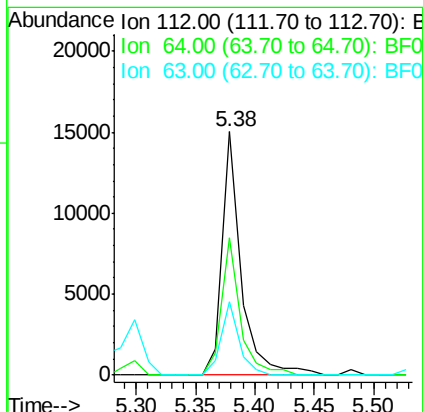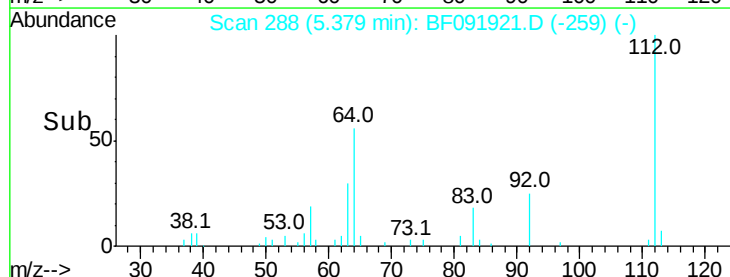

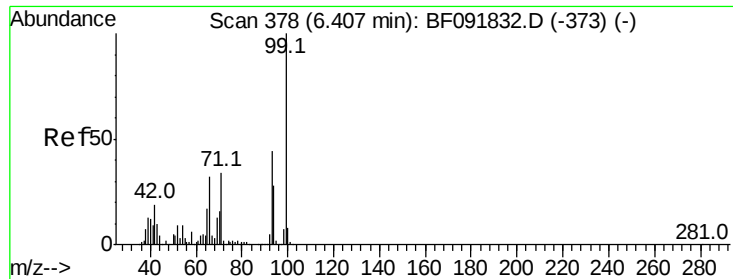

#7

Phenol-d6

Concen: 0.85 ng

RT: 6.43 min Scan# 380

Delta R.T. 0.02 min

Lab File: BF091921.D

Acq: 23 Dec 2016 14:08

Instrument :

BNA_F

ClientSampleId :

WC-201612DL


Tot Ion: 99 Resp: 16465

Ion Ratio Lower Upper

99 100

42 19.5 15.6 23.4




71 30.6 27.5 41.3

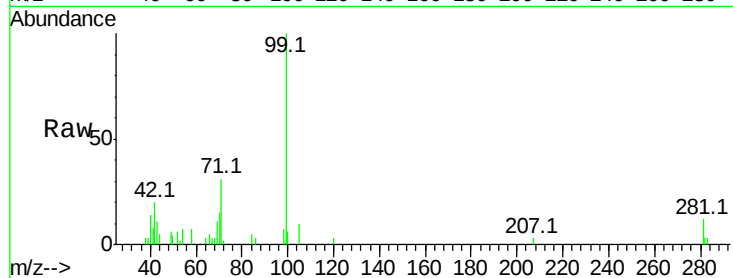

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

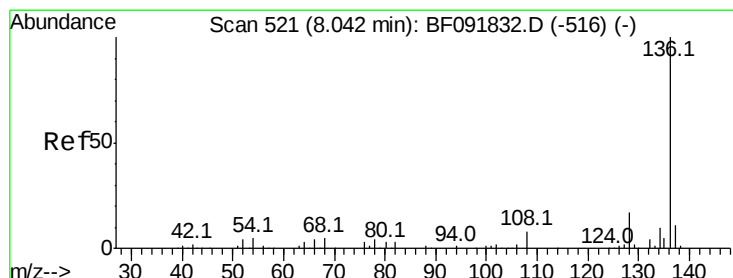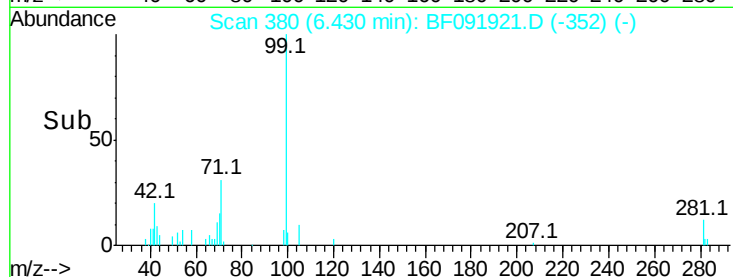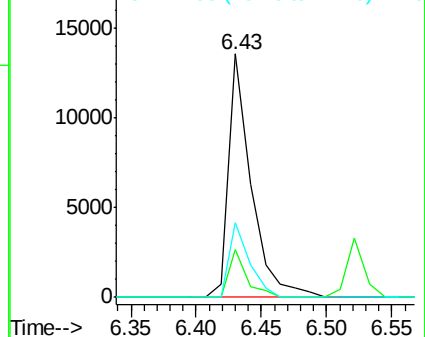

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.03 min Scan# 520

Delta R.T. -0.01 min

Lab File: BF091921.D

Acq: 23 Dec 2016 14:08

Tgt Ion: 136 Resp: 898276


Ion Ratio Lower Upper

136 100

137 10.6 8.4 12.6

54 6.2 4.5 6.7

68 4.8 3.6 5.4


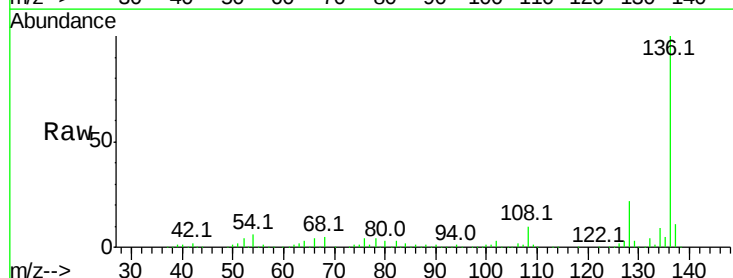



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



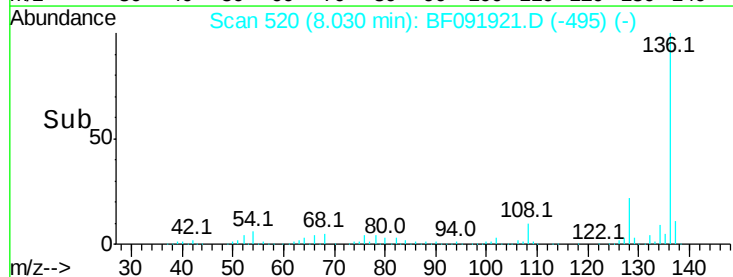
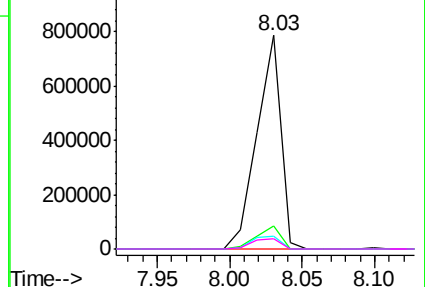


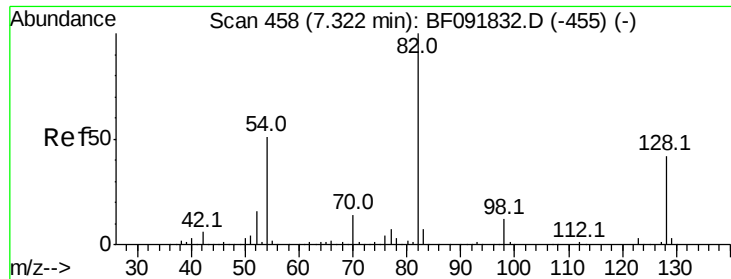

#23
 Nitrobenzene-d5
 Concen: 2.28 ng
 RT: 7.30 min Scan# 456
 Delta R.T. -0.02 min
 Lab File: BF091921.D
 Acq: 23 Dec 2016 14:08




Instrument :
 BNA_F
 ClientSampleId :
 WC-201612DL


Tot Ion: 82 Resp: 36771
 Ion Ratio Lower Upper
 82 100
 128 37.6 34.6 52.0
 54 52.3 39.5 59.3

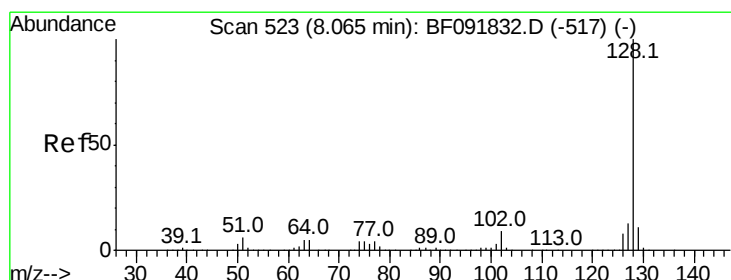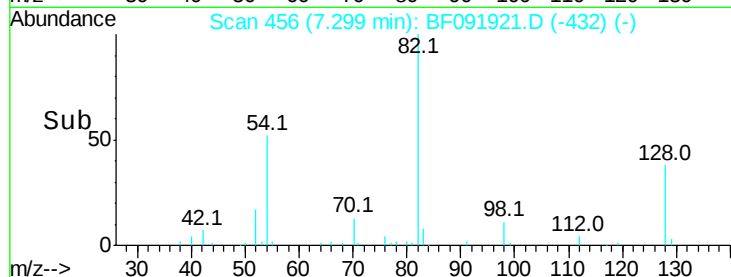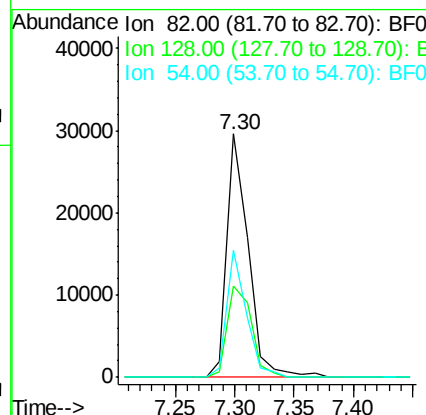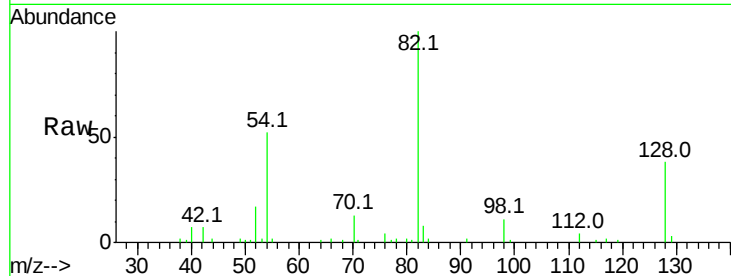

#31
 Naphthalene
 Concen: 46.36 ng
 RT: 8.05 min Scan# 522
 Delta R.T. -0.01 min
 Lab File: BF091921.D
 Acq: 23 Dec 2016 14:08

Tgt Ion: 128 Resp: 1905878
 Ion Ratio Lower Upper
 128 100
 129 10.9 9.5 14.3
 127 13.5 10.8 16.2

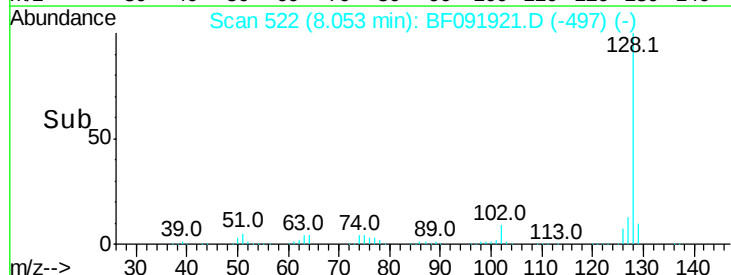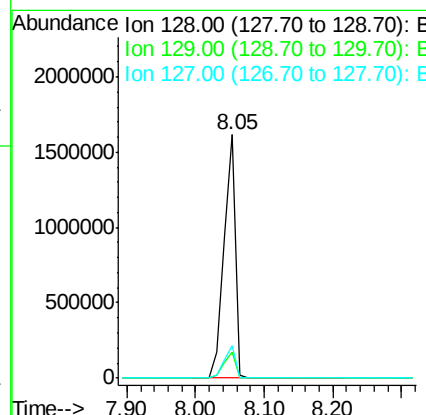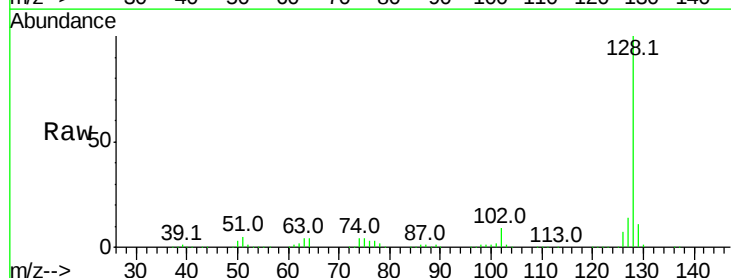


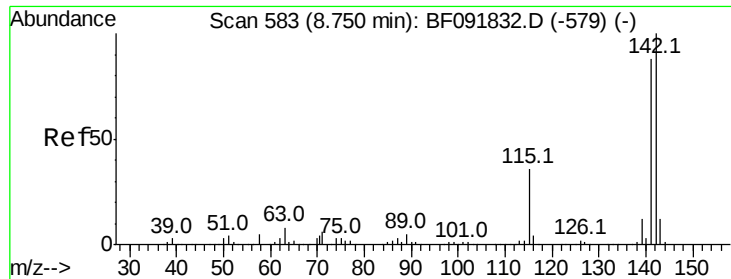




#37
2-Methylnaphthalene
Concen: 2.43 ng
RT: 8.74 min Scan# 582
Delta R.T. -0.01 min
Lab File: BF091921.D
Acq: 23 Dec 2016 14:08

Instrument :
BNA_F
ClientSampleId :
WC-201612DL

Tot Ion:142 Resp: 92347
Ion Ratio Lower Upper
142 100
141 89.8 71.0 106.6
115 31.5 28.3 42.5

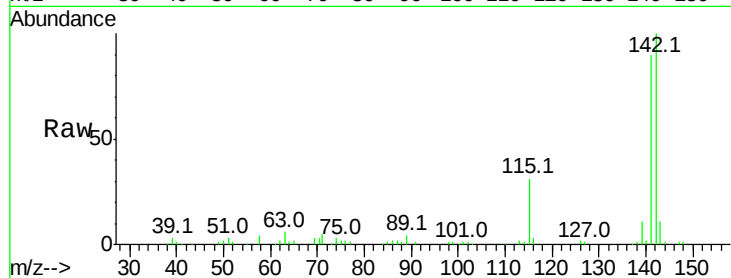


Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 115.00 (114.70 to 115.70): E

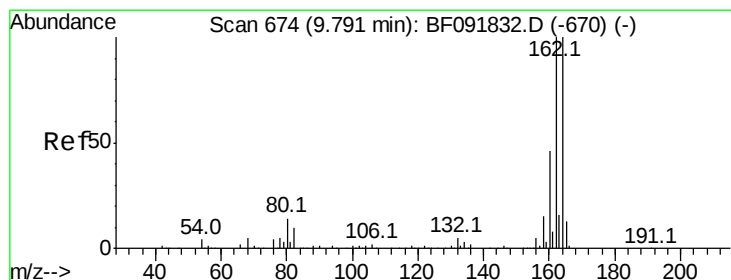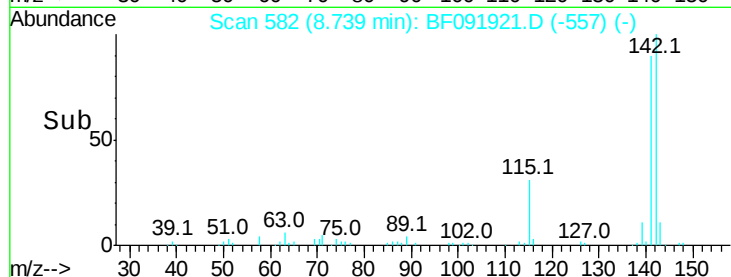
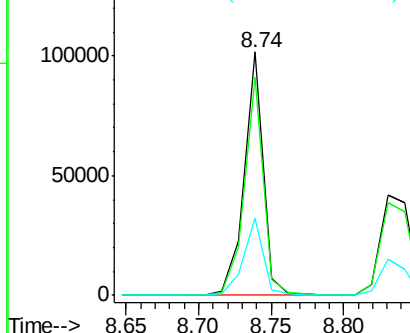



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.78 min Scan# 673
Delta R.T. -0.01 min
Lab File: BF091921.D
Acq: 23 Dec 2016 14:08

Tgt Ion:164 Resp: 495614
Ion Ratio Lower Upper
164 100
162 100.8 80.2 120.2
160 45.4 36.9 55.3

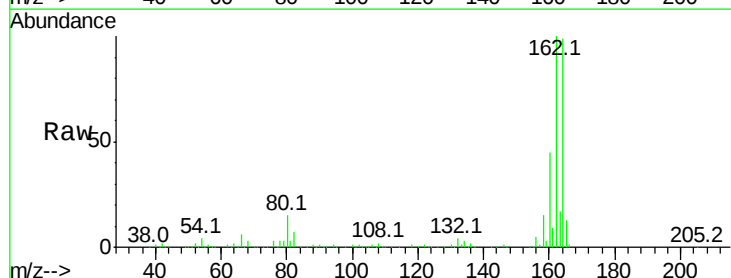

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

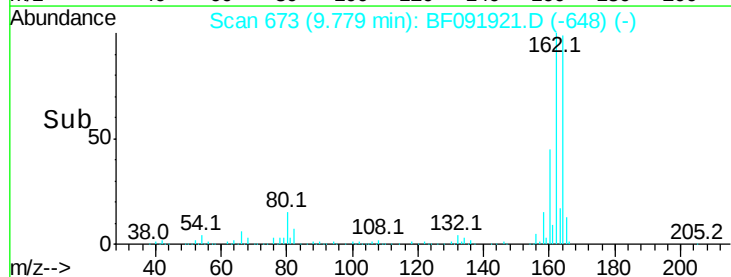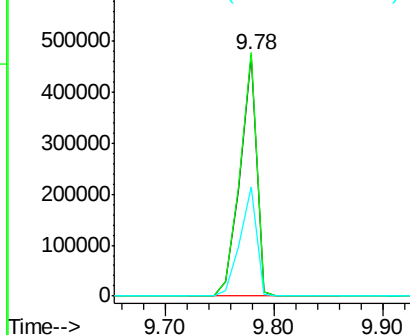


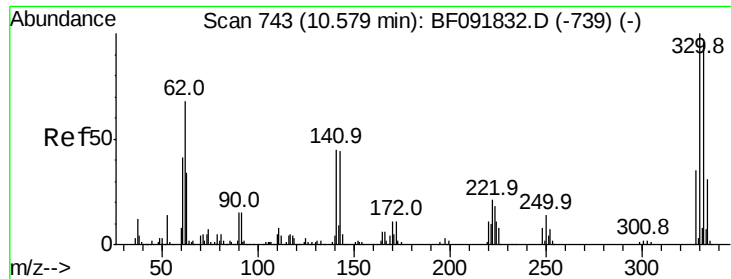




#41
 2,4,6-Tribromophenol
 Concen: 3.23 ng
 RT: 10.57 min Scan# 742
 Delta R.T. -0.01 min
 Lab File: BF091921.D
 Acq: 23 Dec 2016 14:08

Instrument :
 BNA_F
 ClientSampleId :
 WC-201612DL

Tot Ion:330 Resp: 13247
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.4 116.2
 141 35.4 34.1 51.1

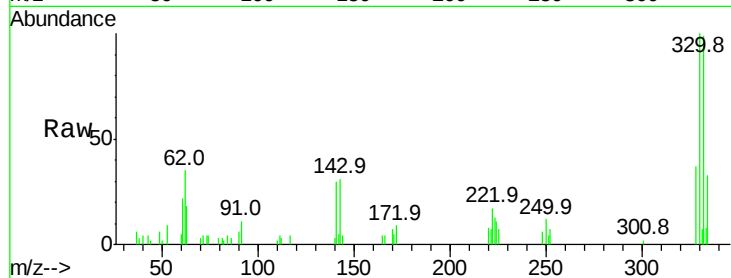


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

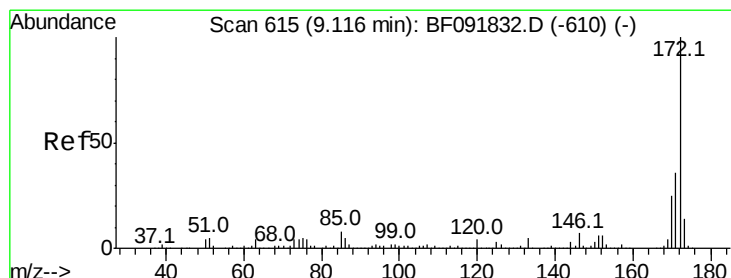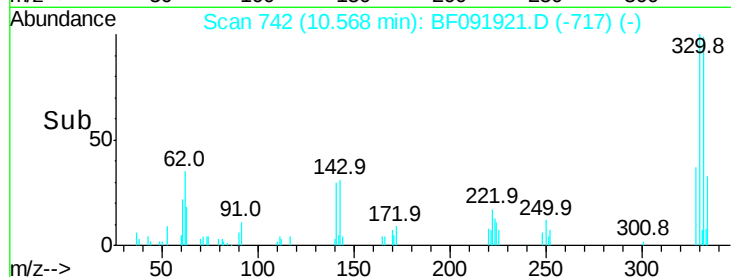
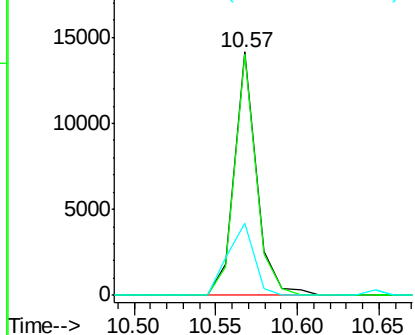



#44
 2-Fluorobiphenyl
 Concen: 2.43 ng
 RT: 9.10 min Scan# 614
 Delta R.T. -0.01 min
 Lab File: BF091921.D
 Acq: 23 Dec 2016 14:08

Tgt Ion:172 Resp: 62788
 Ion Ratio Lower Upper
 172 100
 171 34.1 29.4 44.0
 170 24.7 20.2 30.4

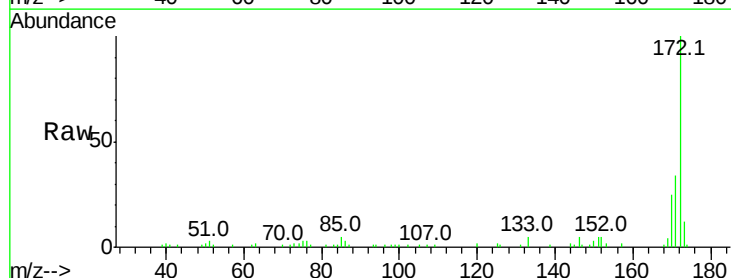

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

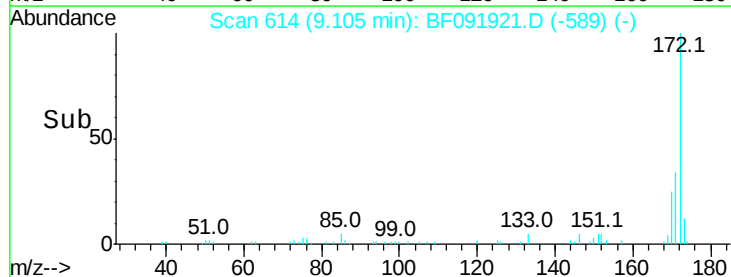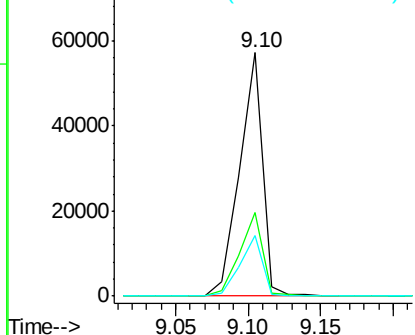


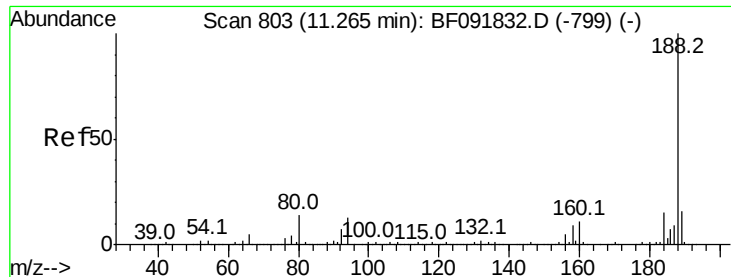




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.25 min Scan# 802
Delta R.T. -0.01 min
Lab File: BF091921.D
Acq: 23 Dec 2016 14:08

Instrument :
BNA_F
ClientSampleId :
WC-201612DL

Tot Ion:188 Resp: 770885
Ion Ratio Lower Upper
188 100
94 11.1 10.0 15.0
80 12.4 11.2 16.8

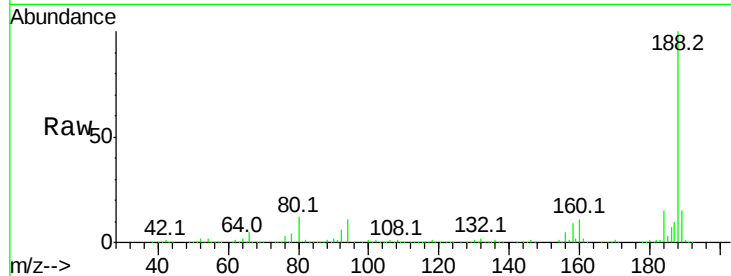


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

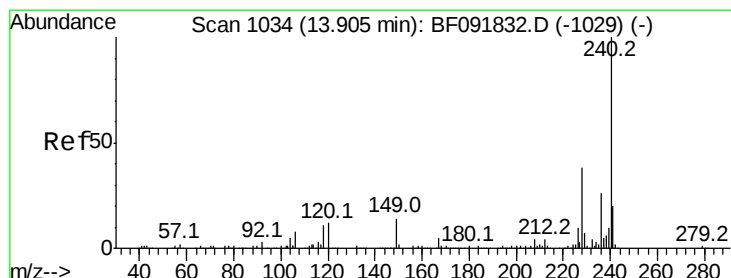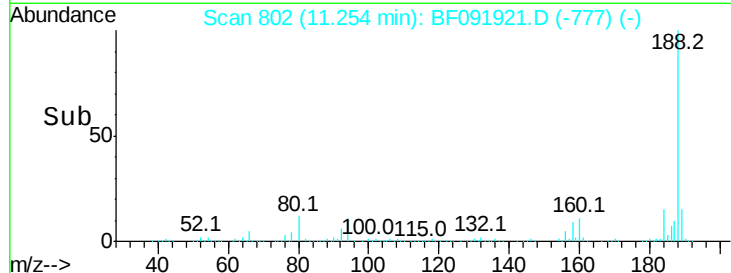
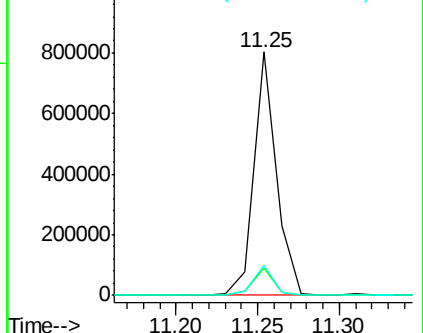



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.88 min Scan# 1032
Delta R.T. -0.02 min
Lab File: BF091921.D
Acq: 23 Dec 2016 14:08

Tgt Ion:240 Resp: 609833
Ion Ratio Lower Upper
240 100
120 15.2 12.9 19.3
236 25.9 20.9 31.3

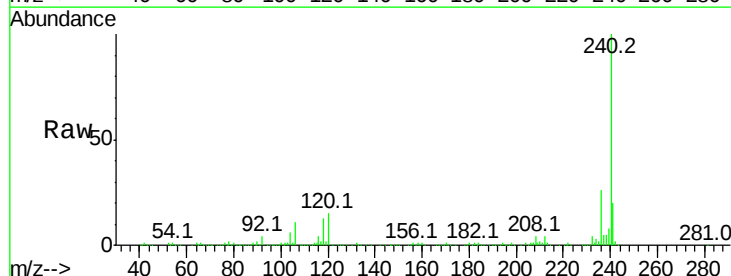

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



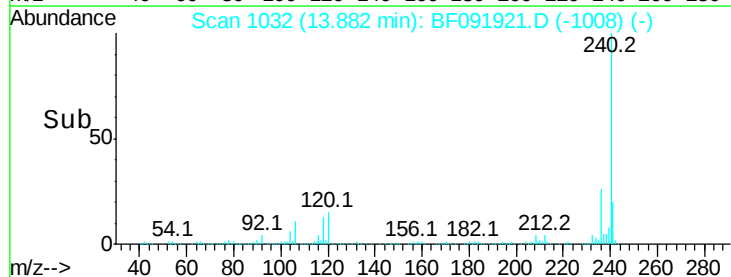
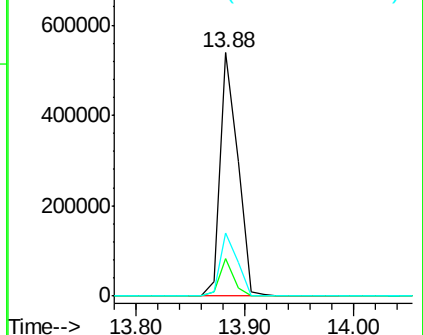


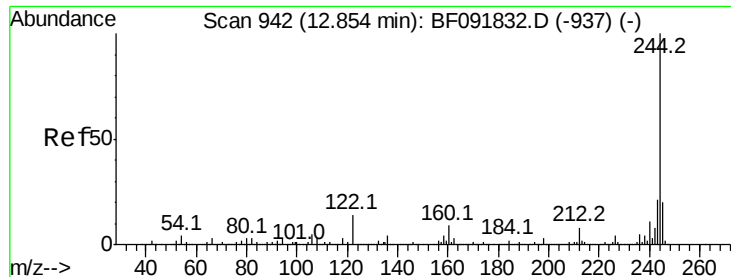

#78
 Terphenyl-d14
 Concen: 2.09 ng
 RT: 12.84 min Scan# 941
 Delta R.T. -0.01 min
 Lab File: BF091921.D
 Acq: 23 Dec 2016 14:08

Instrument :
 BNA_F
 ClientSampleID :
 WC-201612DL

Tot Ion:244 Resp: 52450
 Ion Ratio Lower Upper
 244 100
 212 5.3 6.2 9.2#
 122 6.7 11.4 17.2#

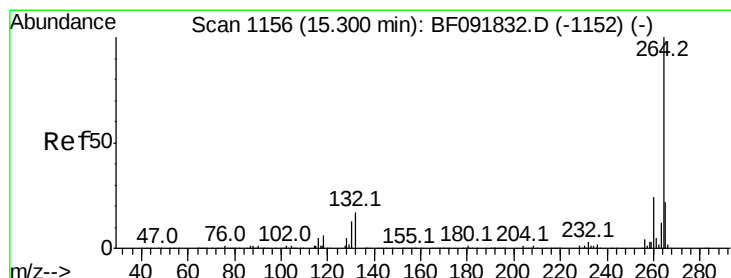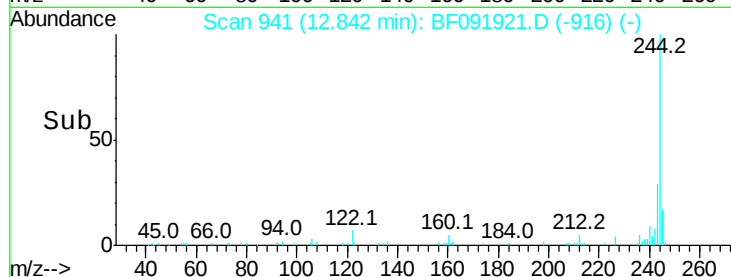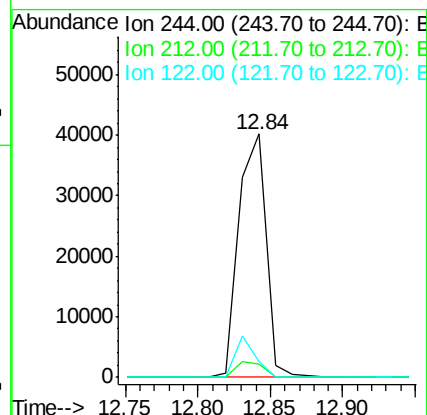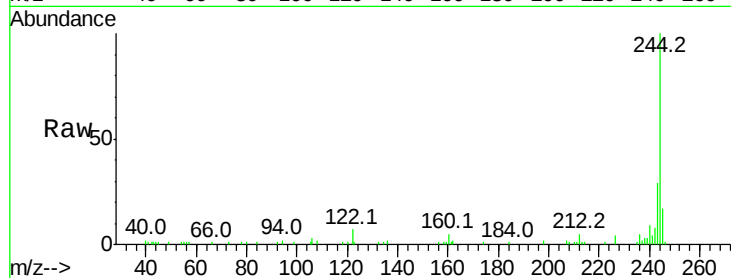

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.28 min Scan# 1154
 Delta R.T. -0.02 min
 Lab File: BF091921.D
 Acq: 23 Dec 2016 14:08

Tgt Ion:264 Resp: 492438
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.2 28.8
 265 21.9 17.4 26.0

