


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122316\
 Data File : BF091916.D
 Acq On : 23 Dec 2016 11:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 16:17:51 2016

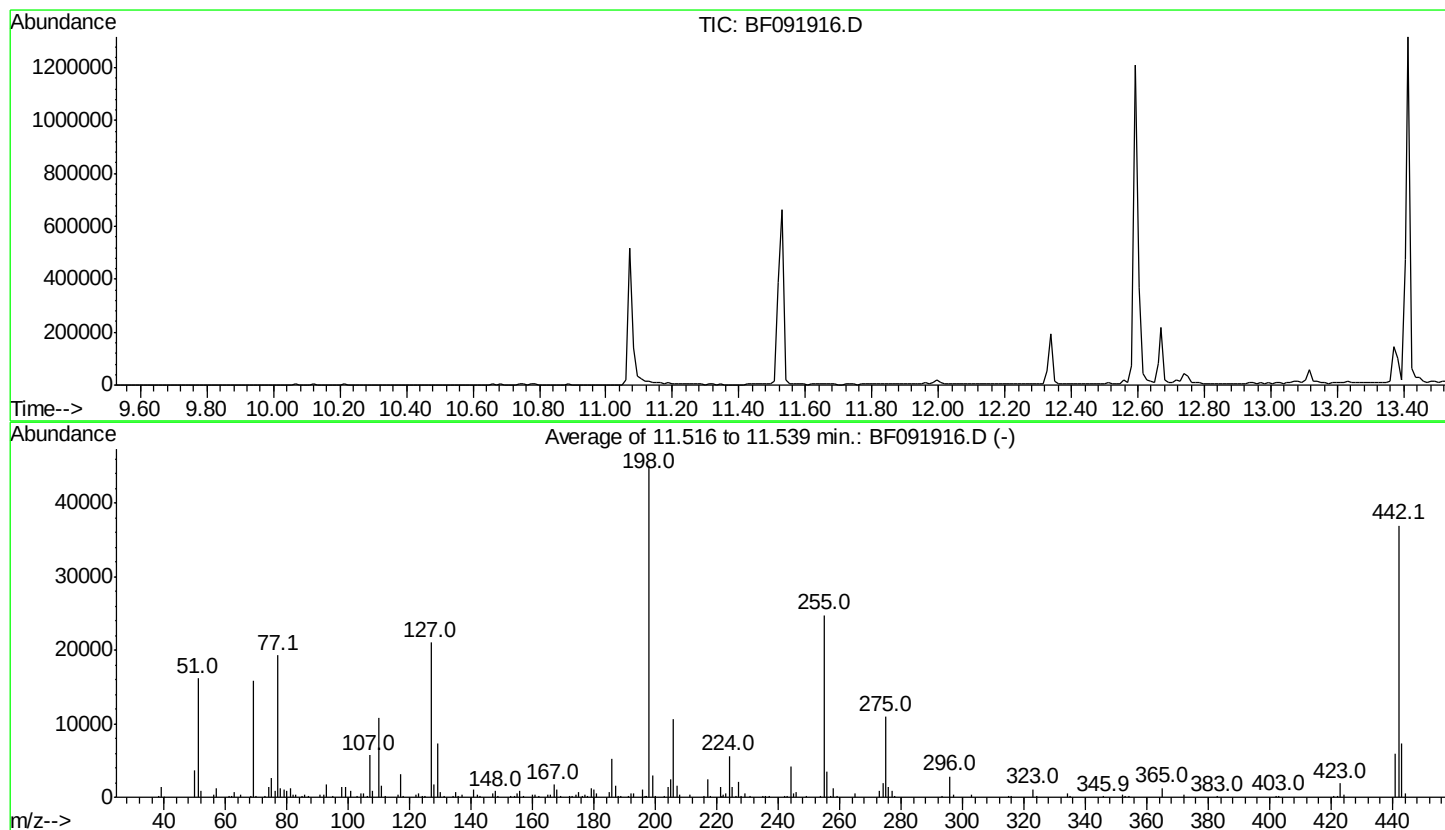

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	16195	PASS
68	69	0.00	2	1.1	181	PASS
69	198	0.00	100	35.0	15800	PASS
70	69	0.00	2	0.9	142	PASS
127	198	10	80	46.7	21064	PASS
197	198	0.00	2	0.5	209	PASS
198	198	100	100	100.0	45115	PASS
199	198	5	9	6.6	2979	PASS
275	198	10	60	24.2	10931	PASS
365	198	1	100	2.9	1311	PASS
441	442	0.01	24	15.9	5861	PASS
442	198	50	100	81.9	36934	PASS
443	442	15	24	20.0	7375	PASS