
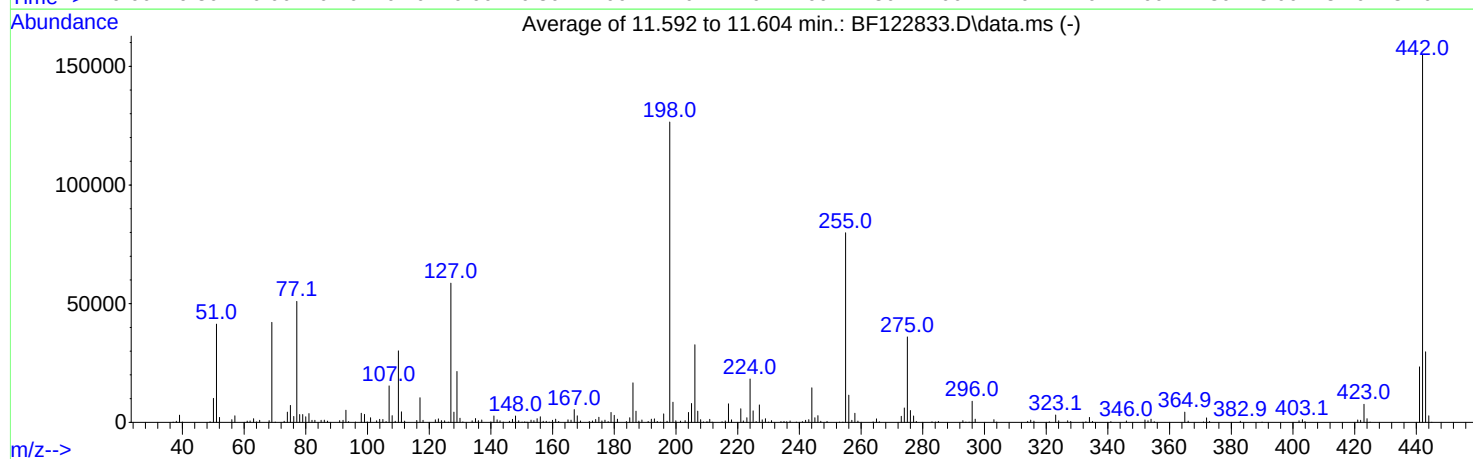


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122320\
 Data File : BF122833.D
 Acq On : 23 Dec 2020 12:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

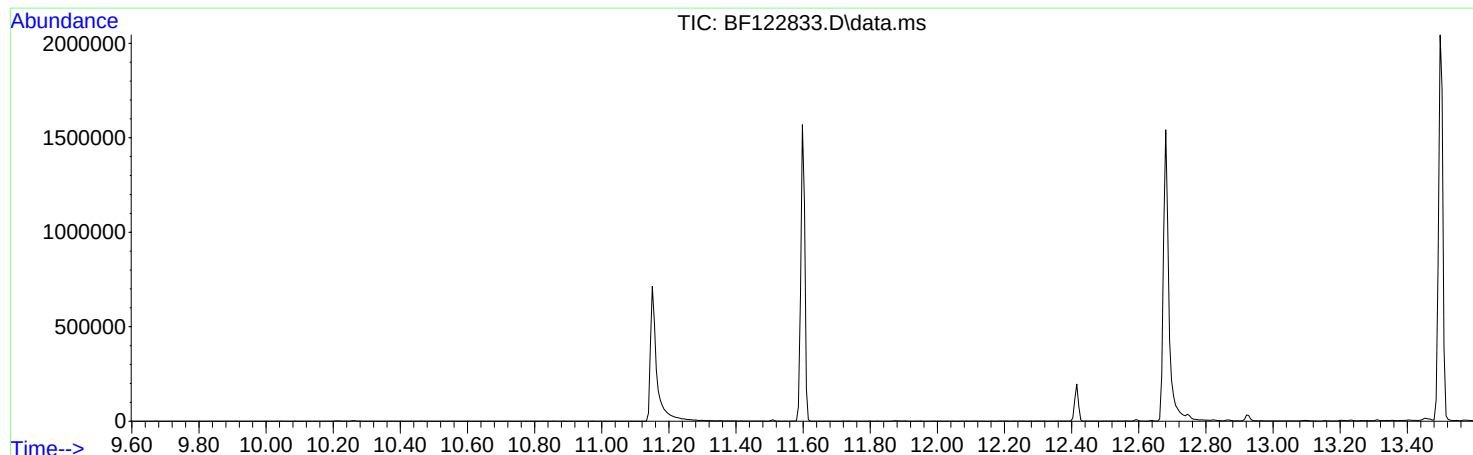

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	41411	PASS
68	69	0.00	2	1.8	763	PASS
69	198	0.00	100	33.3	42107	PASS
70	69	0.00	2	0.2	104	PASS
127	198	10	80	46.3	58619	PASS
197	198	0.00	2	0.4	492	PASS
198	198	100	100	100.0	126509	PASS
199	198	5	9	6.7	8531	PASS
275	198	10	60	28.4	35984	PASS
365	198	1	100	3.4	4300	PASS
441	198	0.01	100	18.5	23377	PASS
442	442	100	100	100.0	154973	PASS
443	442	15	24	19.2	29724	PASS