


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122322\  
 Data File : BF131800.D  
 Acq On : 23 Dec 2022 10:00  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122022.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Dec 24 00:05:44 2022

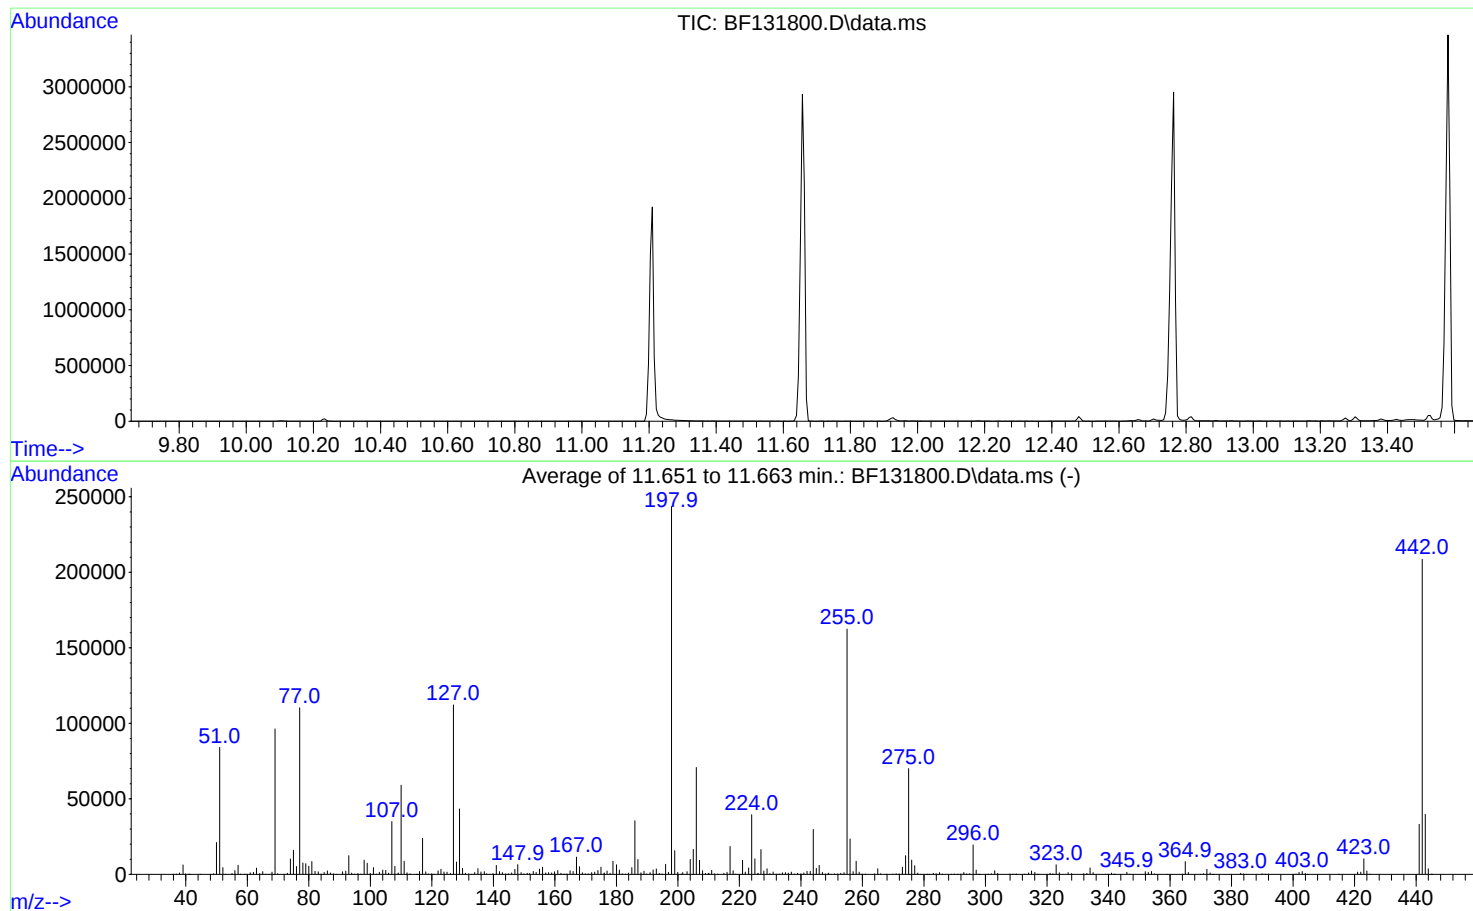




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.5         | 84107      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 1493       | PASS                |
| 69             | 198             | 0.00            | 100             | 39.5         | 96325      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 480        | PASS                |
| 127            | 198             | 10              | 80              | 46.0         | 112163     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1369       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 243584     | PASS                |
| 199            | 198             | 5               | 9               | 6.4          | 15657      | PASS                |
| 275            | 198             | 10              | 60              | 28.8         | 70072      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 8461       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.6         | 33125      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 208656     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 39784      | PASS                |

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122322\  
Data File : BF131800.D  
Acq On    : 23 Dec 2022  10:00  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

**Instrument :**  
BNA\_F  
**ClientSampleId :**  
DFTPP

Quant Time: Dec 24 06:08:06 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122022.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 24 00:05:44 2022  
Response via : Initial Calibration

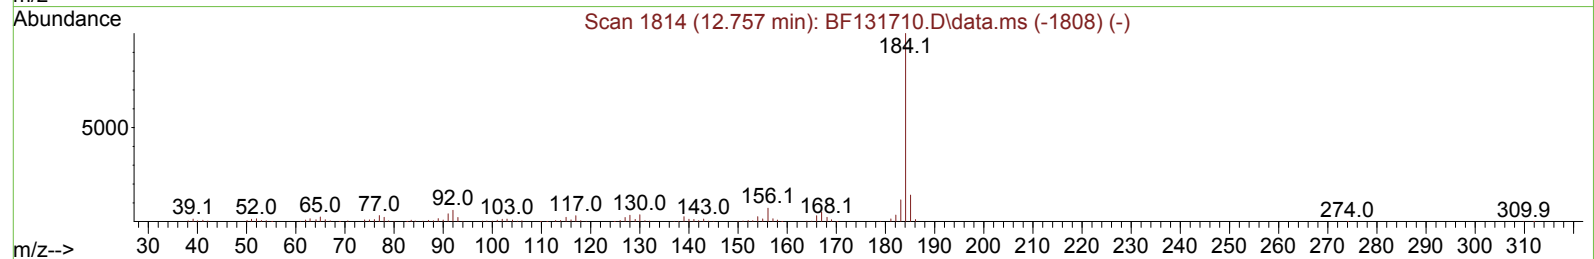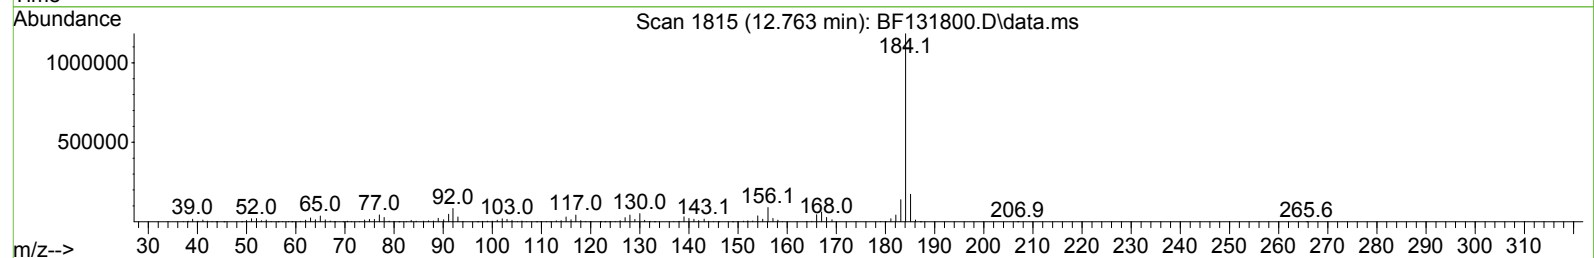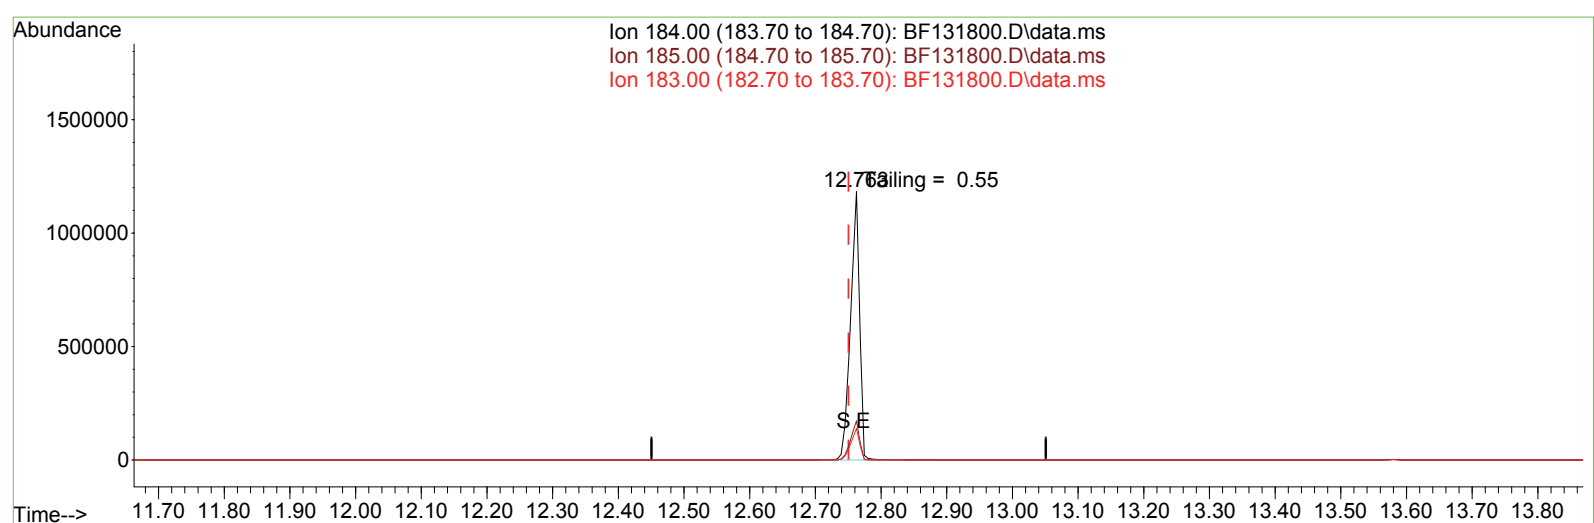

TIC: BF131800.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng




```
response      1132447
```

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.64  |
| 183.00 | 11.60  | 11.79  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122322\  
Data File : BF131800.D  
Acq On : 23 Dec 2022 10:00  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Dec 24 06:08:06 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122022.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 24 00:05:44 2022  
Response via : Initial Calibration

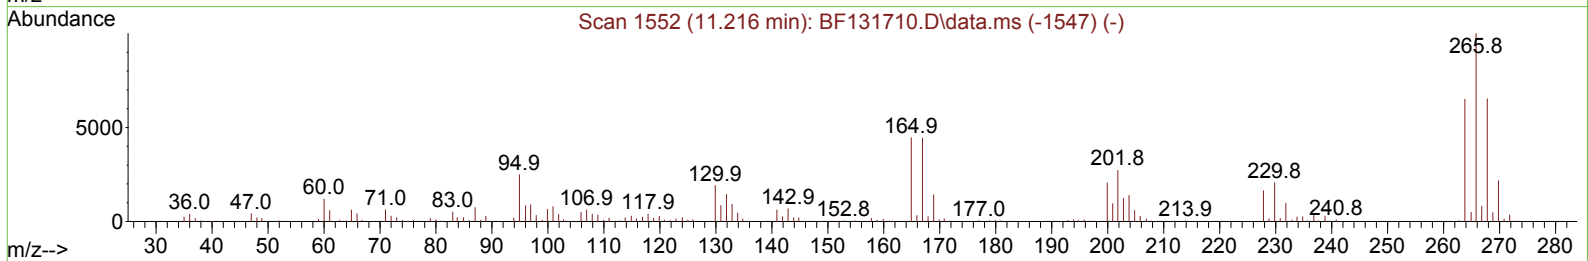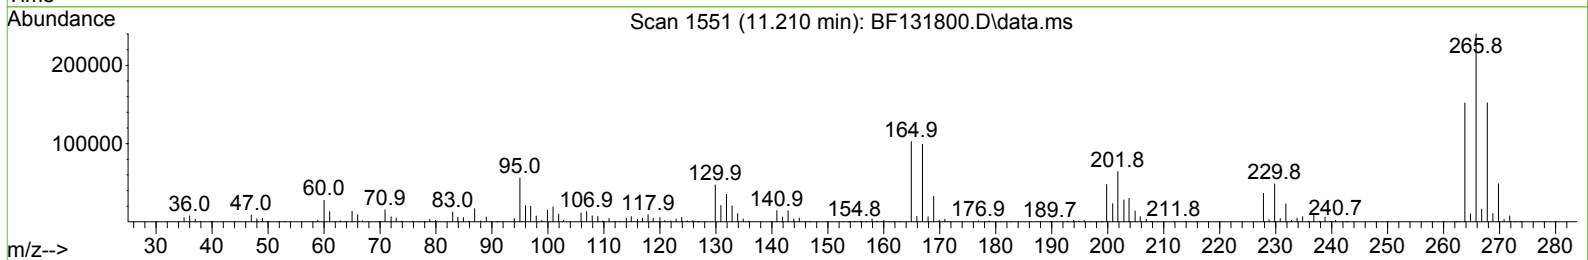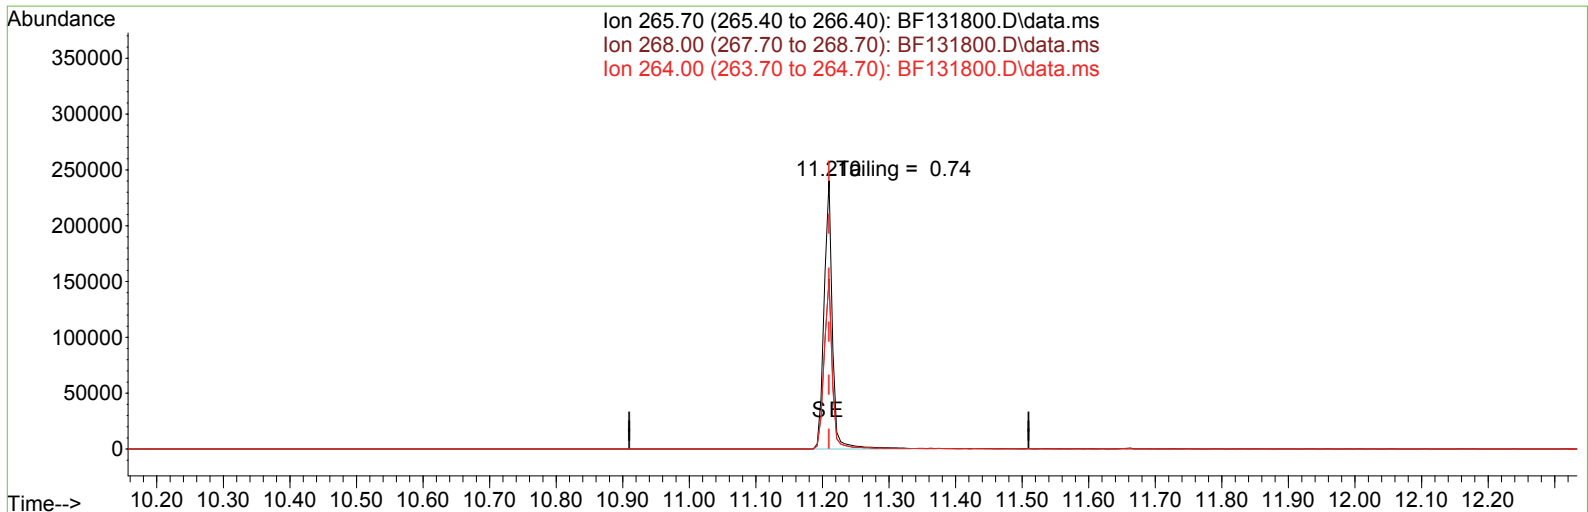

TIC: BF131800.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 24633.95 ng

response 208724

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.30  | 63.26  |
| 264.00 | 65.00  | 63.15  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/23/2022    | BNA_F            | <u>BF131800.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 589805           | 13.58              |
| DDD           | 10180            | 13.304             |
| DDE           | 579              | 12.933             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10759         | 600564           | 1.79               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP