
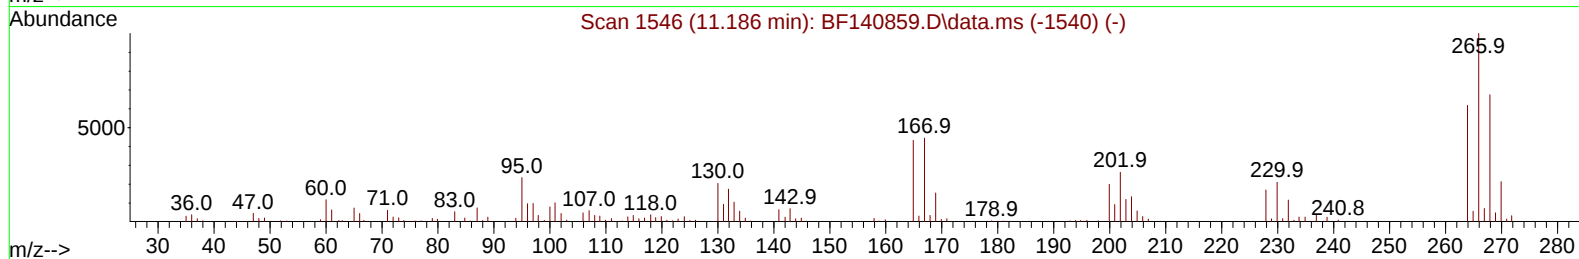
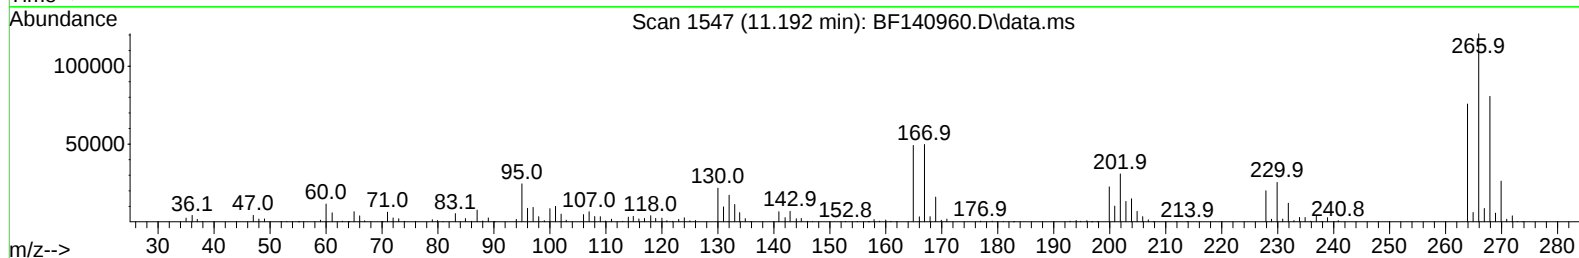


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122324\
Data File : BF140960.D
Acq On : 23 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 11:30:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

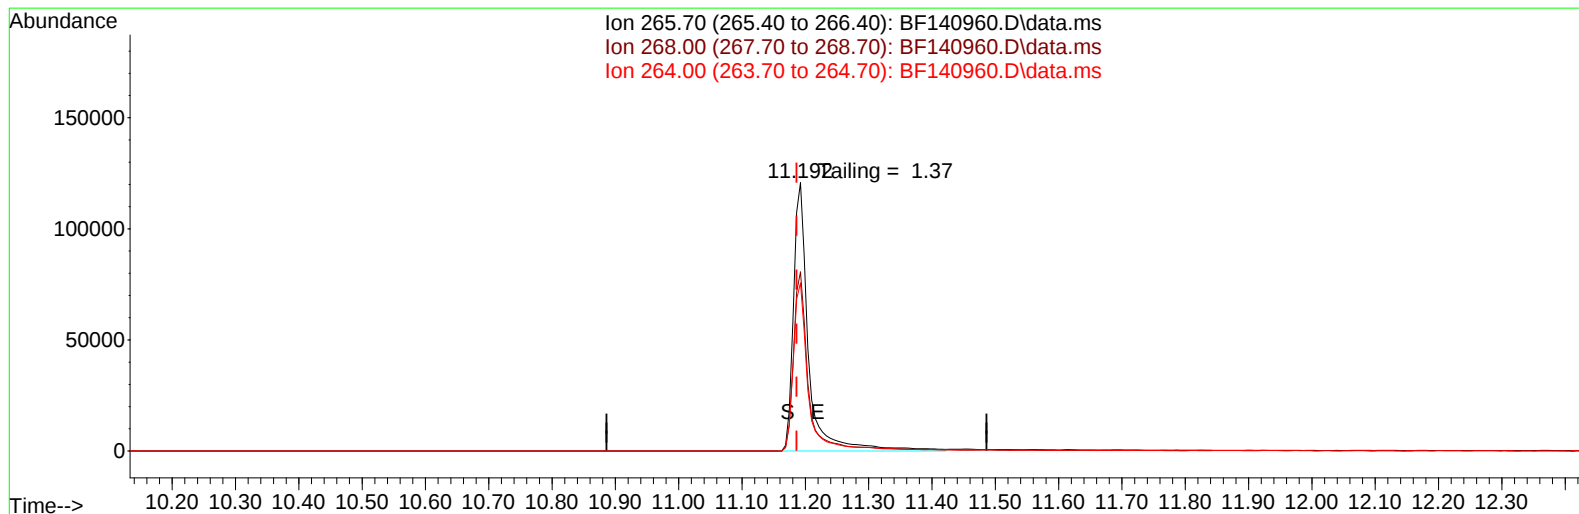

TIC: BF140960.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.006) 23080.12 ng

response 202074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	66.80
264.00	61.80	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122324\
Data File : BF140960.D
Acq On : 23 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 11:30:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

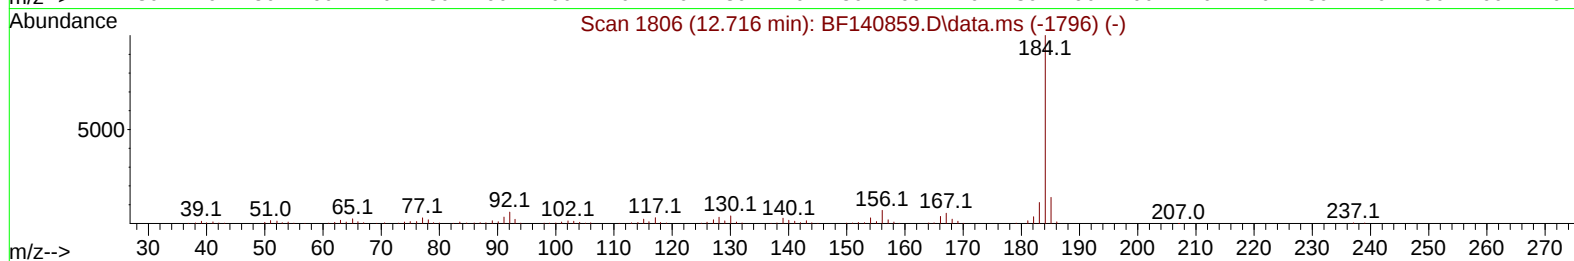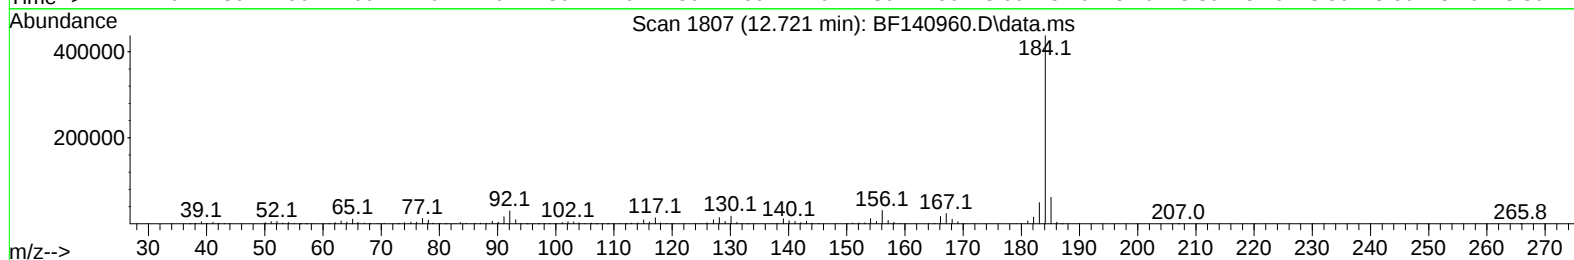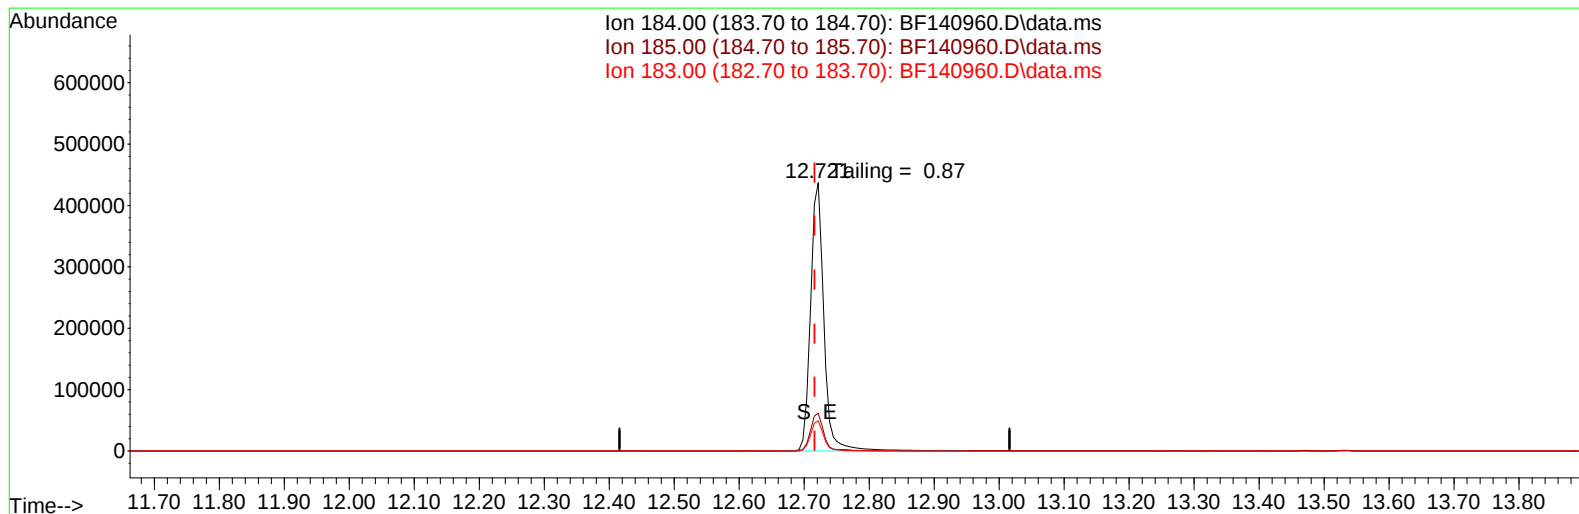

TIC: BF140960.D\data.ms

(77) Benzidine

12.721min (+ 0.005) 19990.23 ng

response 627493

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.08
183.00	11.20	11.28
0.00	0.00	0.00