



Hexachlorocyclopentadiene

Response Ratio

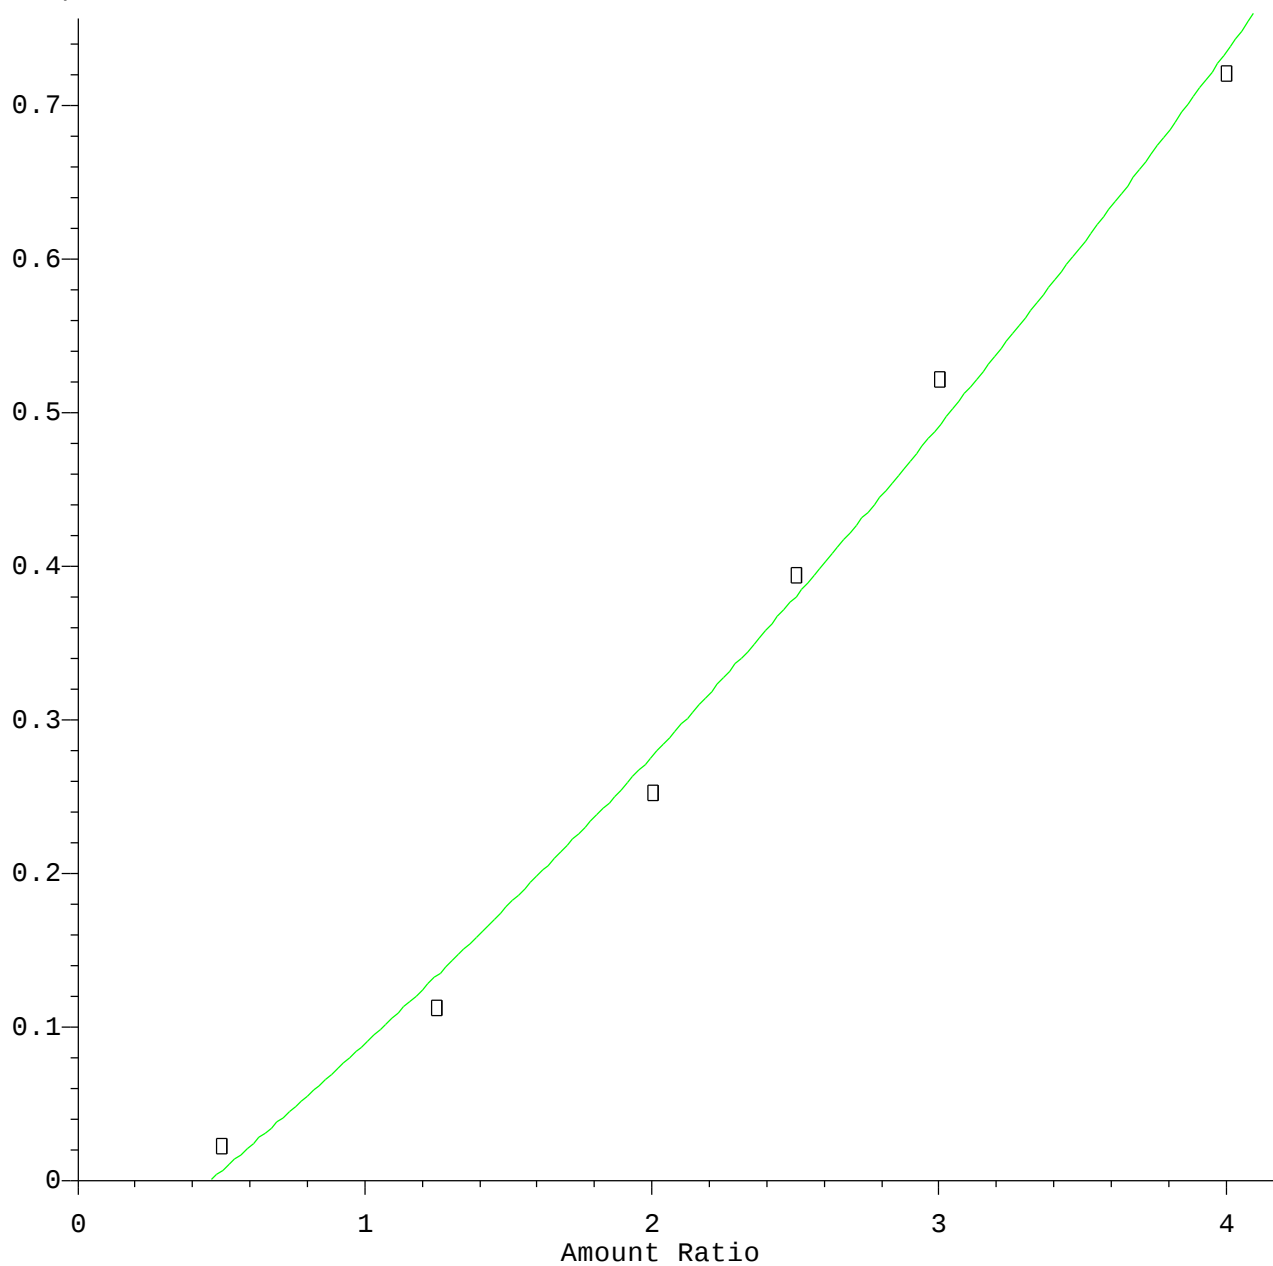


$R = 1.41e-002 A^2 + 1.44e-001 A - 6.90e-002$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Calibration Table Last Updated: Thu Dec 24 16:48:39 2015

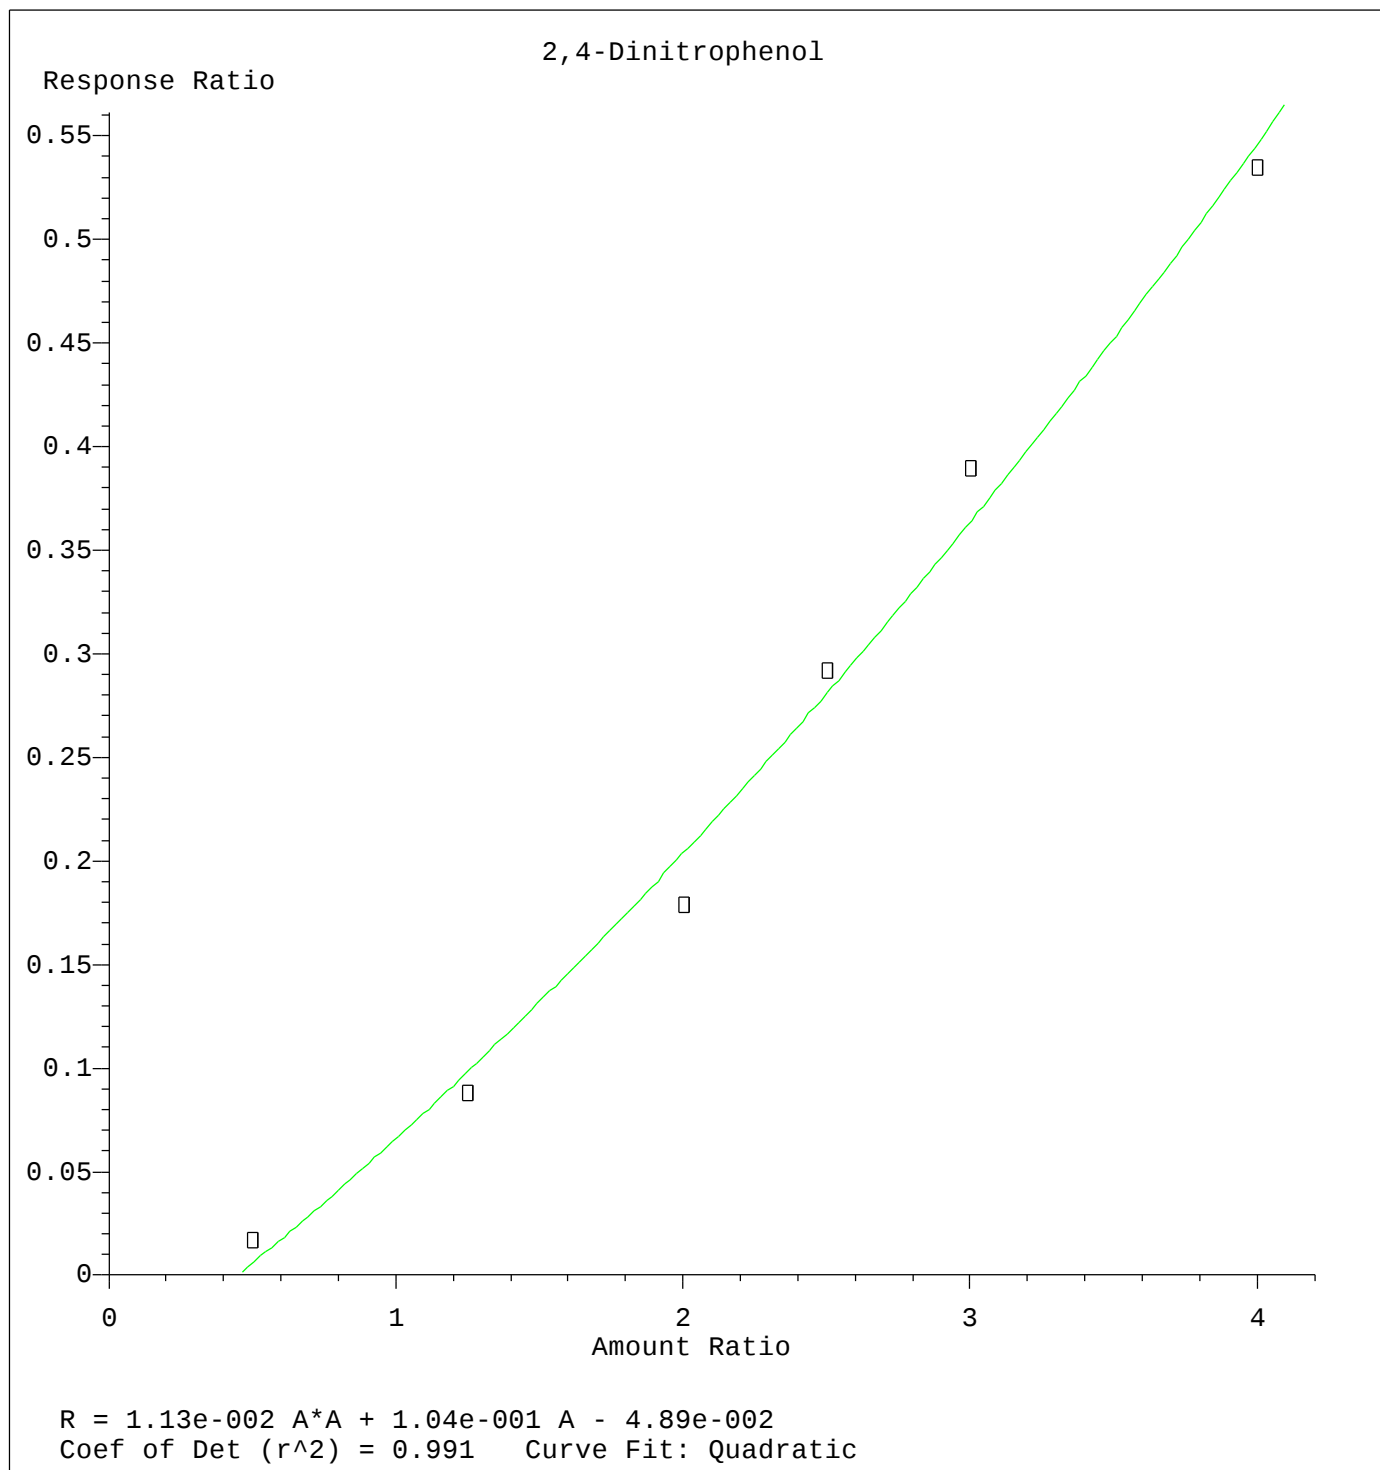


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Calibration Table Last Updated: Thu Dec 24 16:48:39 2015

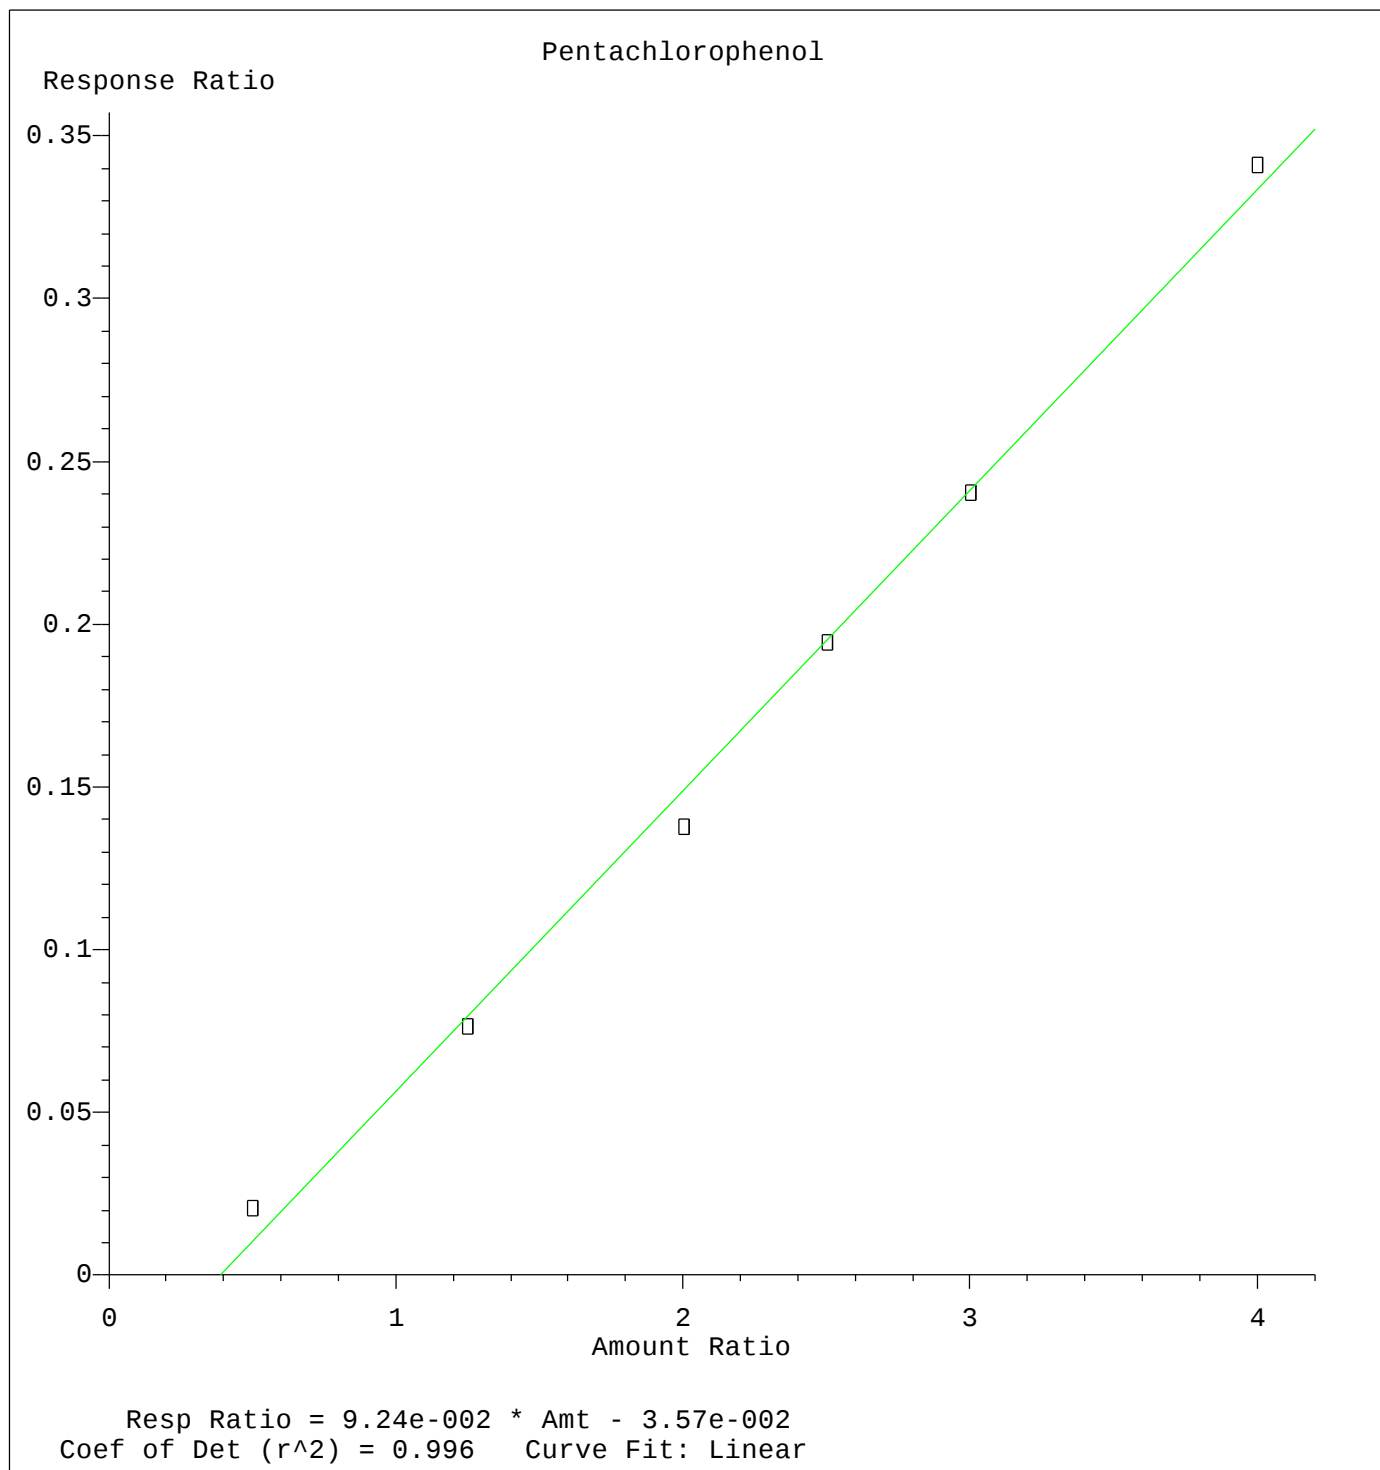

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Calibration Table Last Updated: Thu Dec 24 16:48:39 2015

Fluoranthene

Response Ratio

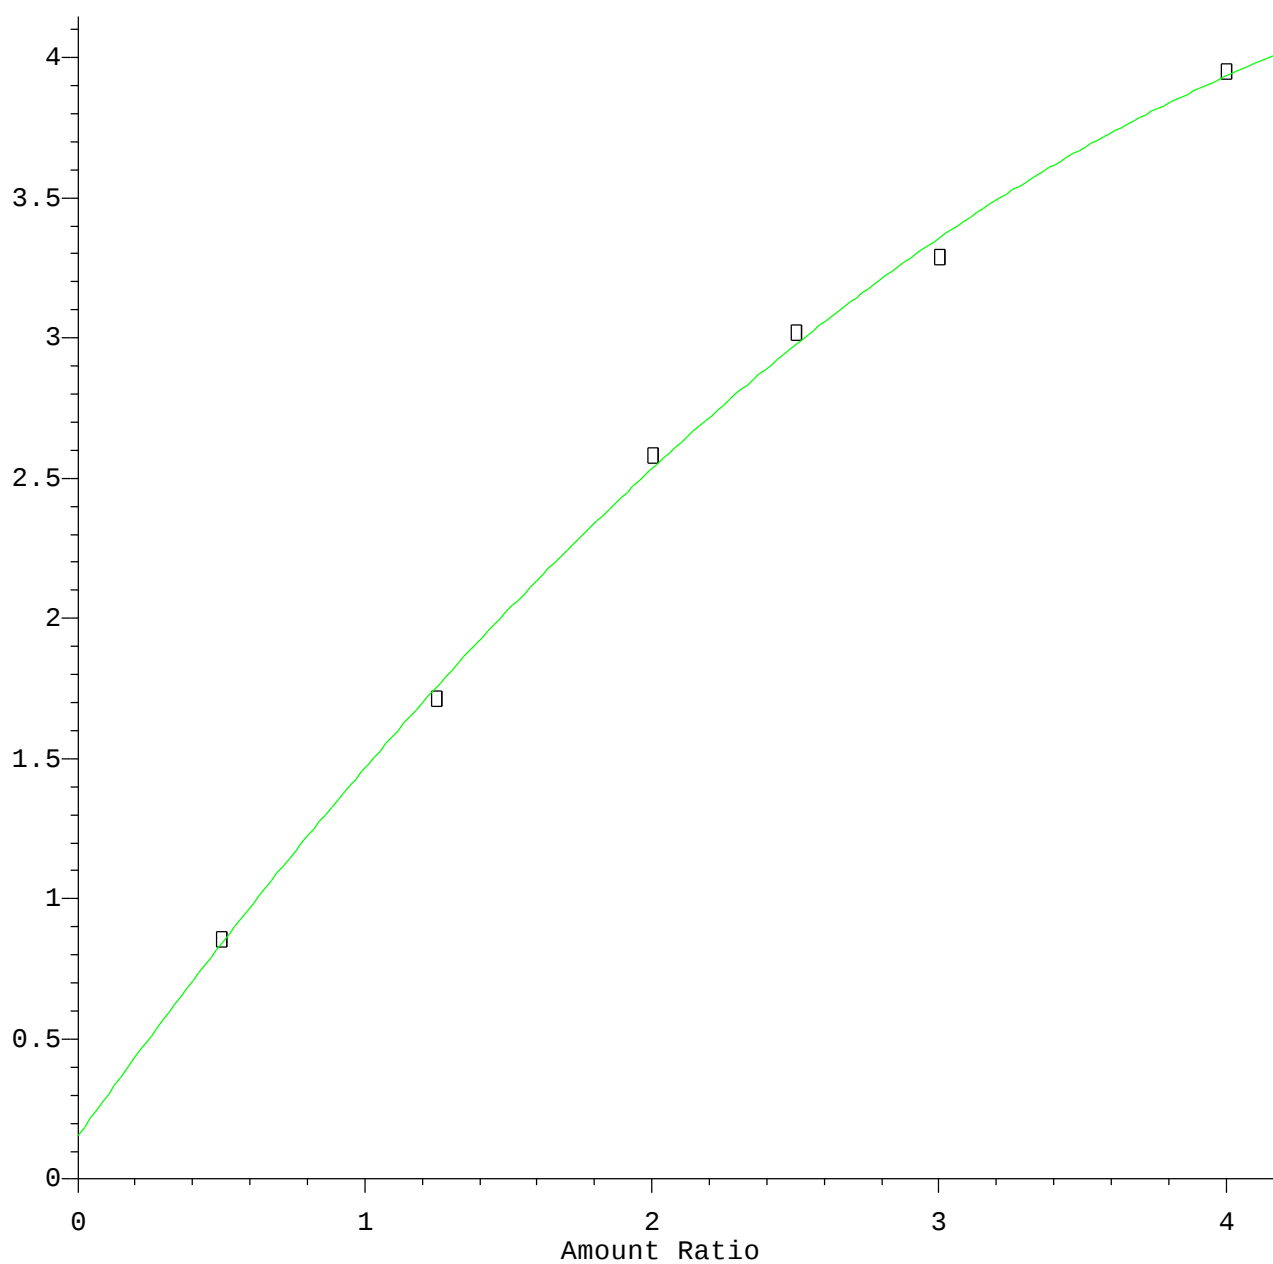

$R = -1.23e-001 A^2 + 1.43e+000 A + 1.54e-001$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Calibration Table Last Updated: Thu Dec 24 16:48:39 2015