
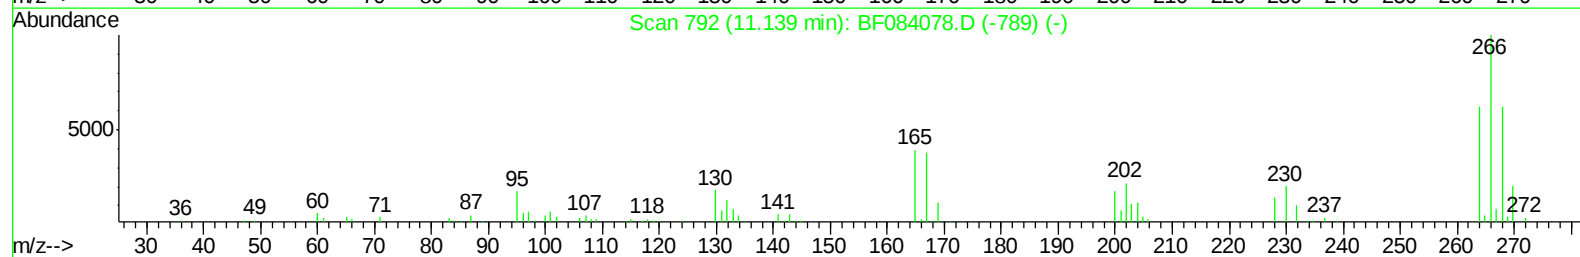
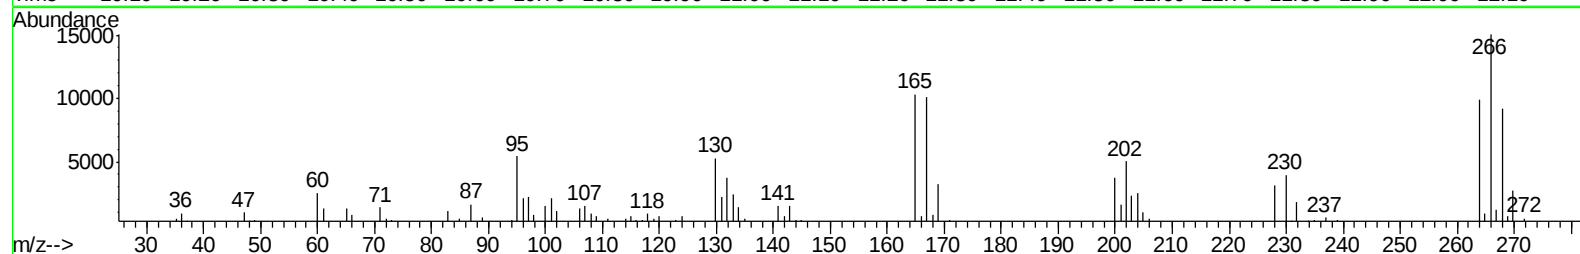


Data Path : Z:\HPCHEM1\BNA F\Data\BF122415\
Data File : BF084084.D
Acq On : 24 Dec 2015 17:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 02:54:49 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 24 16:48:39 2015
Response via : Initial Calibration

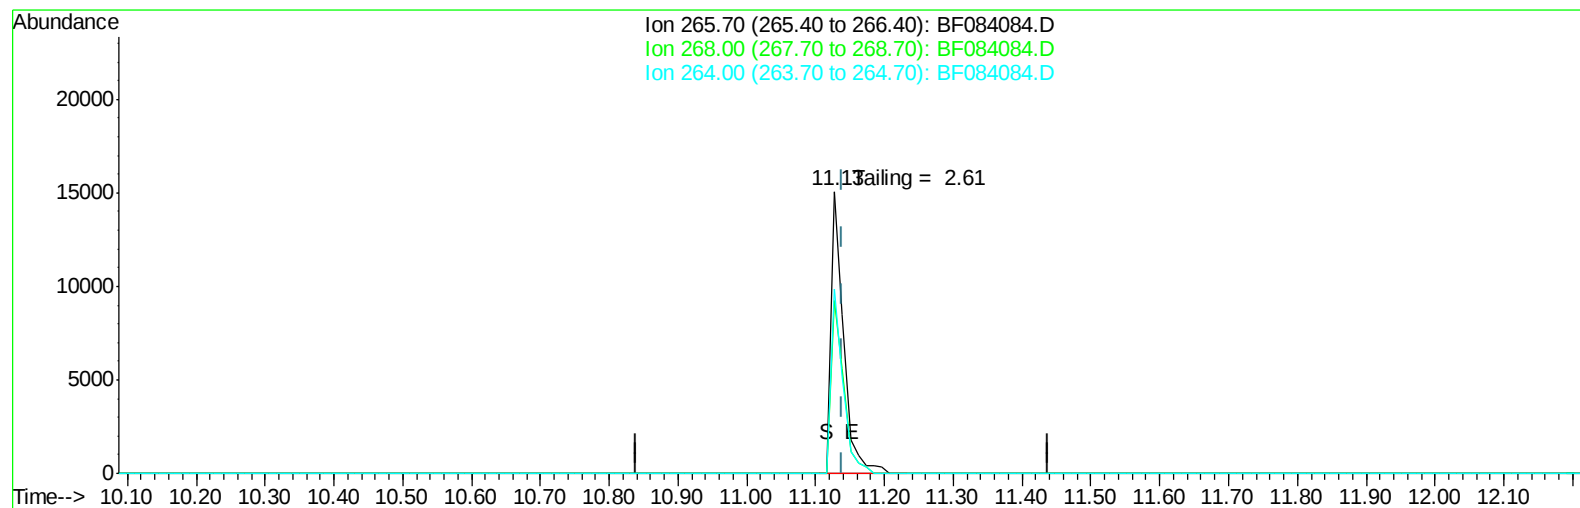

TIC: BF084084.D

(69) Pentachlorophenol (C)




11.128min (-0.011) 17188.37ng

response 18802

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.21
264.00	62.70	65.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF122415\
 Data File : BF084084.D
 Acq On : 24 Dec 2015 17:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 02:54:49 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 24 16:48:39 2015
 Response via : Initial Calibration

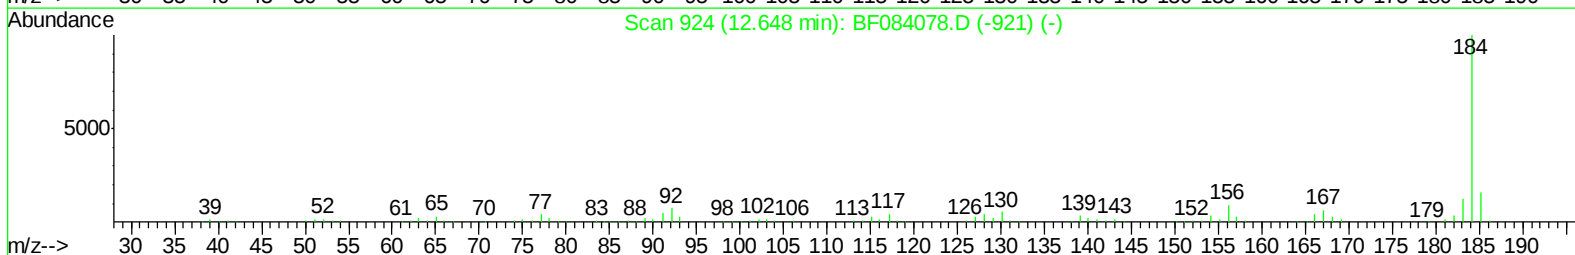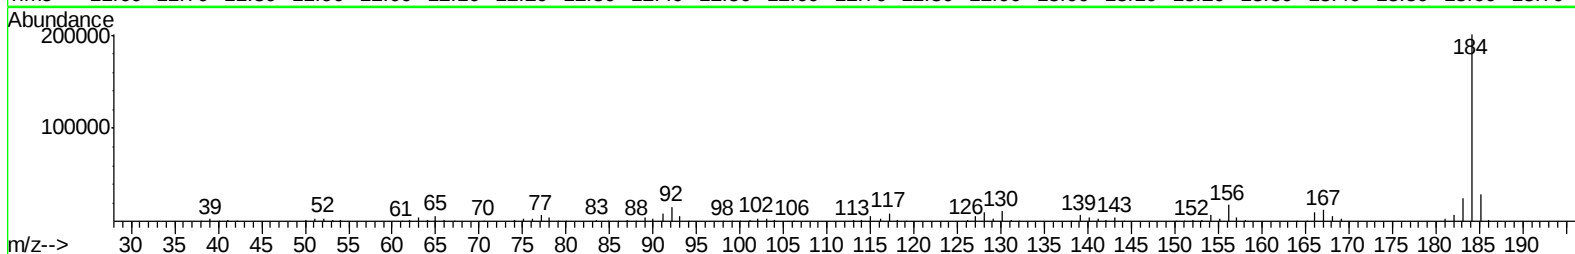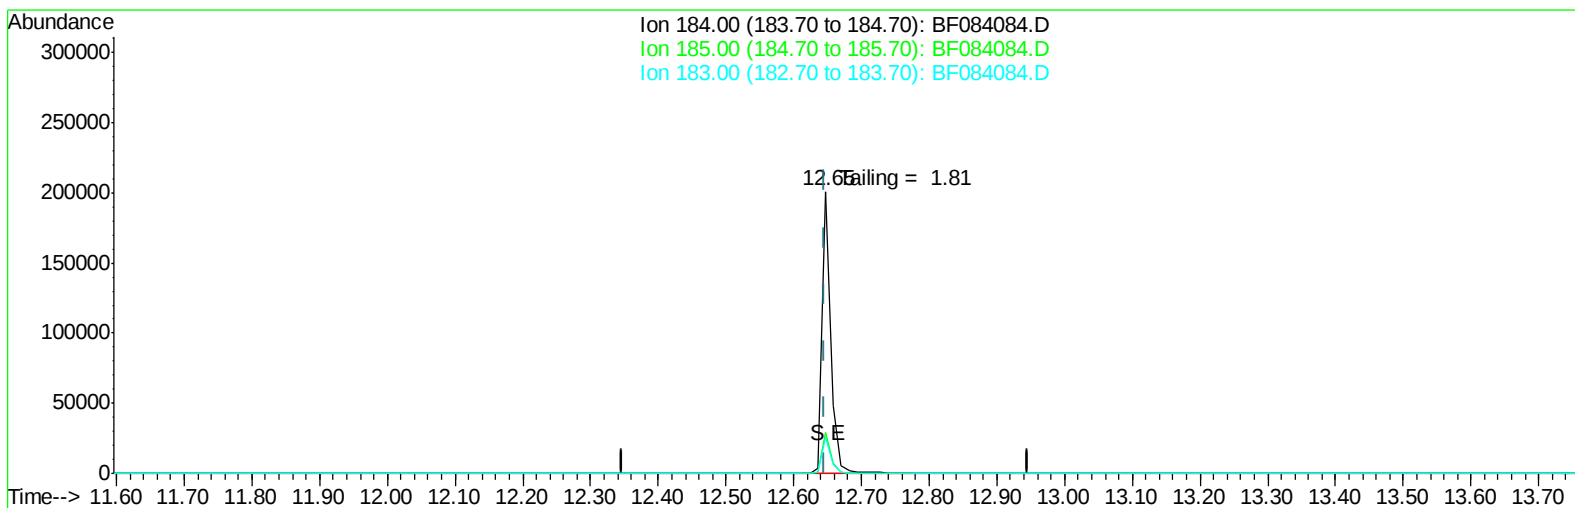

TIC: BF084084.D

(76) Benzidine

12.648min (+0.001) 1672.43ng

response 181327

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.61
183.00	12.30	12.66
0.00	0.00	0.00