
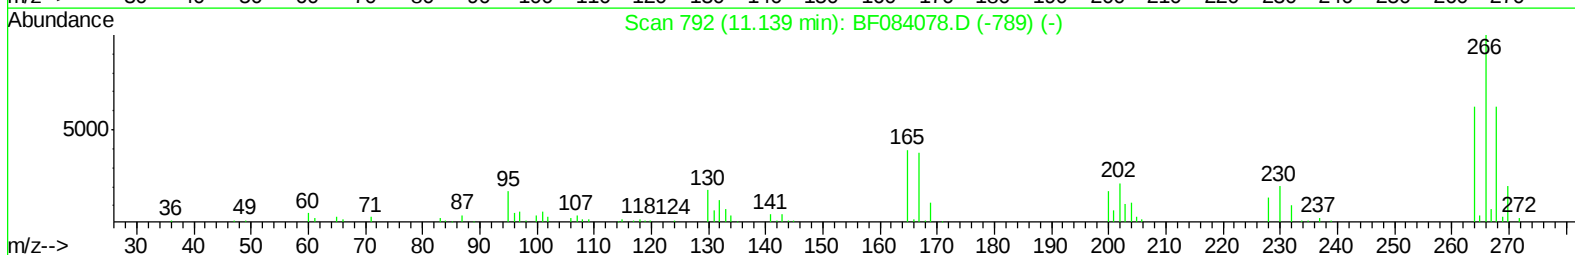
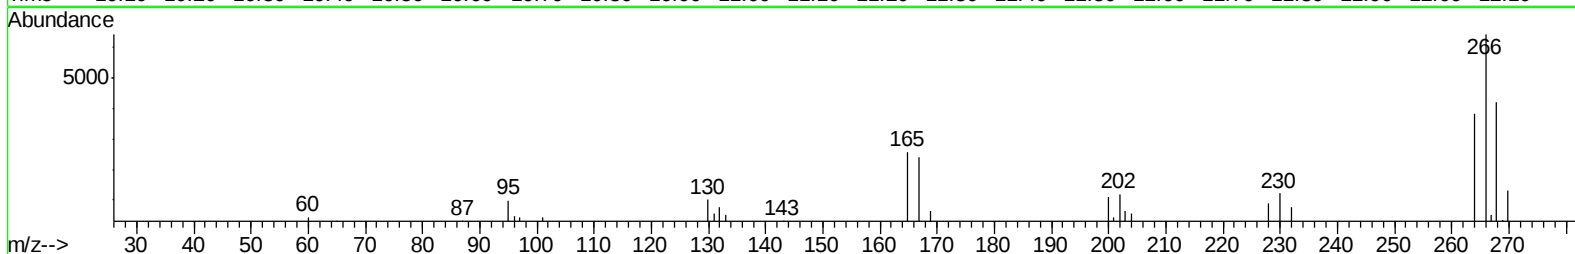


Data Path : Z:\HPCHEM1\BNA F\Data\BF122415\
Data File : BF084108.D
Acq On : 25 Dec 2015 5:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 02:56:23 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 24 16:48:39 2015
Response via : Initial Calibration

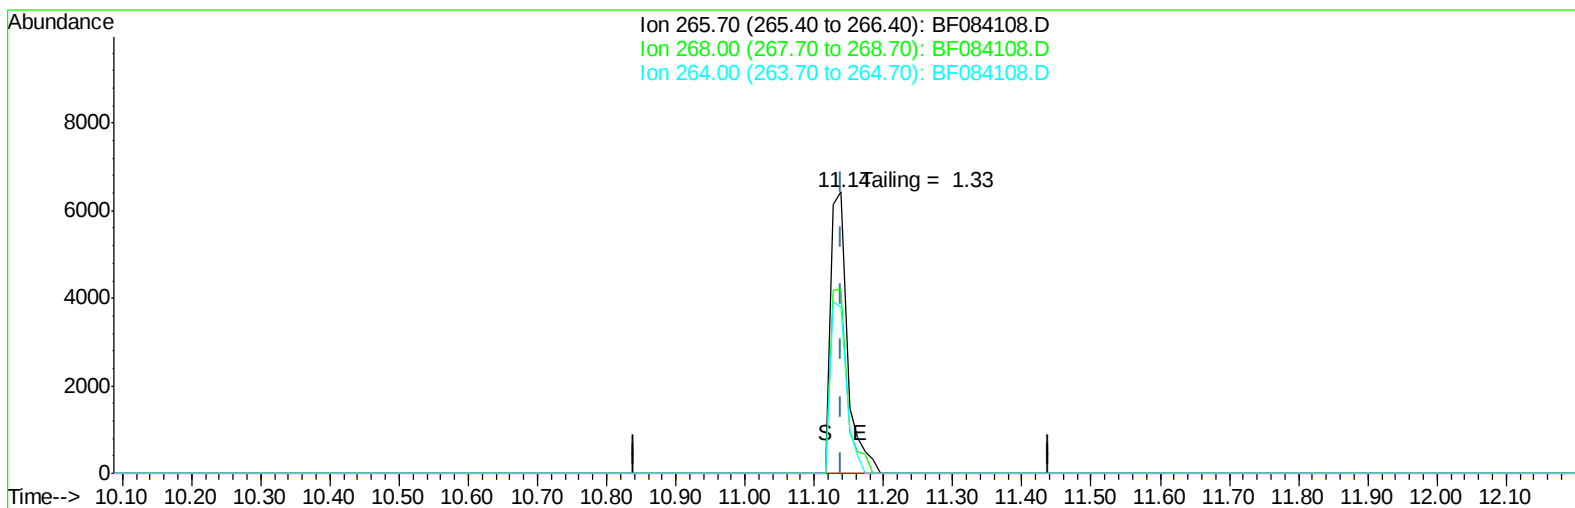

TIC: BF084108.D

(69) Pentachlorophenol (C)




11.139min (+0.000) 0.00ng

response 10756

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	65.52
264.00	62.70	59.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF122415\
Data File : BF084108.D
Acq On : 25 Dec 2015 5:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 02:56:23 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 24 16:48:39 2015
Response via : Initial Calibration

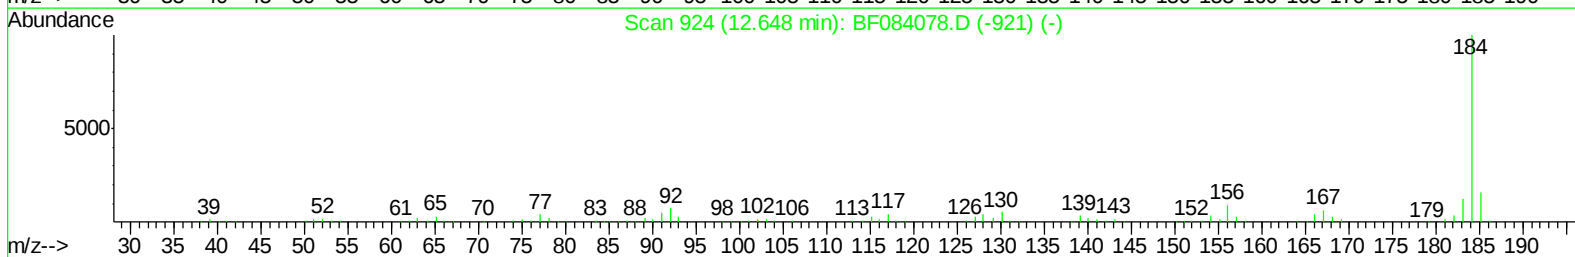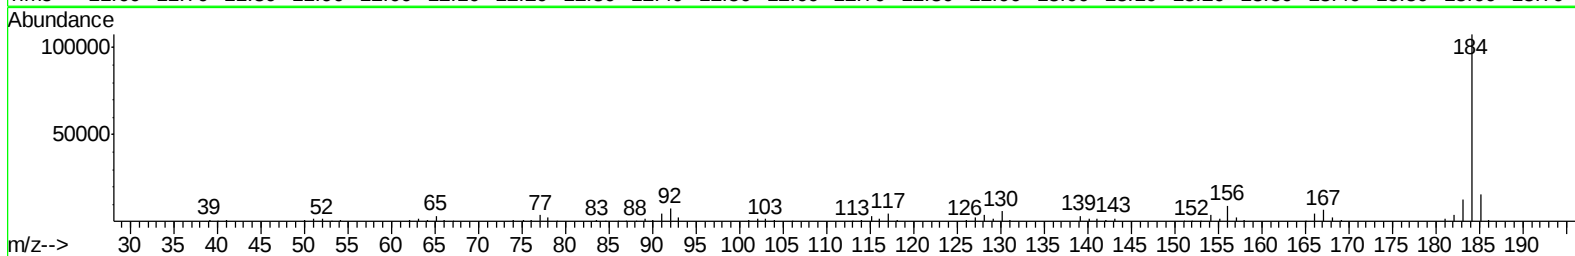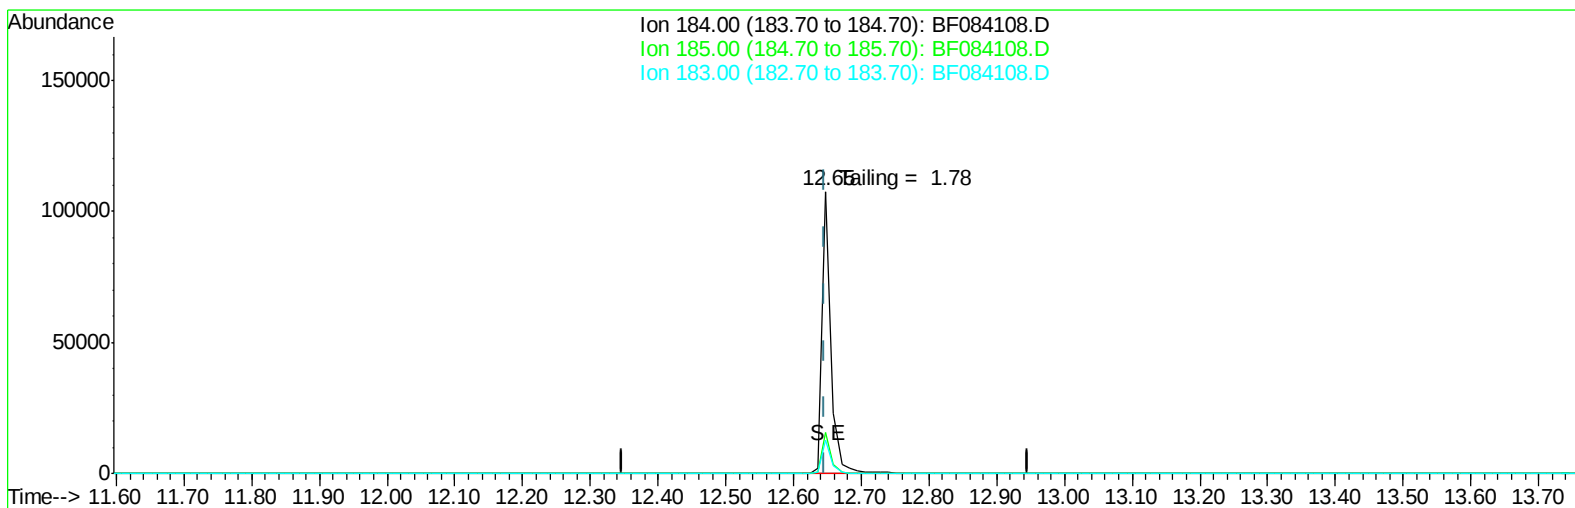

TIC: BF084108.D

(76) Benzidine

12.648min (+0.001) 2661.45ng

response 96518

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.76
183.00	12.30	11.87
0.00	0.00	0.00