

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122415\
 Data File : BF084083.D
 Acq On : 24 Dec 2015 17:07
 Operator : UM/SJ
 Sample : PB87523BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB87523BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.979	251	253	256	rBV	281291	405703	27.89%	4.179%
2	5.424	290	292	302	rBB	595849	674692	46.38%	6.949%
3	6.453	380	382	384	rBV	540459	688668	47.34%	7.093%
4	6.567	390	392	395	rBV	822927	729198	50.12%	7.510%
5	6.796	410	412	415	rBV	320431	267906	18.41%	2.759%
6	6.956	424	426	428	rBV	880472	904004	62.14%	9.311%
7	7.356	459	461	464	rBV	473218	637391	43.81%	6.565%
8	8.088	522	525	527	rBV	255152	349569	24.03%	3.600%
9	9.162	616	619	621	rBV	1381539	1454857	100.00%	14.984%
10	9.836	675	678	680	rBV	434704	409353	28.14%	4.216%
11	10.625	744	747	749	rBV	510420	549988	37.80%	5.665%
12	11.322	806	808	810	rBV	336022	424355	29.17%	4.371%
13	12.522	911	913	918	rBB	31791	41861	2.88%	0.431%
14	12.728	929	931	932	rBV	37173	33057	2.27%	0.340%
15	12.751	932	933	936	rVB	21864	27254	1.87%	0.281%
16	12.899	943	946	949	rBV	1478885	1378995	94.79%	14.203%
17	13.425	991	992	995	rVB	16230	24489	1.68%	0.252%
18	13.814	1022	1026	1029	rVB	20321	33307	2.29%	0.343%
19	13.951	1036	1038	1041	rBV	385435	401766	27.62%	4.138%
20	15.380	1161	1163	1169	rVB	158268	249394	17.14%	2.569%
21	15.791	1195	1199	1207	rBV2	7697	23313	1.60%	0.240%


Sum of corrected areas: 9709120

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122415\
Data File : BF084083.D
Acq On : 24 Dec 2015 17:07
Operator : UM/SJ
Sample : PB87523BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87523BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

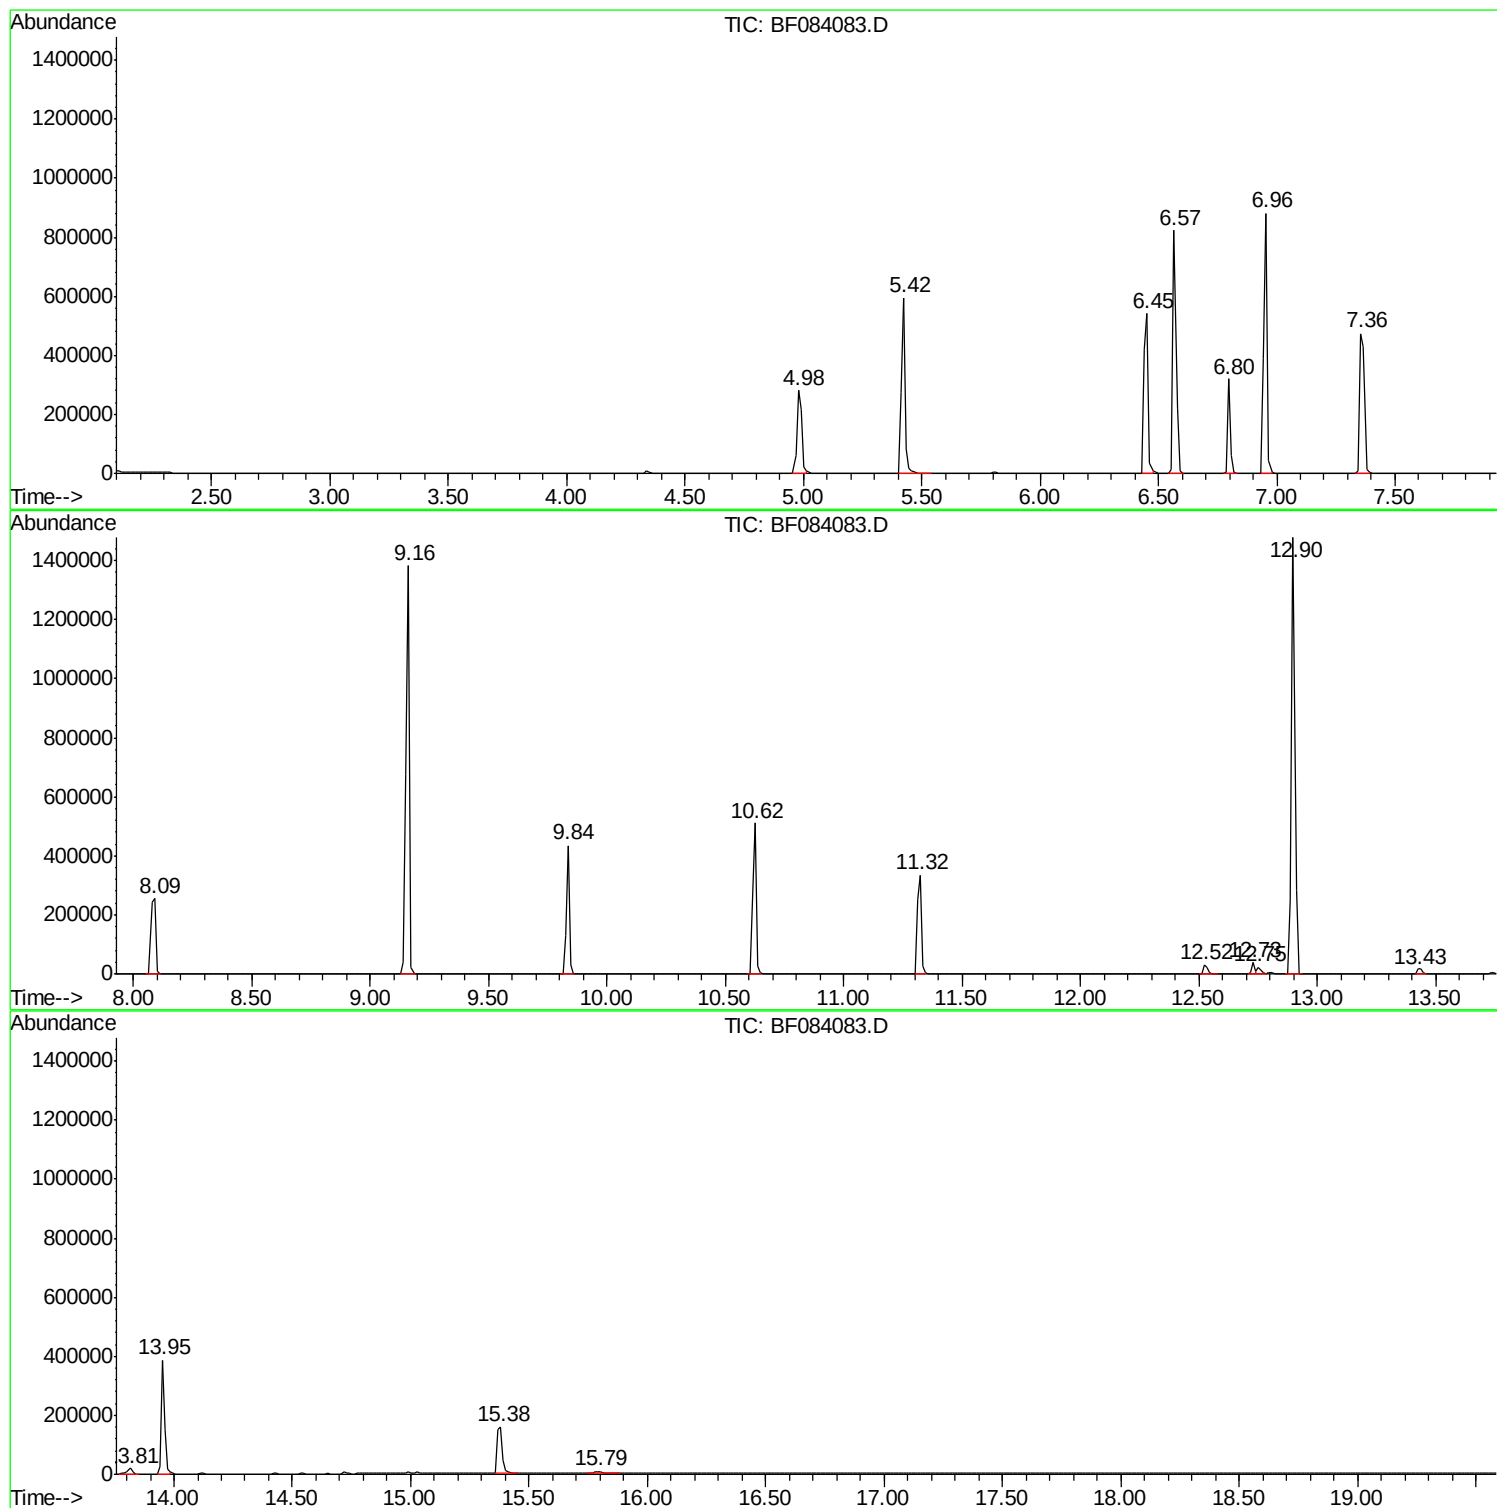

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122415\
Data File : BF084083.D
Acq On : 24 Dec 2015 17:07
Operator : UM/SJ
Sample : PB87523BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87523BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.98	30.29 ng	405703	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	43
3		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
4		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

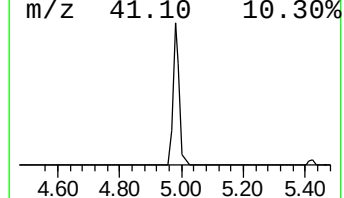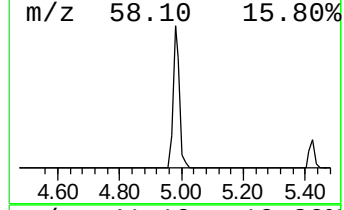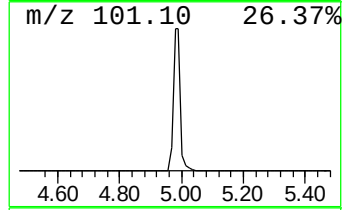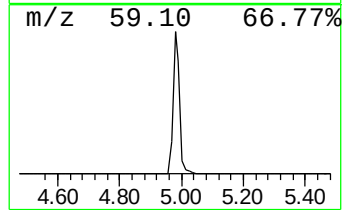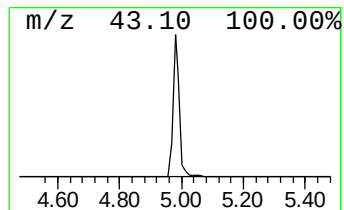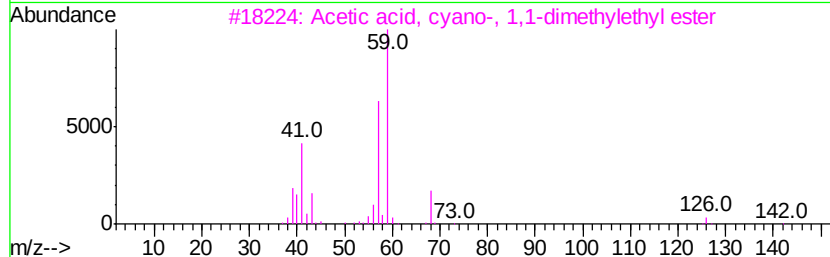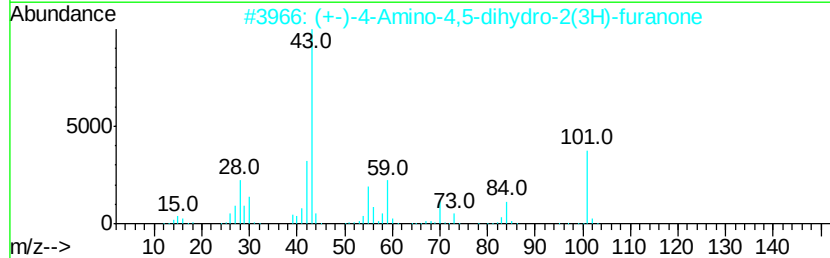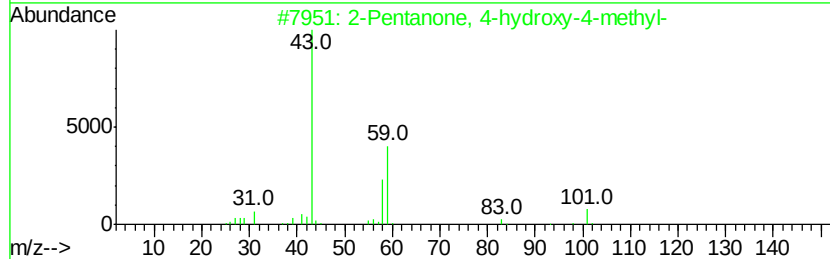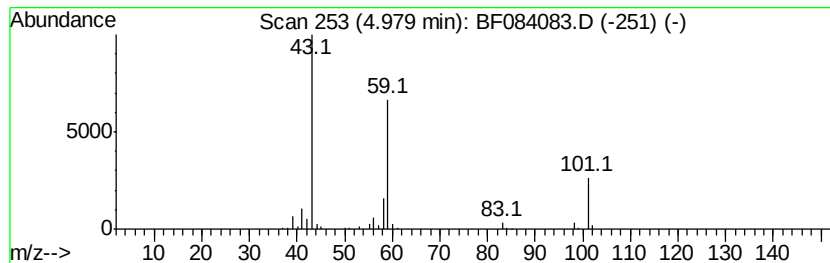

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122415\
Data File : BF084083.D
Acq On : 24 Dec 2015 17:07
Operator : UM/SJ
Sample : PB87523BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87523BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.57 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	54.44 ng	729198	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	14
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

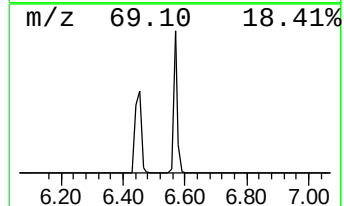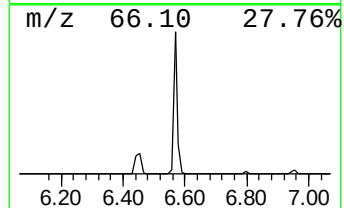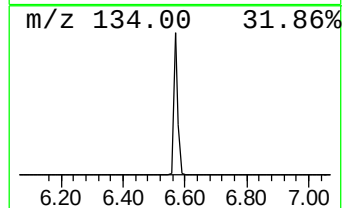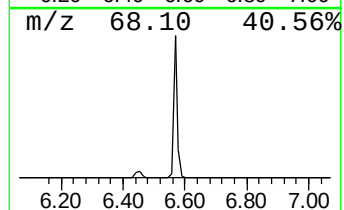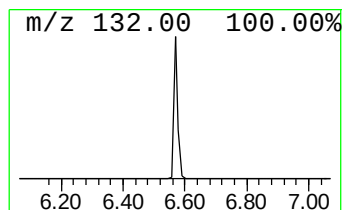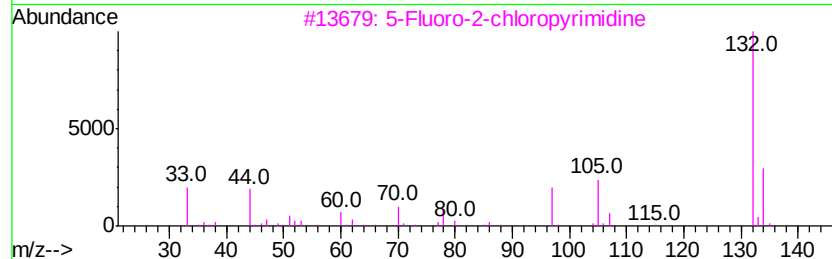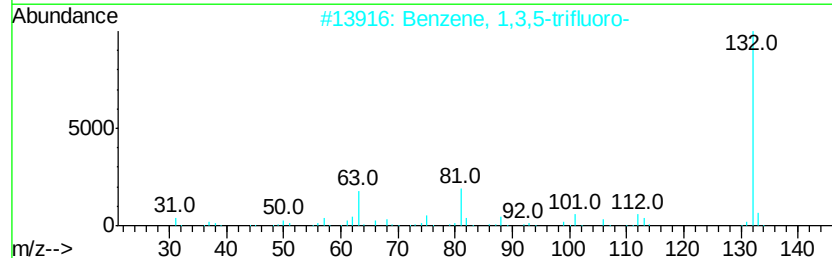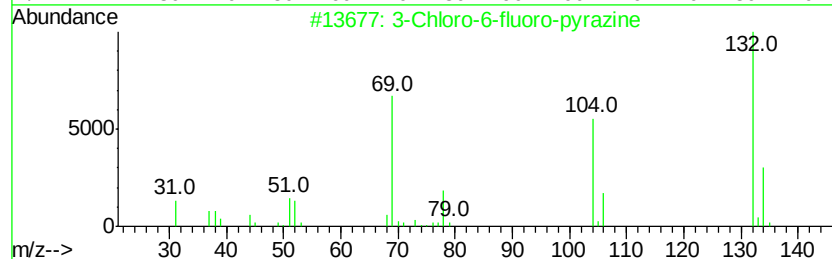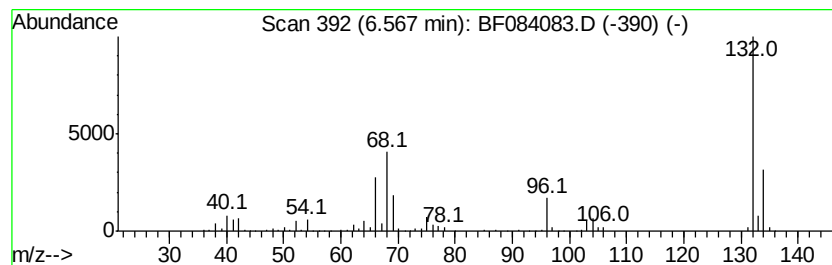

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122415\
Data File : BF084083.D
Acq On : 24 Dec 2015 17:07
Operator : UM/SJ
Sample : PB87523BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB87523BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.98	30.3	ng	405703	1	6.80	267906	20.0
unknown6.57	6.57	54.4	ng	729198	1	6.80	267906	20.0