


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122415\
 Data File : BF084073.D
 Acq On : 24 Dec 2015 12:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 24 16:48:39 2015

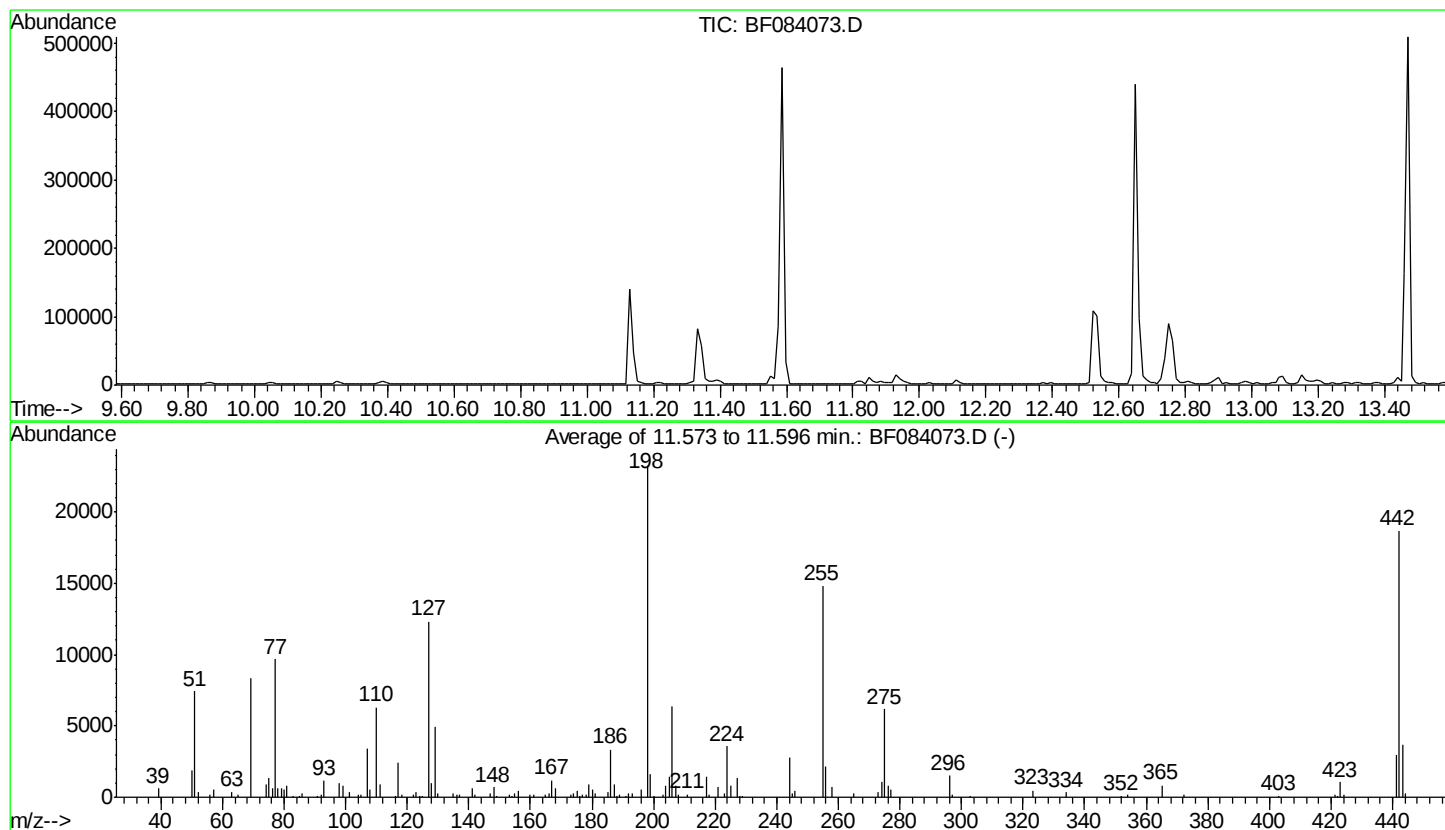

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	7434	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.9	8353	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	12320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23246	PASS
199	198	5	9	6.9	1599	PASS
275	198	10	60	26.6	6186	PASS
365	198	1	100	3.6	841	PASS
441	442	0.01	24	15.8	2950	PASS
442	198	50	100	80.4	18694	PASS
443	442	15	24	19.5	3647	PASS