


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122415\
 Data File : BF084084.D
 Acq On : 24 Dec 2015 17:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 24 16:48:39 2015

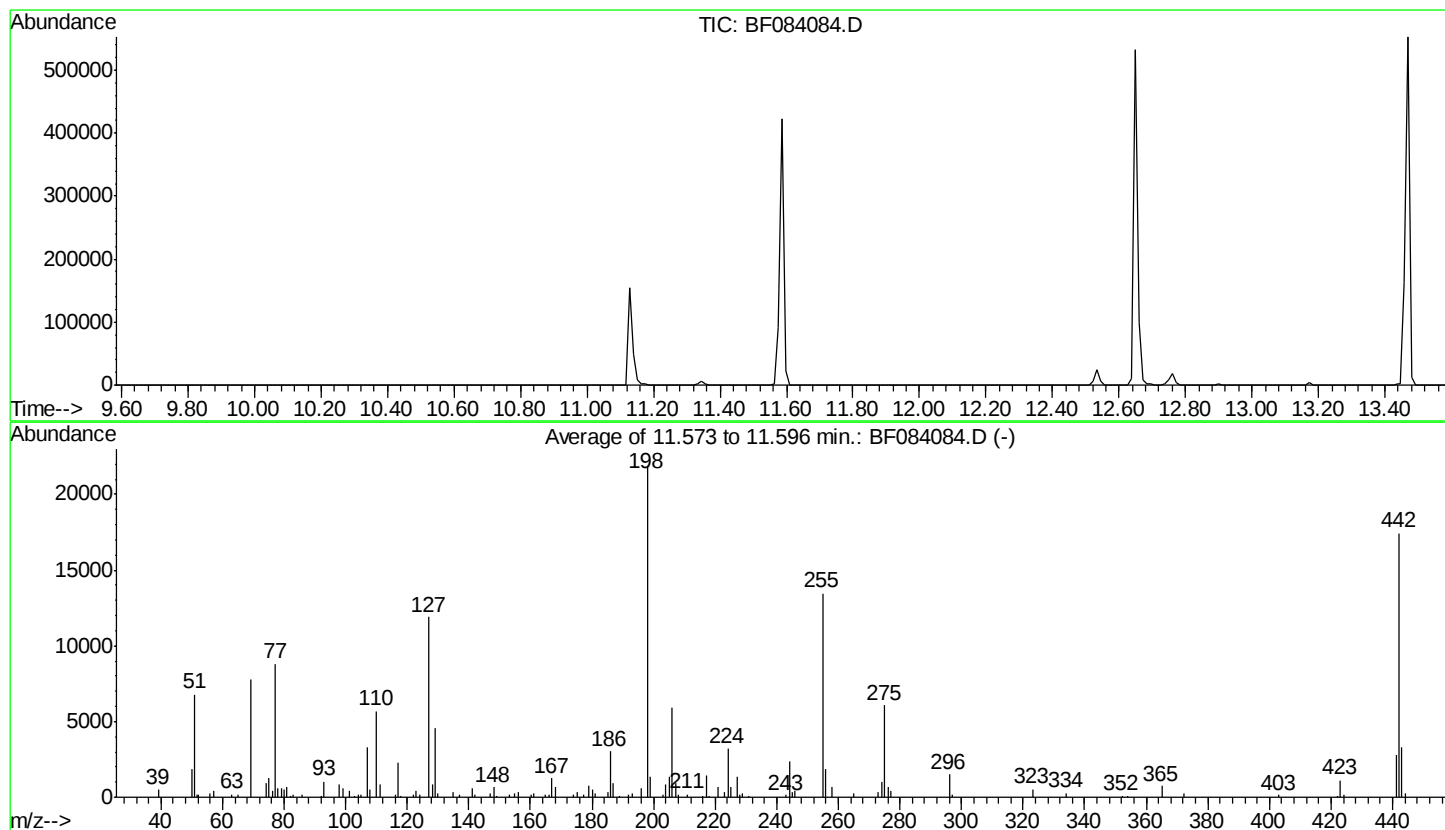

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	6764	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	7746	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	11881	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21899	PASS
199	198	5	9	6.3	1384	PASS
275	198	10	60	27.7	6071	PASS
365	198	1	100	3.4	738	PASS
441	442	0.01	24	16.0	2792	PASS
442	198	50	100	79.7	17448	PASS
443	442	15	24	18.9	3297	PASS