



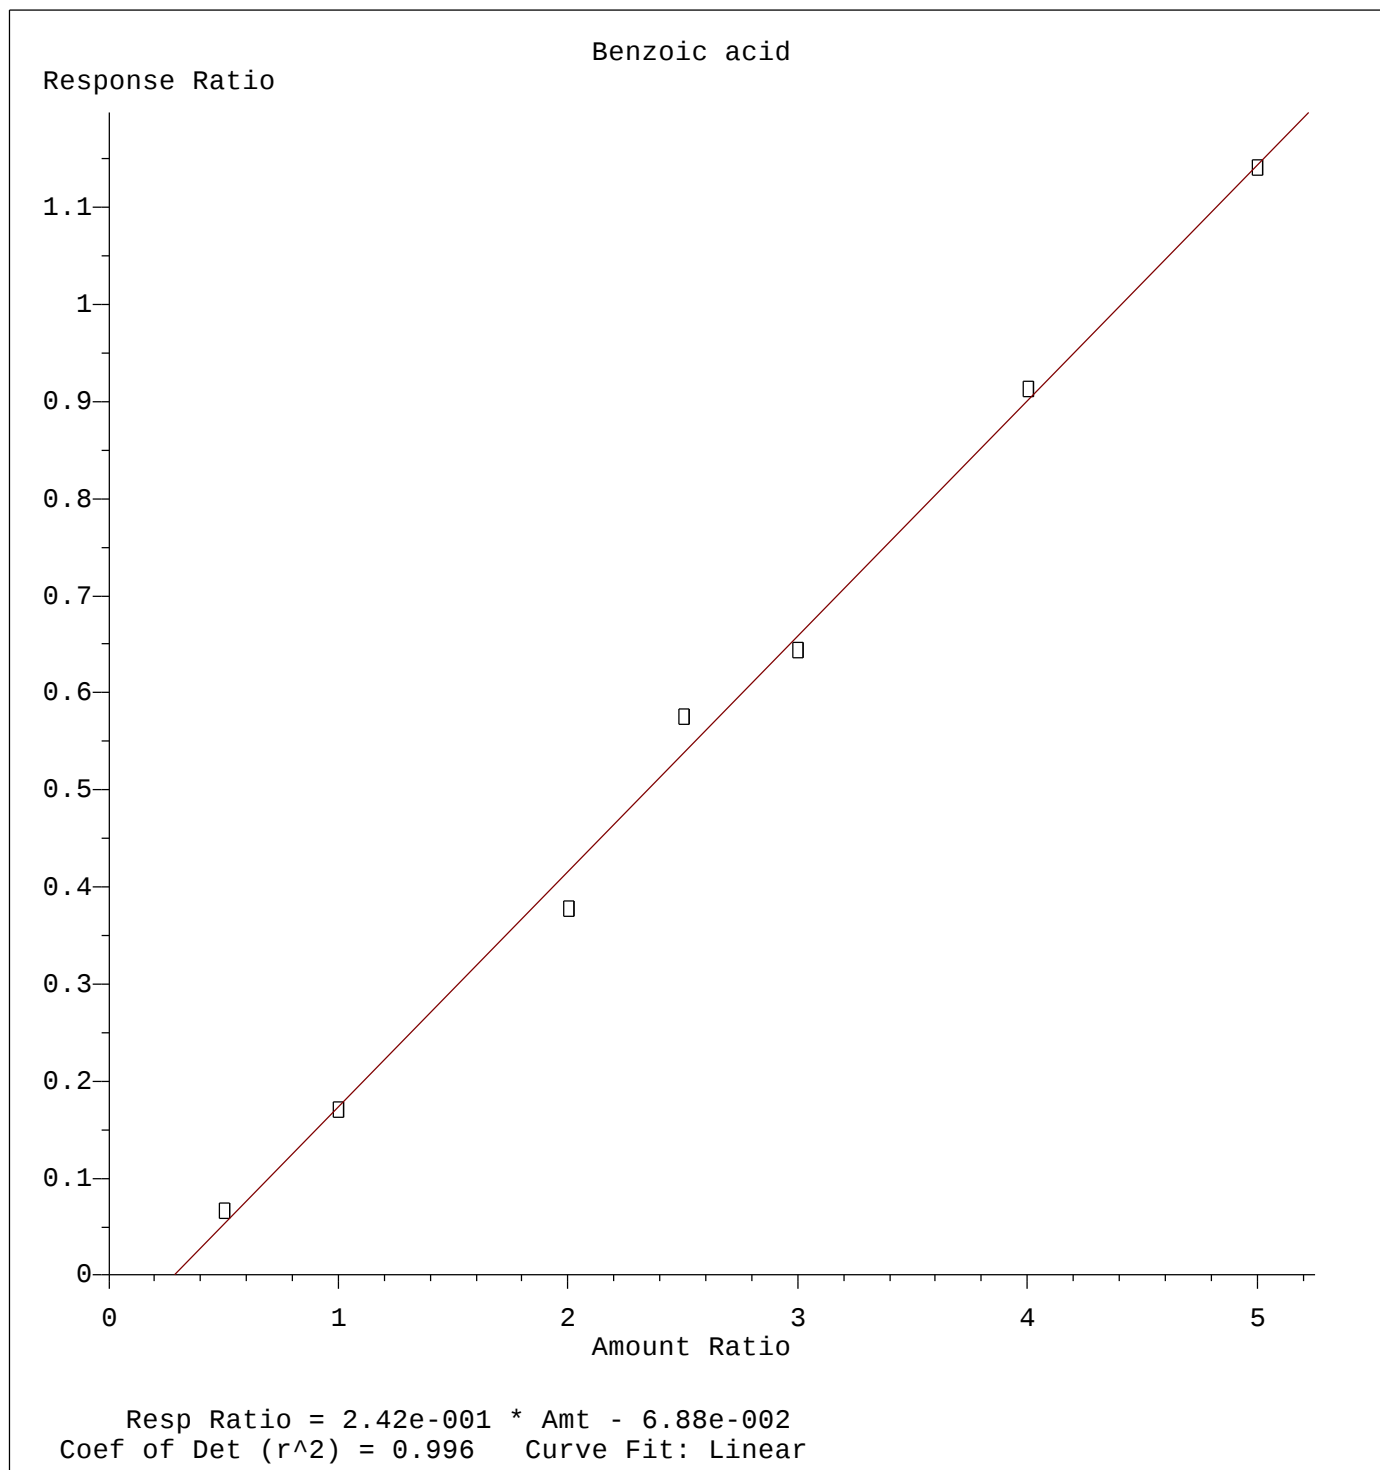

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
Calibration Table Last Updated: Tue Dec 24 15:58:52 2019

Hexachlorocyclopentadiene

Response Ratio

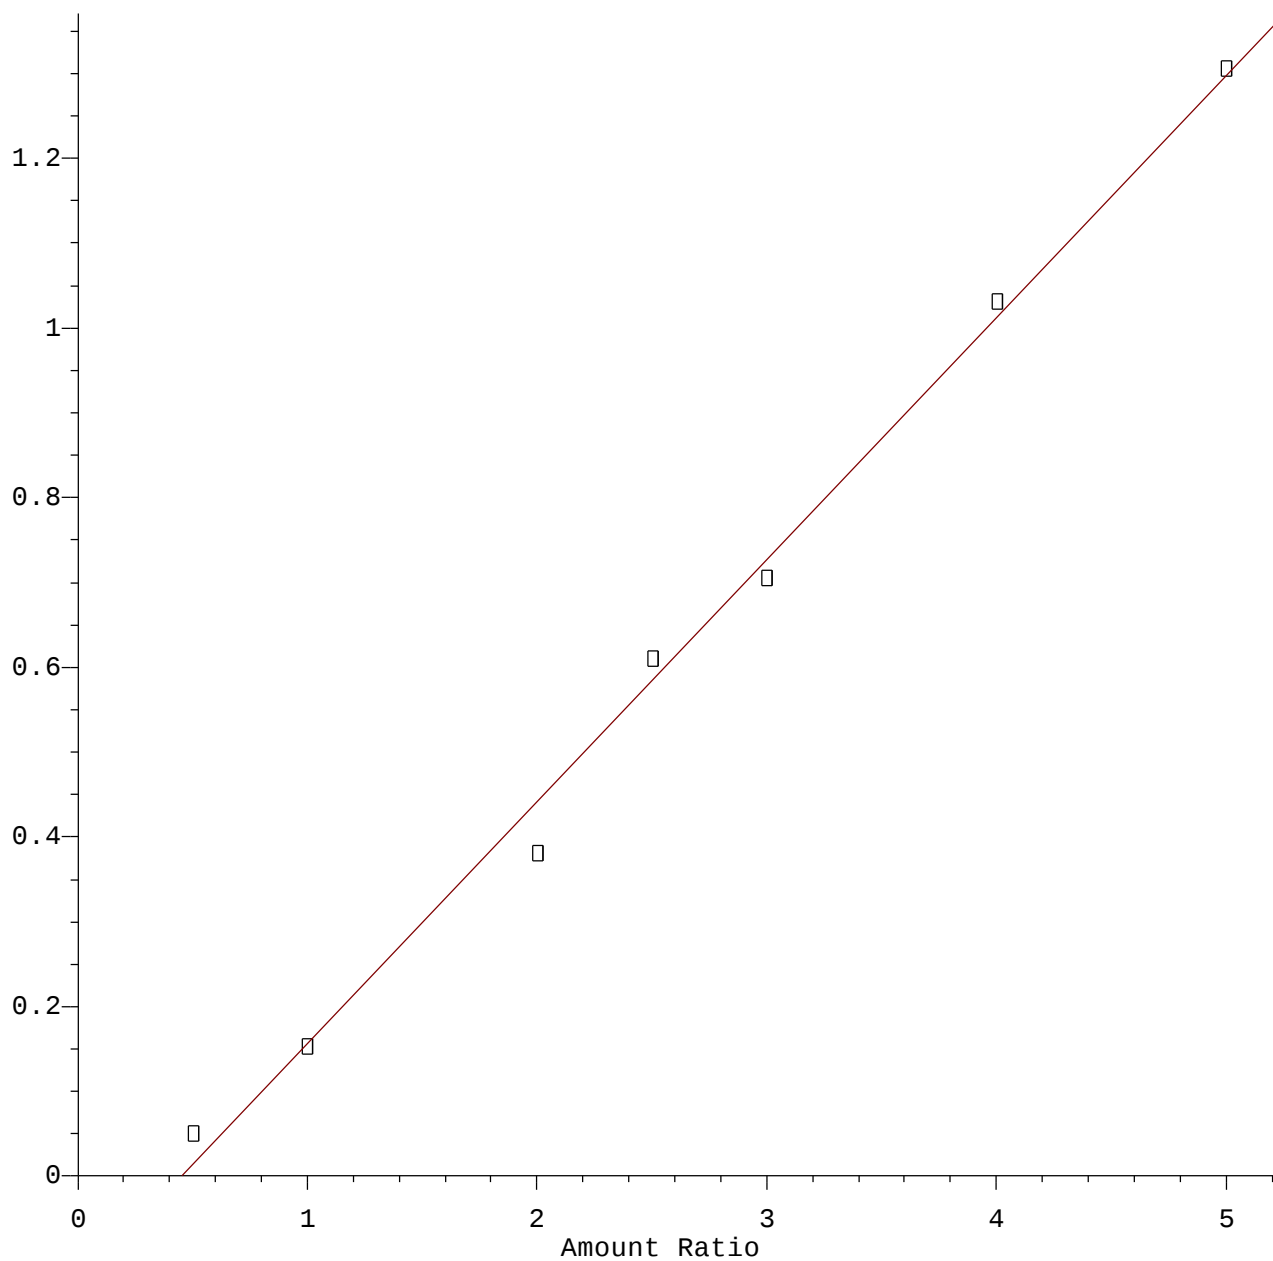


Resp Ratio = $2.85 \times 10^{-1} \times \text{Amt} - 1.29 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
Calibration Table Last Updated: Tue Dec 24 15:58:52 2019

2,4-Dinitrophenol

Response Ratio

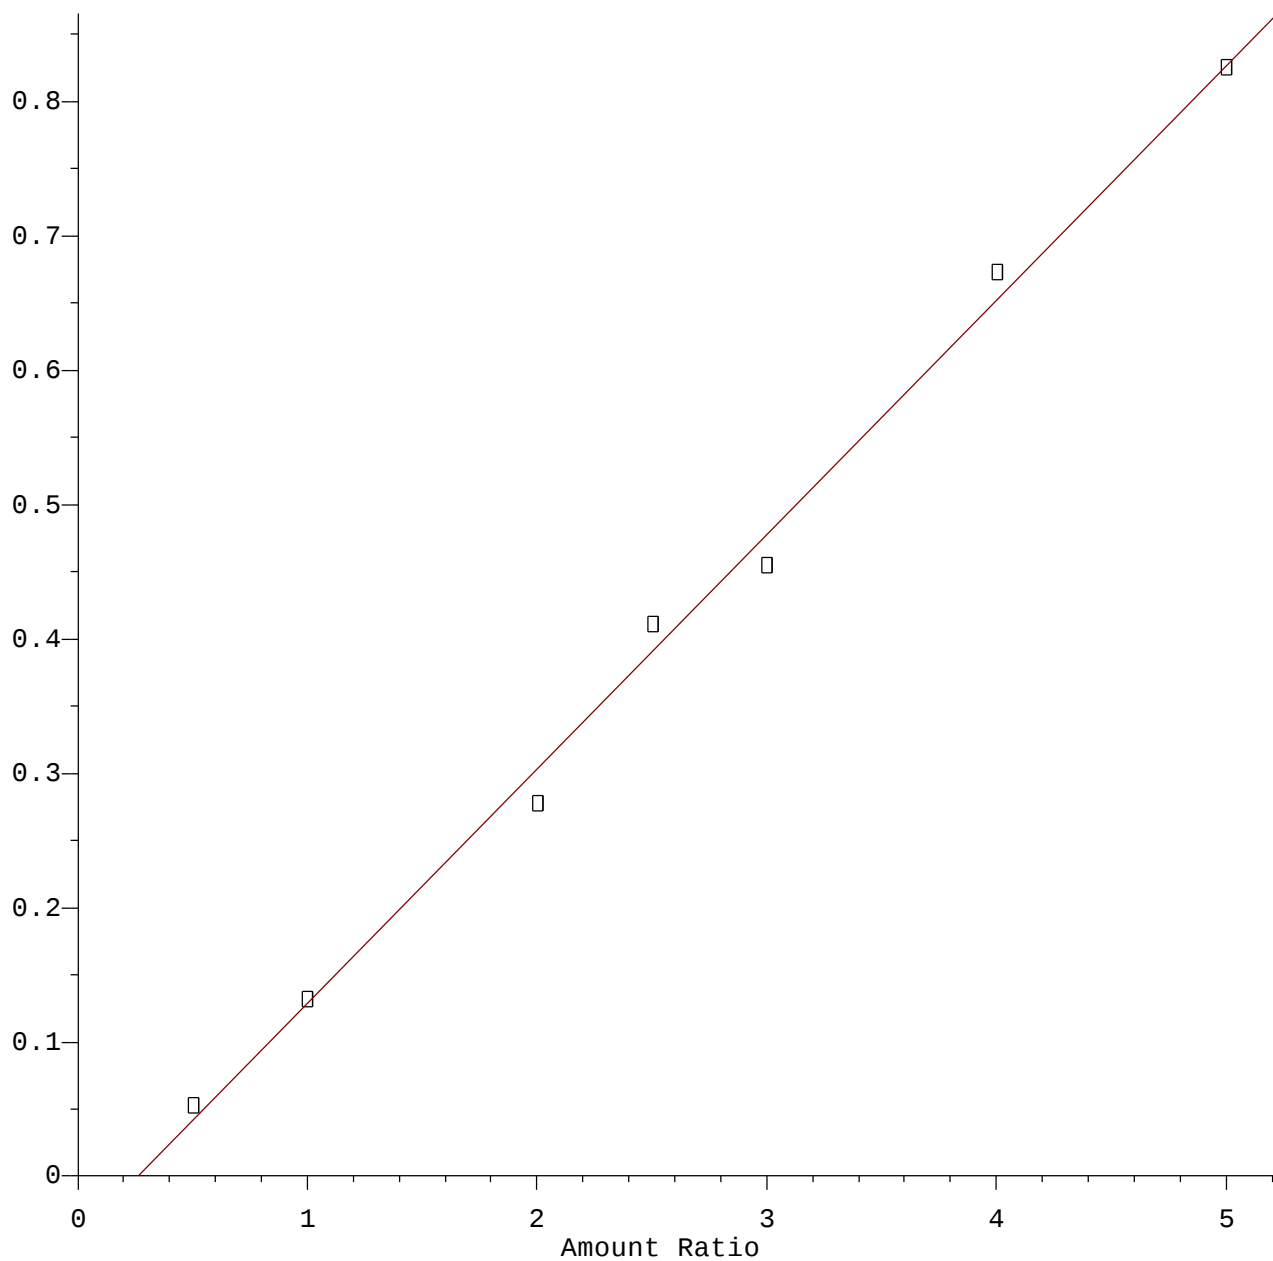

Resp Ratio = $1.75 \times 10^{-1} \times \text{Amt} - 4.52 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
Calibration Table Last Updated: Tue Dec 24 15:58:52 2019