


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122419\
 Data File : BF118299.D
 Acq On : 24 Dec 2019 10:33
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

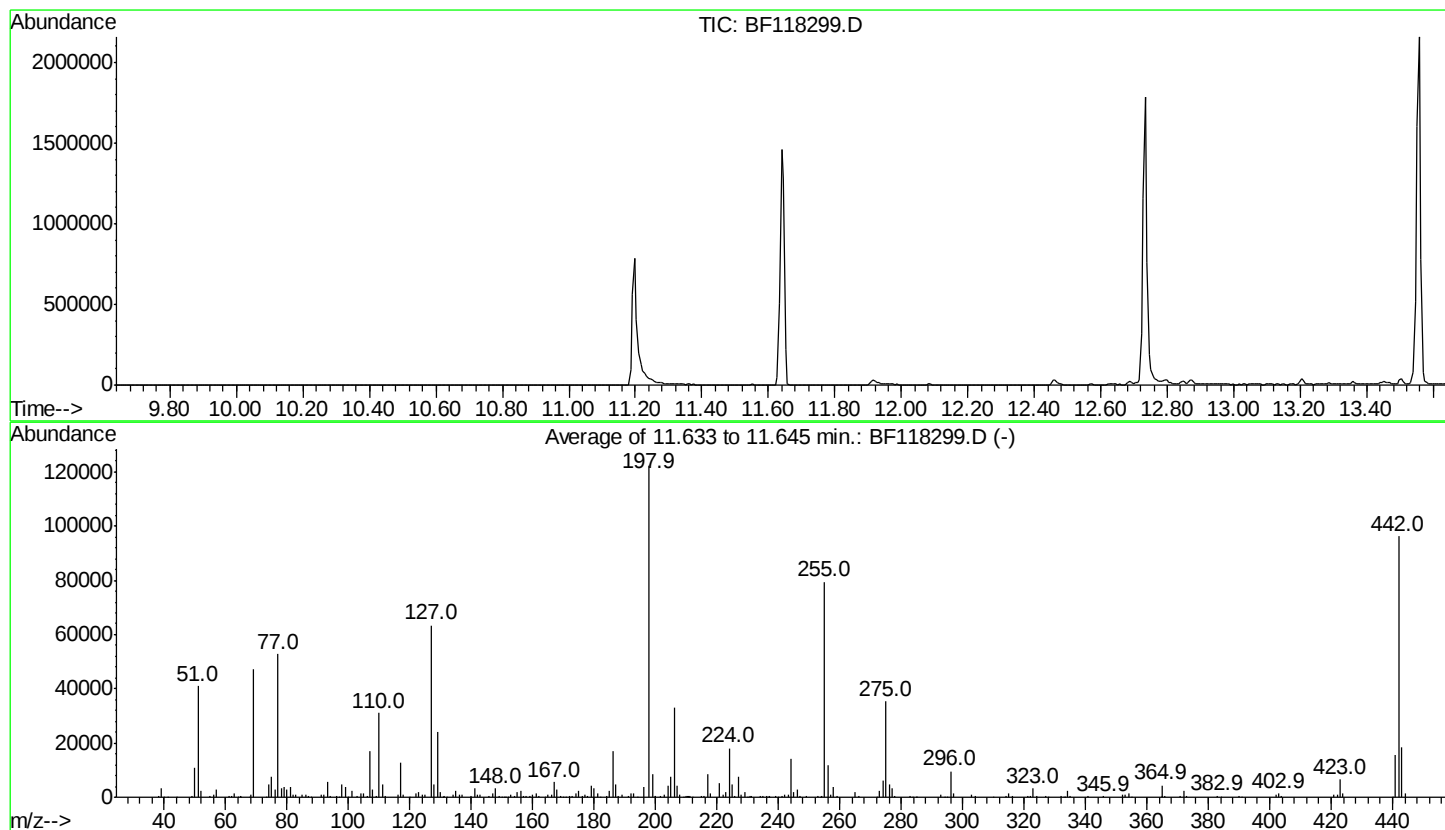

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	40925	PASS
68	69	0.00	2	1.6	770	PASS
69	198	0.00	100	38.5	47026	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	63429	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	122293	PASS
199	198	5	9	6.8	8324	PASS
275	198	10	60	28.9	35339	PASS
365	198	1	100	3.7	4497	PASS
441	198	0.01	100	12.8	15638	PASS
442	198	50	100	78.6	96104	PASS
443	442	15	24	19.0	18224	PASS