
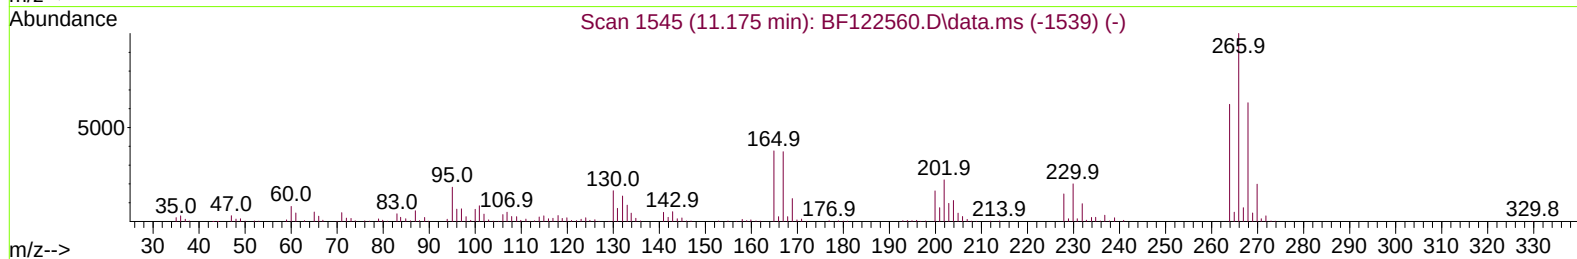
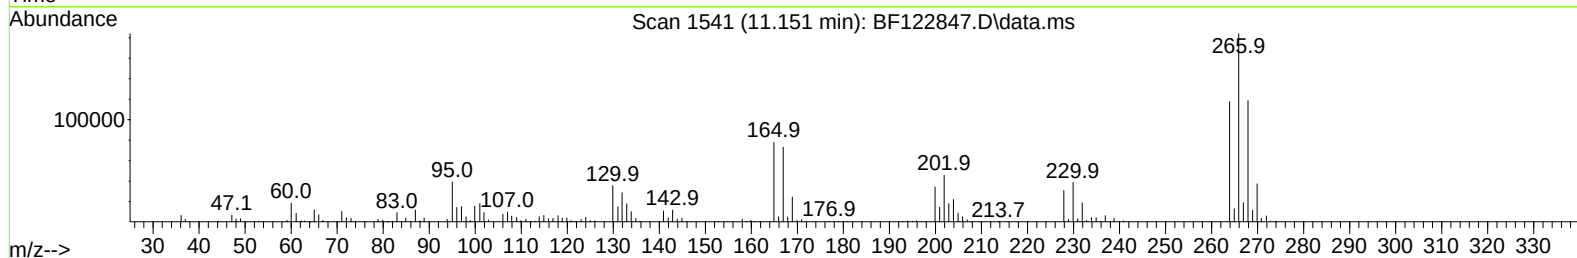


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122420\
Data File : BF122847.D
Acq On : 24 Dec 2020 9:07
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 02:31:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

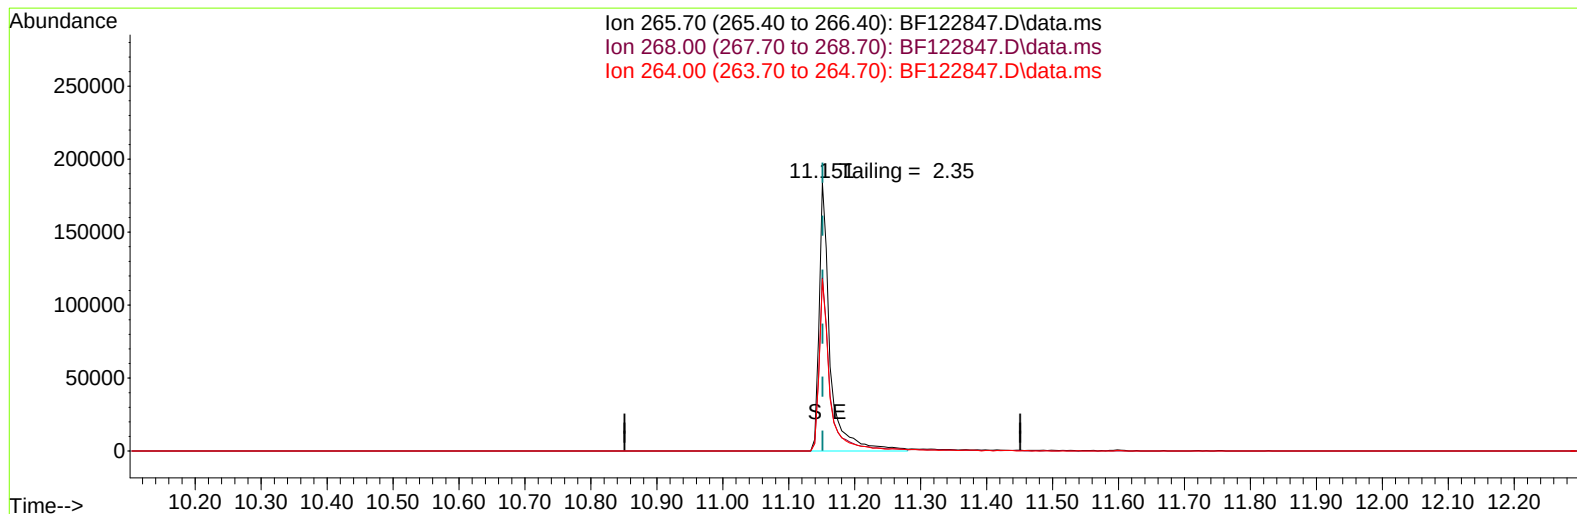

TIC: BF122847.D\data.ms

(70) Pentachlorophenol (C)




11.151min (-0.000) 37912.02 ng

response 216044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.47
264.00	62.30	63.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122420\
Data File : BF122847.D
Acq On : 24 Dec 2020 9:07
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 02:31:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

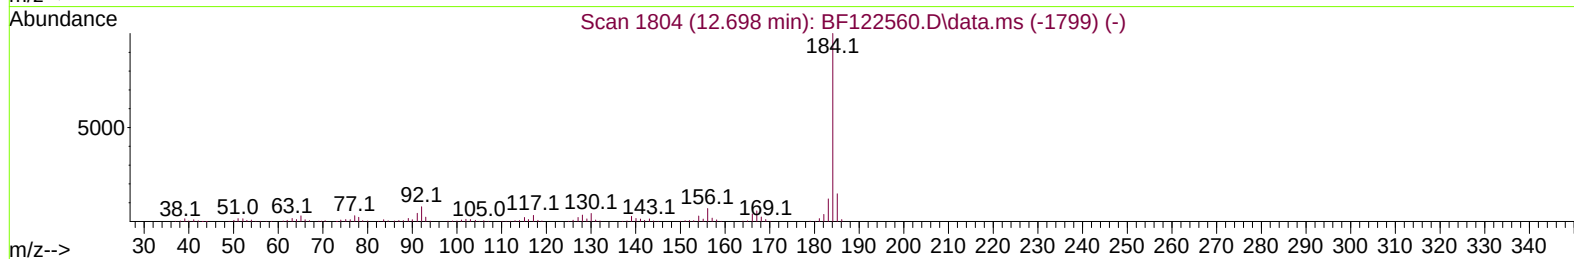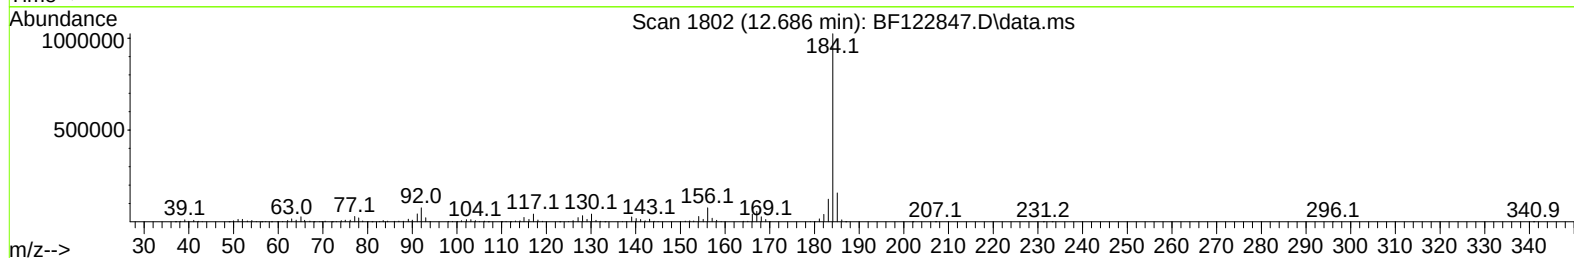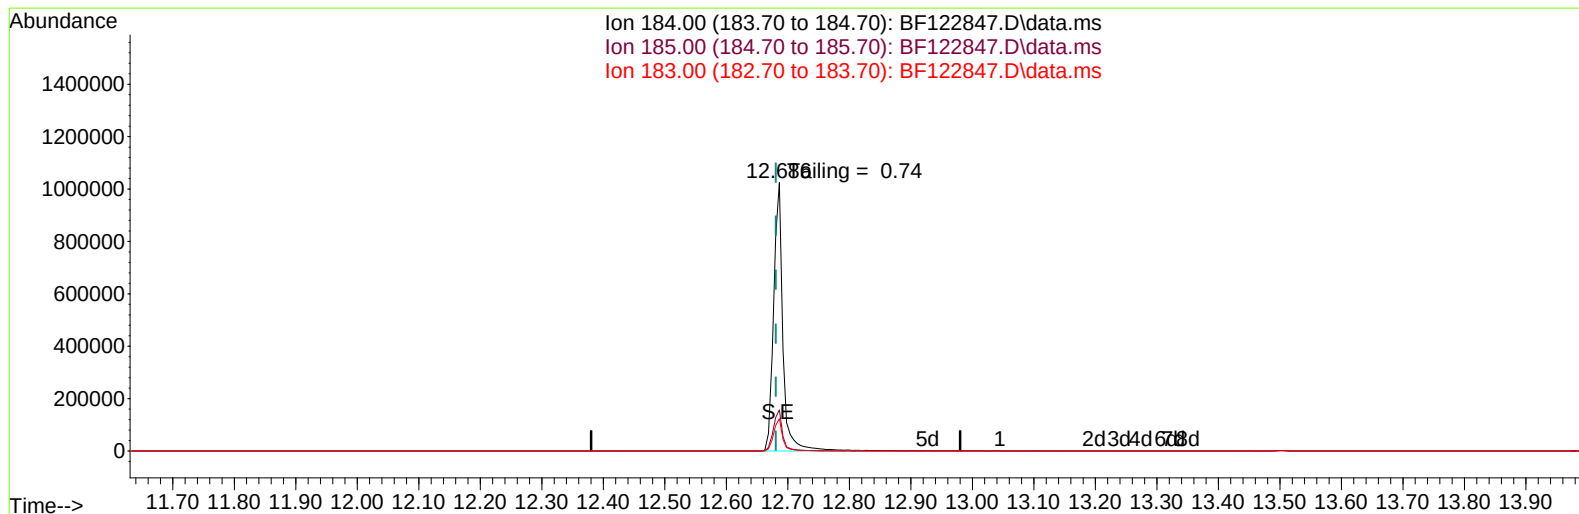

TIC: BF122847.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 467533.05 ng m

response 1082068

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.31
183.00	12.10	12.07
0.00	0.00	0.00