
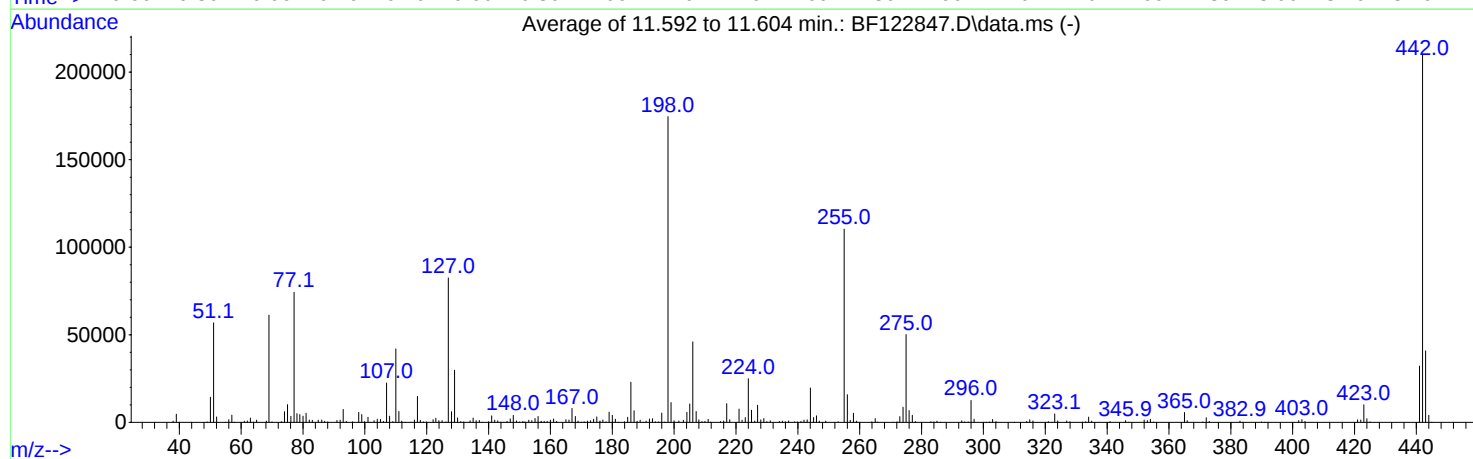


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122420\
 Data File : BF122847.D
 Acq On : 24 Dec 2020 9:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

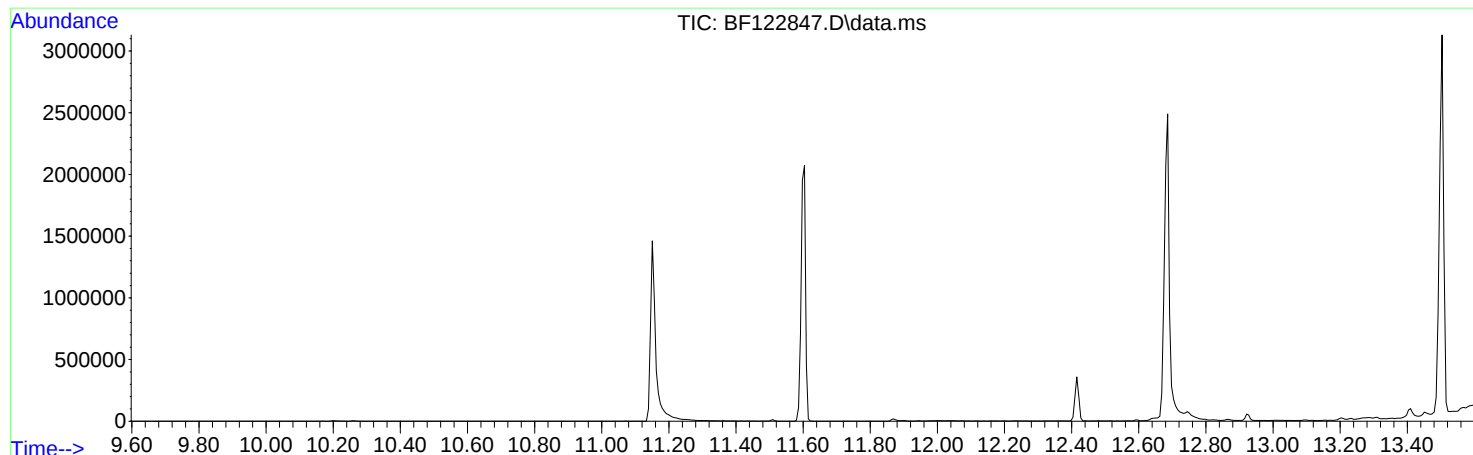

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	56824	PASS
68	69	0.00	2	1.1	699	PASS
69	198	0.00	100	35.0	61176	PASS
70	69	0.00	2	0.4	247	PASS
127	198	10	80	47.3	82512	PASS
197	198	0.00	2	0.1	225	PASS
198	198	100	100	100.0	174613	PASS
199	198	5	9	6.5	11324	PASS
275	198	10	60	28.7	50168	PASS
365	198	1	100	3.2	5653	PASS
441	198	0.01	100	18.4	32207	PASS
442	442	100	100	100.0	210043	PASS
443	442	15	24	19.5	40864	PASS