
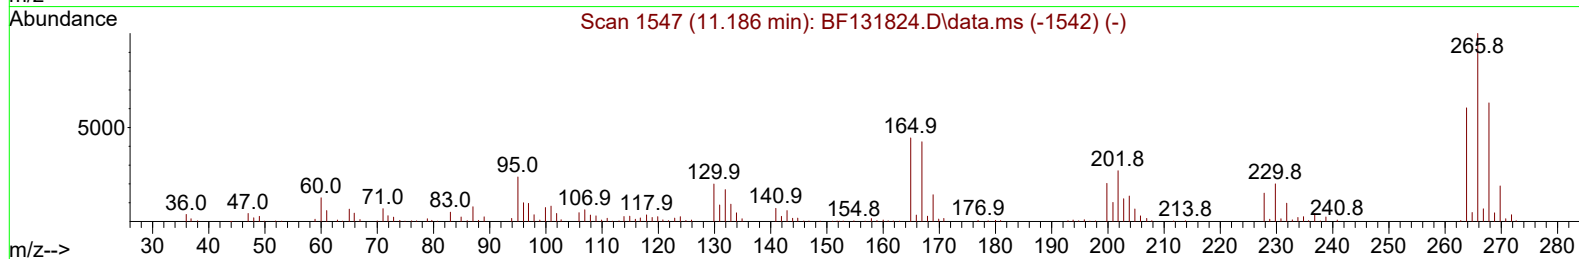
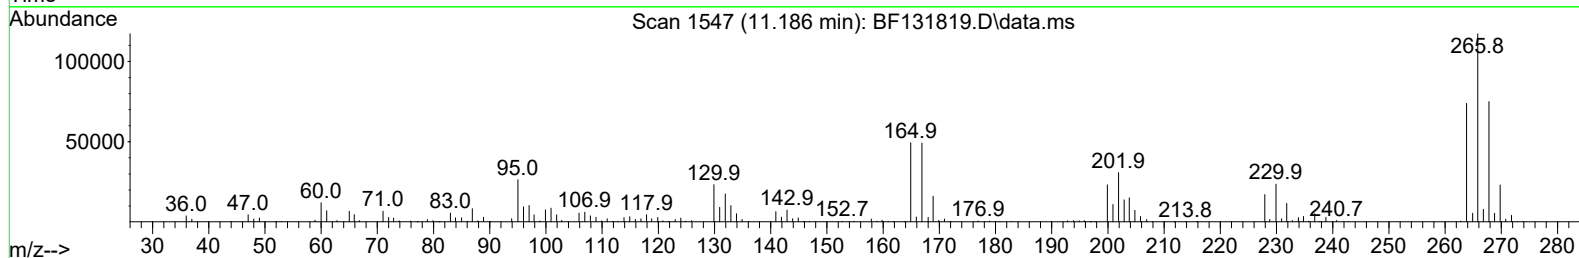


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122422\
Data File : BF131819.D
Acq On : 24 Dec 2022 11:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 05:57:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

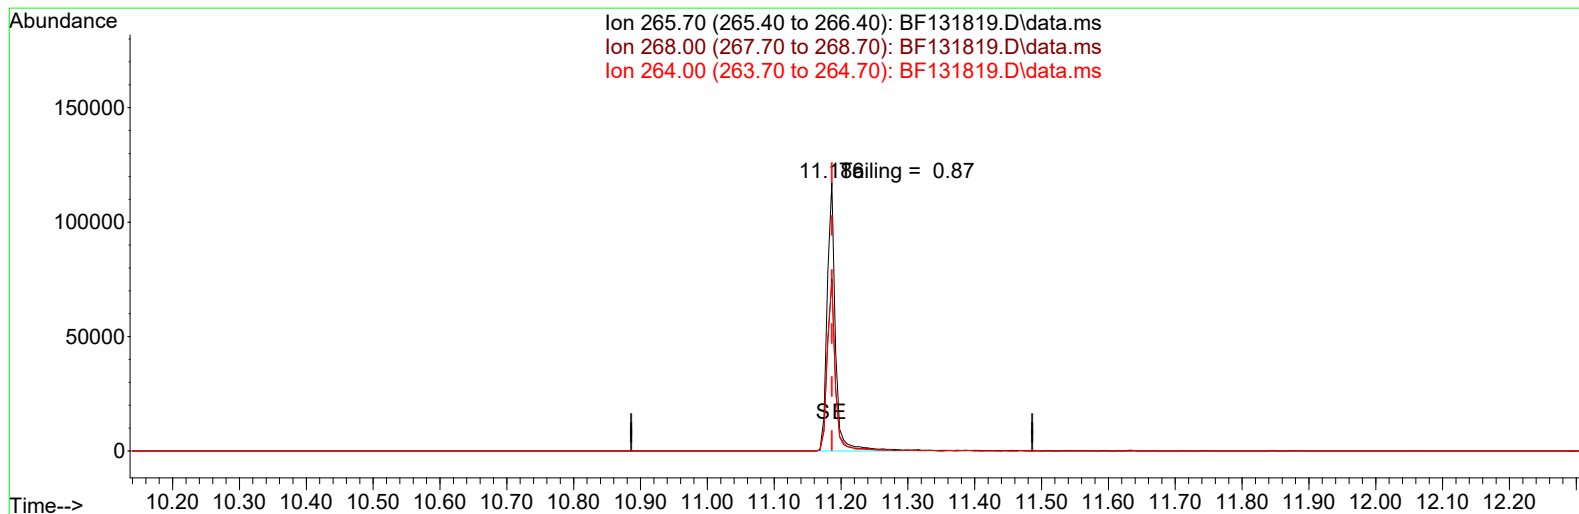

TIC: BF131819.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.000) 29547.12 ng

response 101637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.92
264.00	60.40	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122422\
Data File : BF131819.D
Acq On : 24 Dec 2022 11:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 05:57:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

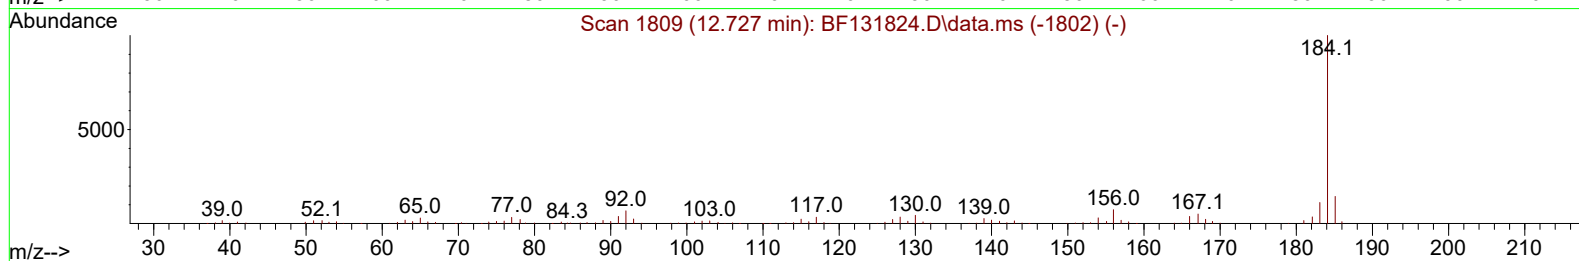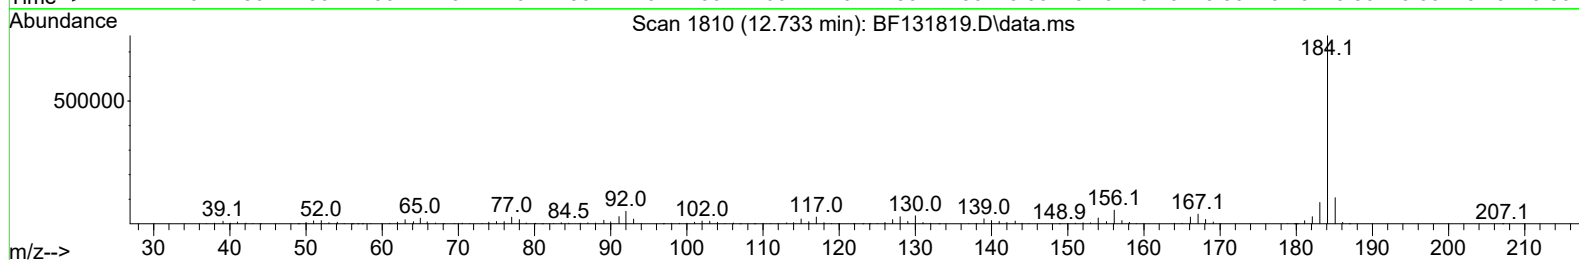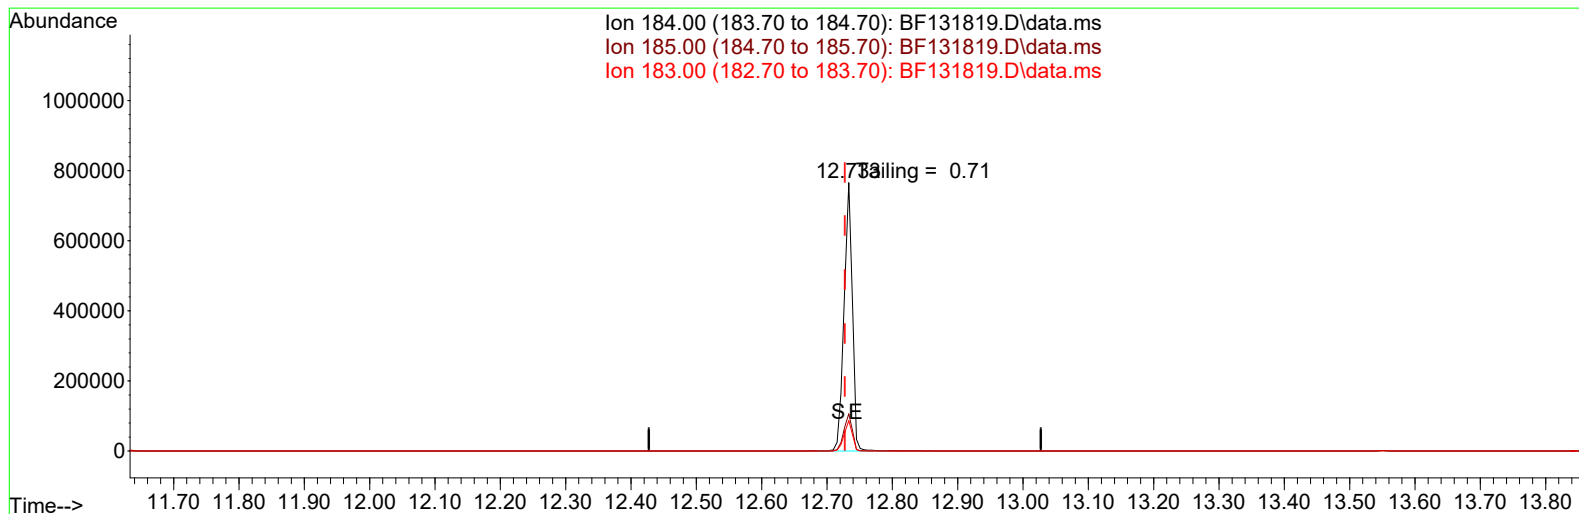

TIC: BF131819.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 673924

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.91
183.00	11.20	11.37
0.00	0.00	0.00