


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122422\
 Data File : BF131819.D
 Acq On : 24 Dec 2022 11:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 26 05:13:34 2022

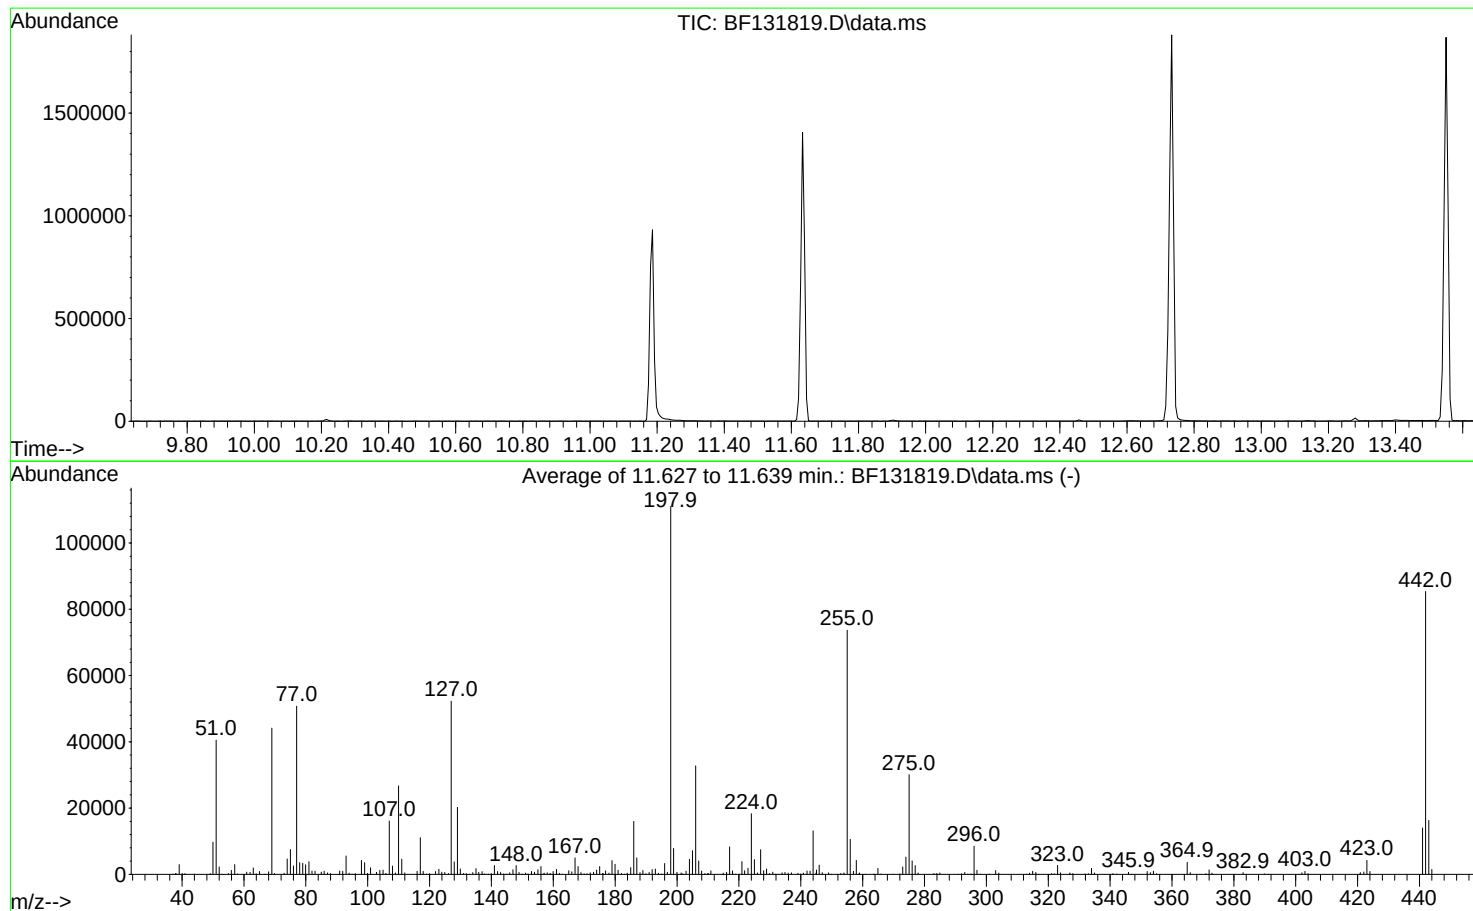




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	40517	PASS
68	69	0.00	2	1.7	757	PASS
69	198	0.00	100	39.8	44131	PASS
70	69	0.00	2	0.5	238	PASS
127	198	10	80	47.1	52240	PASS
197	198	0.00	2	0.6	637	PASS
198	198	100	100	100.0	111008	PASS
199	198	5	9	7.1	7830	PASS
275	198	10	60	27.1	30104	PASS
365	198	1	100	3.3	3637	PASS
441	198	0.01	100	12.6	14002	PASS
442	442	50	100	100.0	85389	PASS
443	442	15	24	19.1	16298	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122422\
Data File : BF131819.D
Acq On : 24 Dec 2022 11:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 26 05:57:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

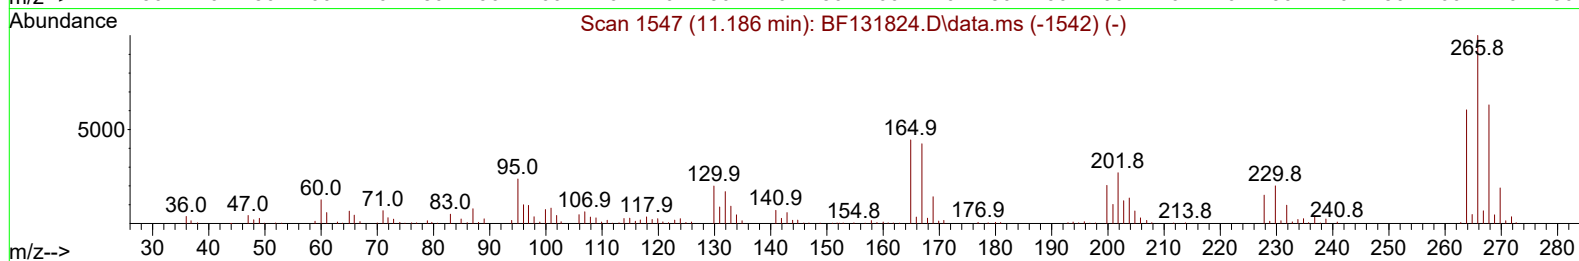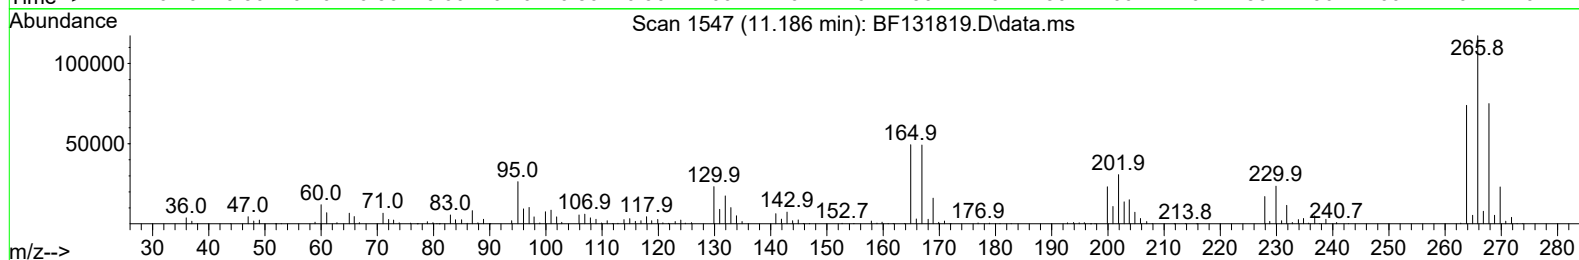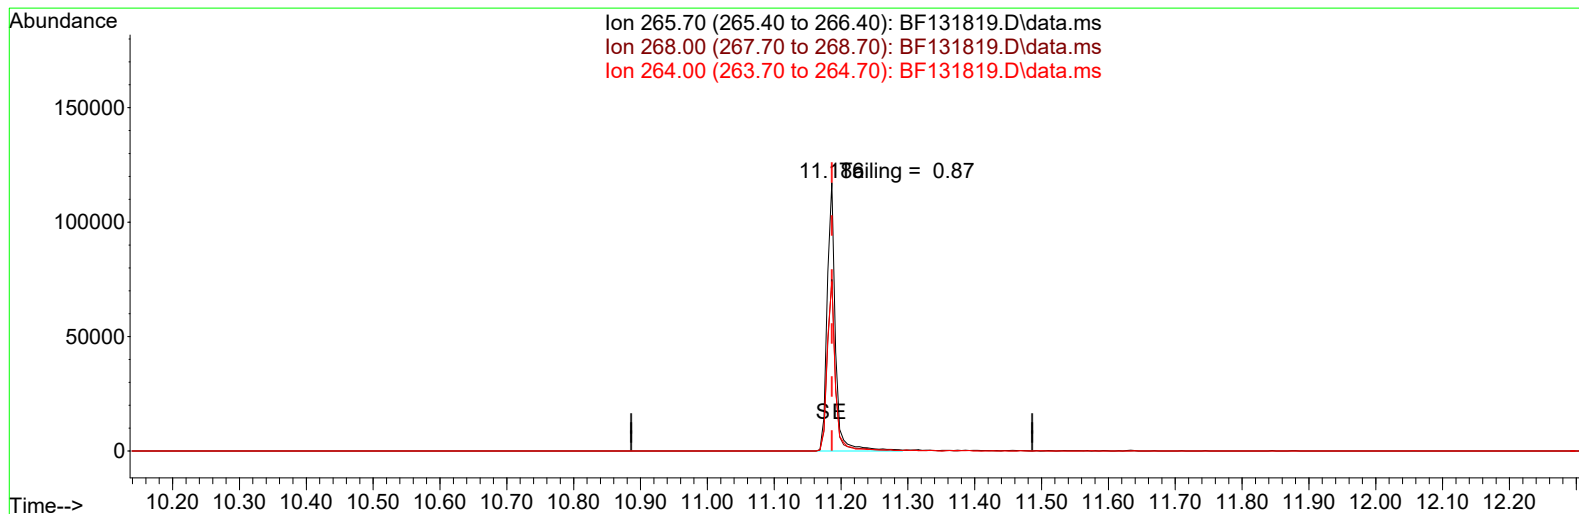

TIC: BF131819.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.000) 29547.12 ng




response 101637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.92
264.00	60.40	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122422\
Data File : BF131819.D
Acq On : 24 Dec 2022 11:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 26 05:57:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

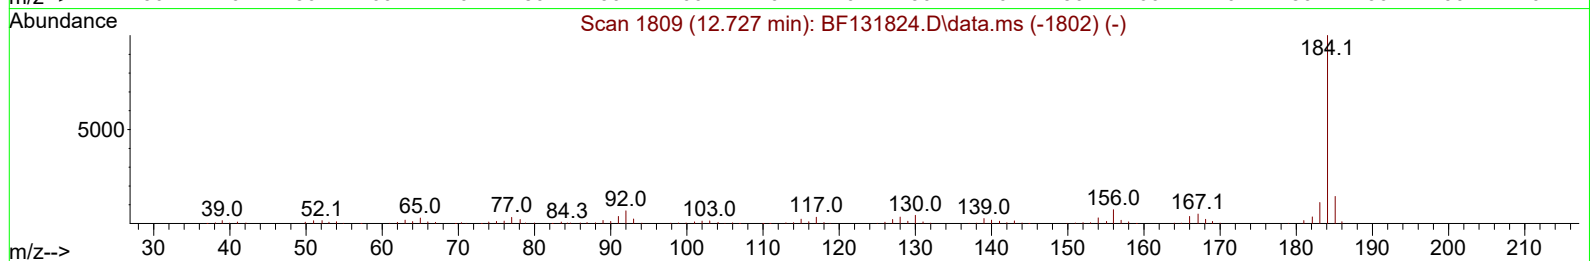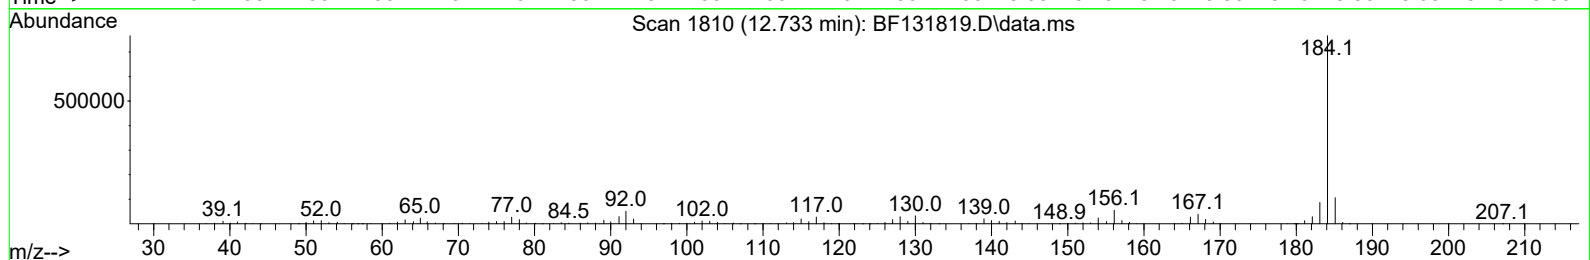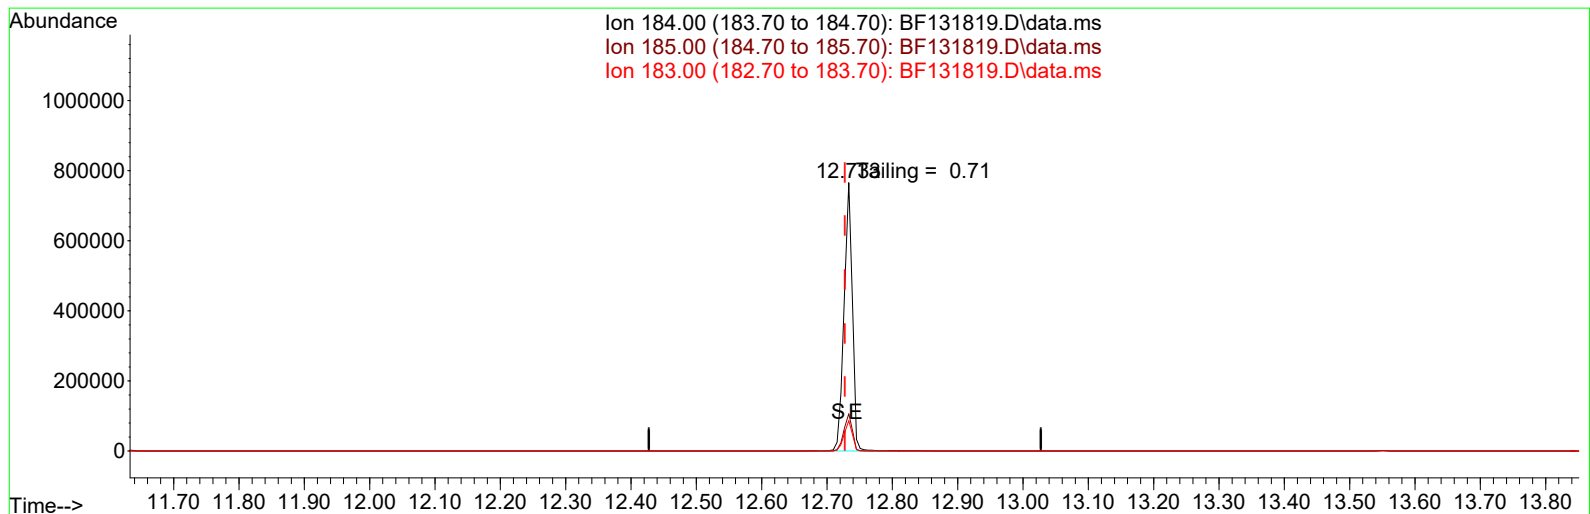

TIC: BF131819.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 673924

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.91
183.00	11.20	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/24/2022	BNA_F	<u>BF131819.D</u>
Compound Name	Response	Retention Time
DDT	304990	13.551
DDD	3306	13.28
DDE	64	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3370	308360	1.09

Instrument :
BNA_F
ClientSampleId :
DFTPP