
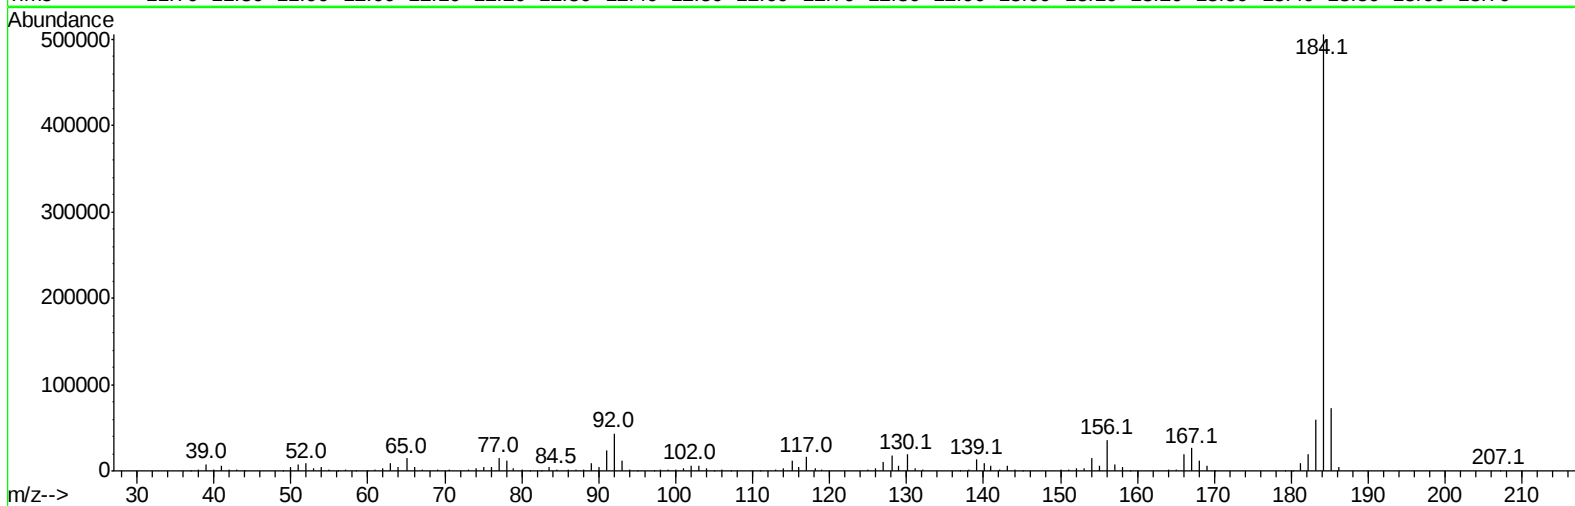


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122617\
Data File : BF101702.D
Acq On : 26 Dec 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 08:24:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

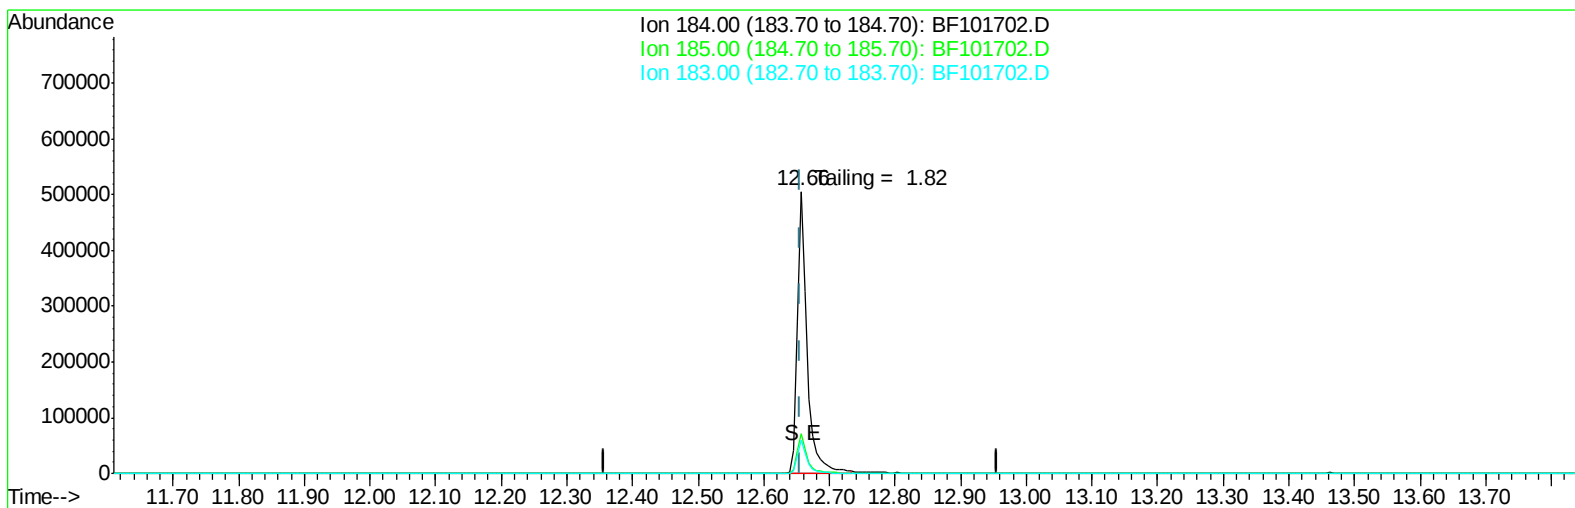

TIC: BF101702.D

(76) Benzidine


12.656min (-0.000) 0.00ng

response 533802

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.28
183.00	11.60	11.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122617\
Data File : BF101702.D
Acq On : 26 Dec 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 08:24:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

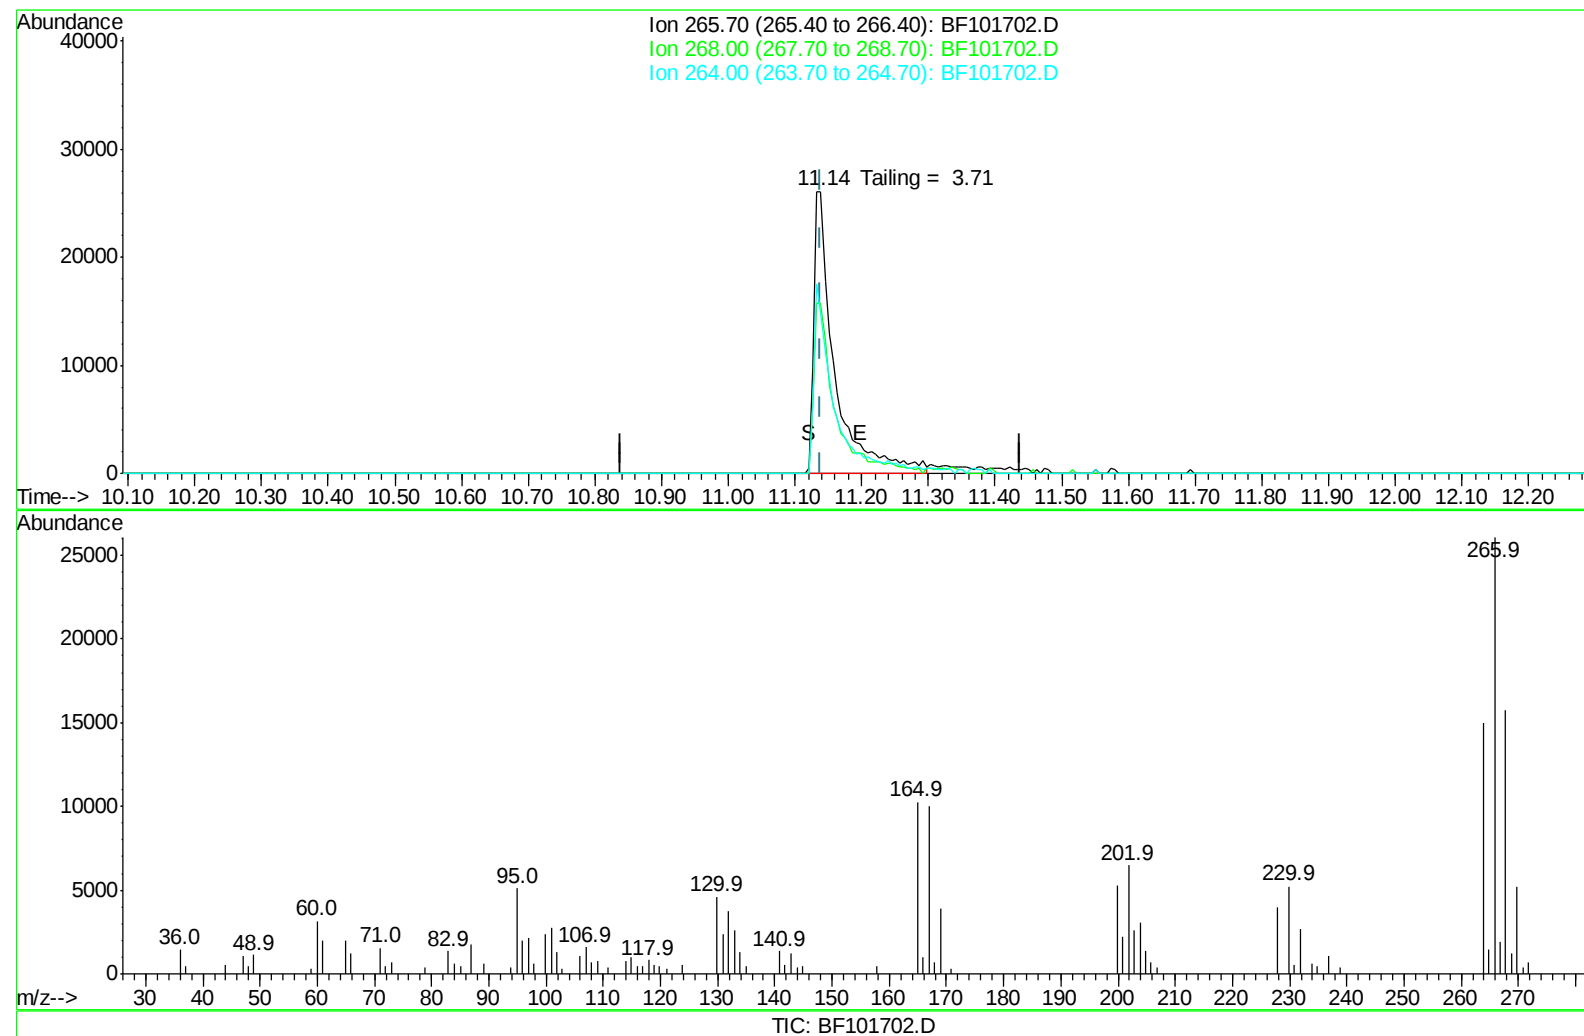

(69) Pentachlorophenol (C)

11.139min (-0.000) 27899.56ng

response 54377

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.37
264.00	61.90	57.45
0.00	0.00	0.00