
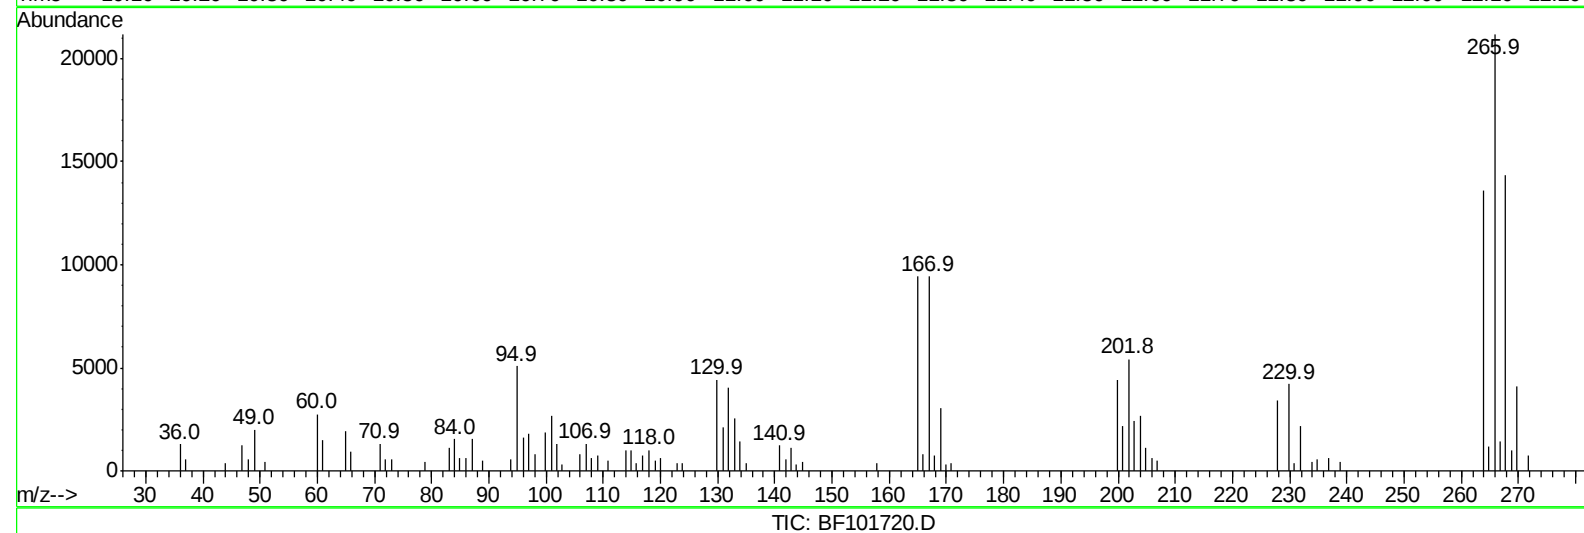


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122617\
Data File : BF101720.D
Acq On : 26 Dec 2017 17:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 08:25:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

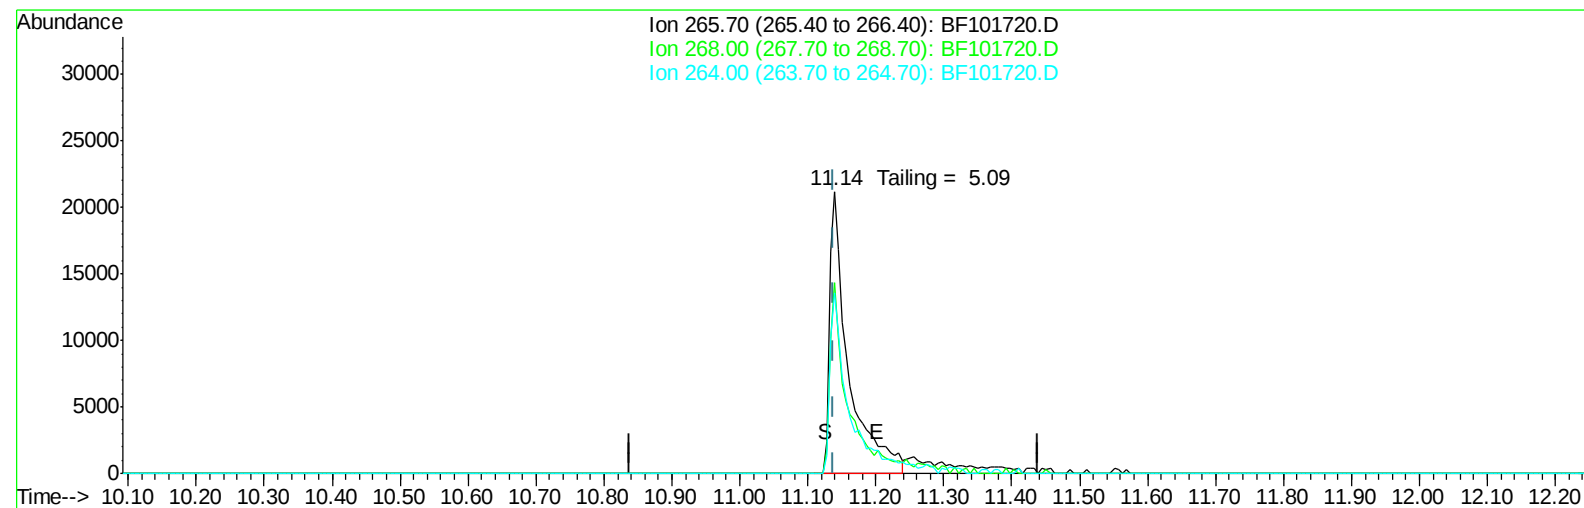

(69) Pentachlorophenol (C)



11.139min (-0.000) 47779.57ng

response 41633

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.63
264.00	61.90	64.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122617\
Data File : BF101720.D
Acq On : 26 Dec 2017 17:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 08:25:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

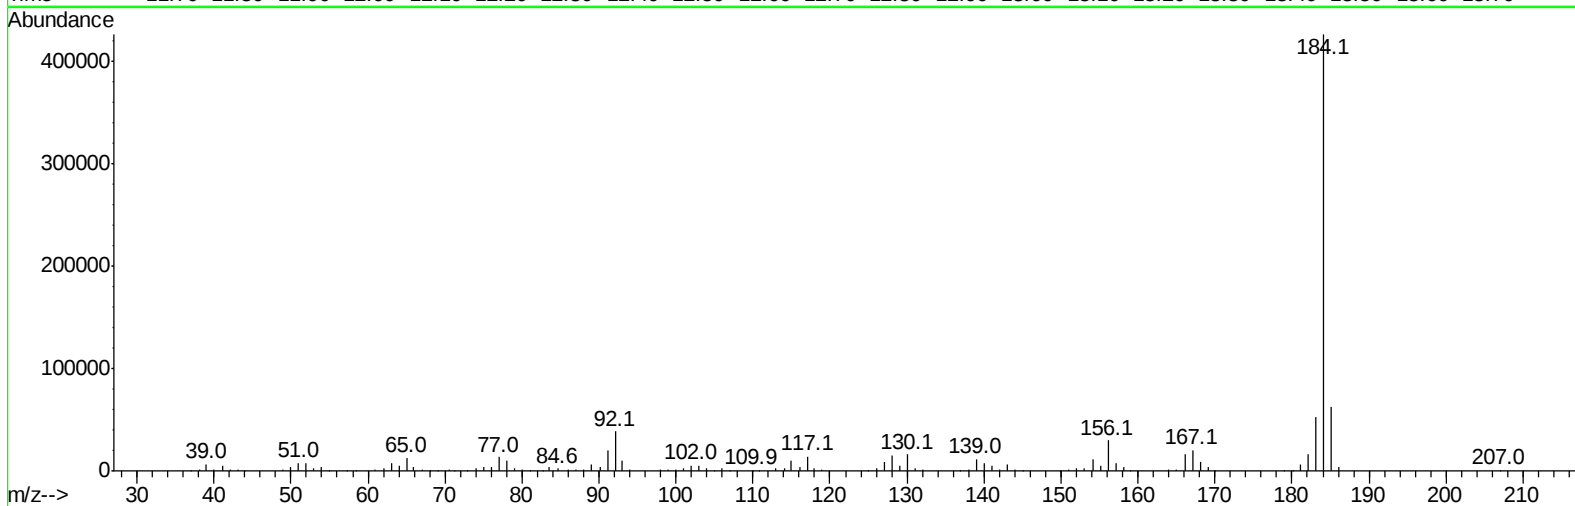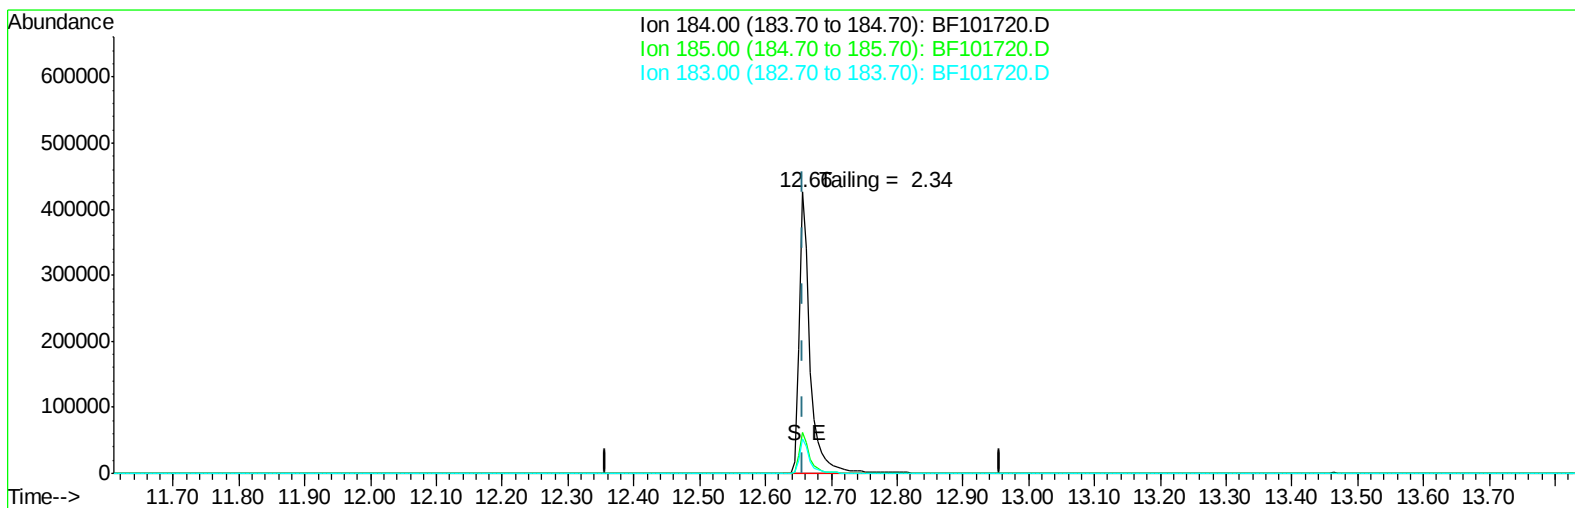

TIC: BF101720.D

(76) Benzidine

12.657min (-0.000) 0.00ng

response 493526

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.59
183.00	11.60	12.44
0.00	0.00	0.00