
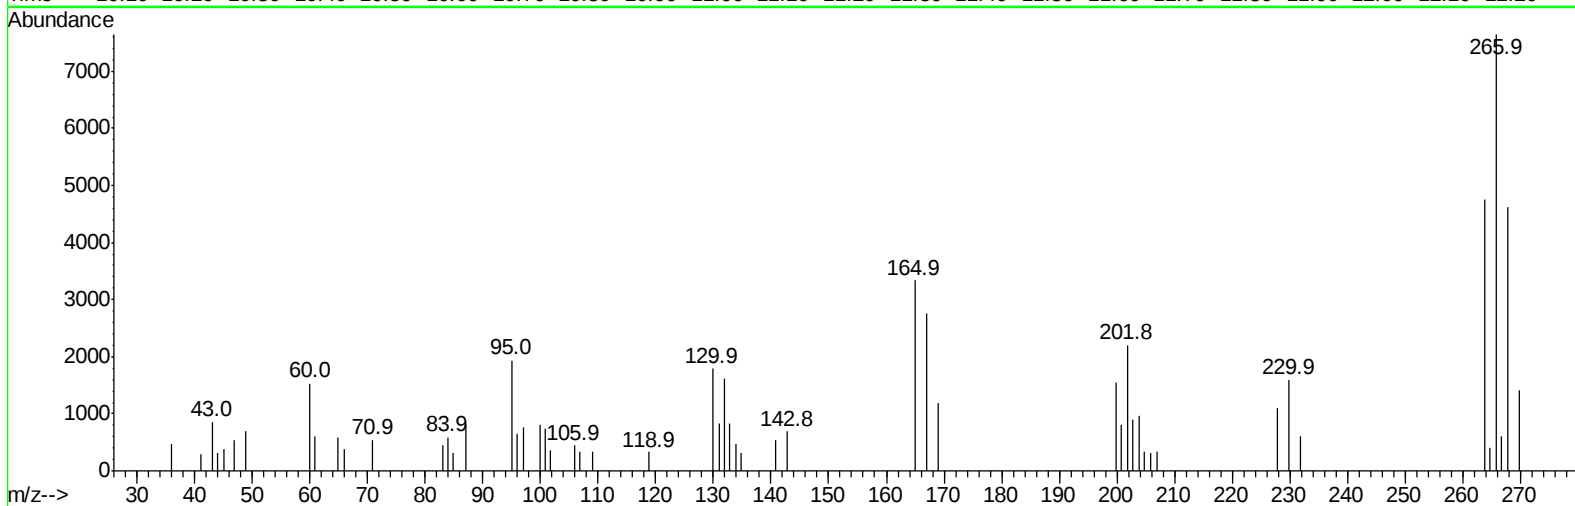


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122617\
Data File : BF101746.D
Acq On : 27 Dec 2017 6:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 08:26:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

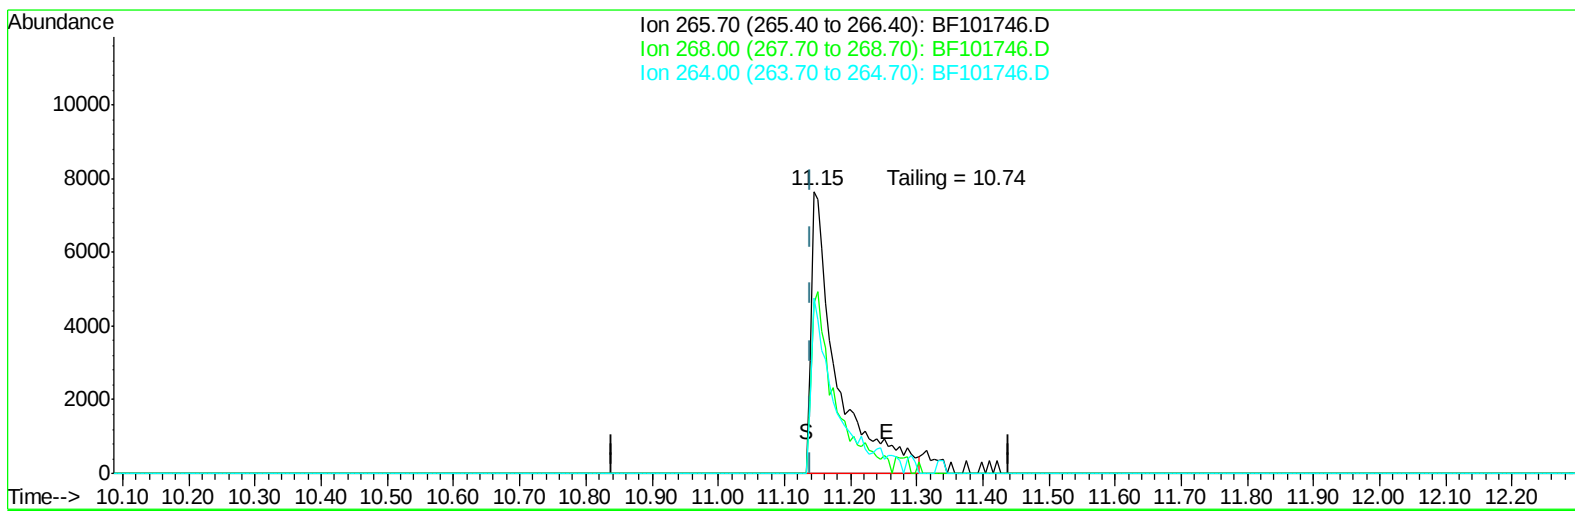

TIC: BF101746.D

(69) Pentachlorophenol (C)



11.145min (+0.006) 0.00ng m

response 20610

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.33
264.00	61.90	62.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122617\
 Data File : BF101746.D
 Acq On : 27 Dec 2017 6:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 08:26:45 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 10:48:01 2017
 Response via : Initial Calibration

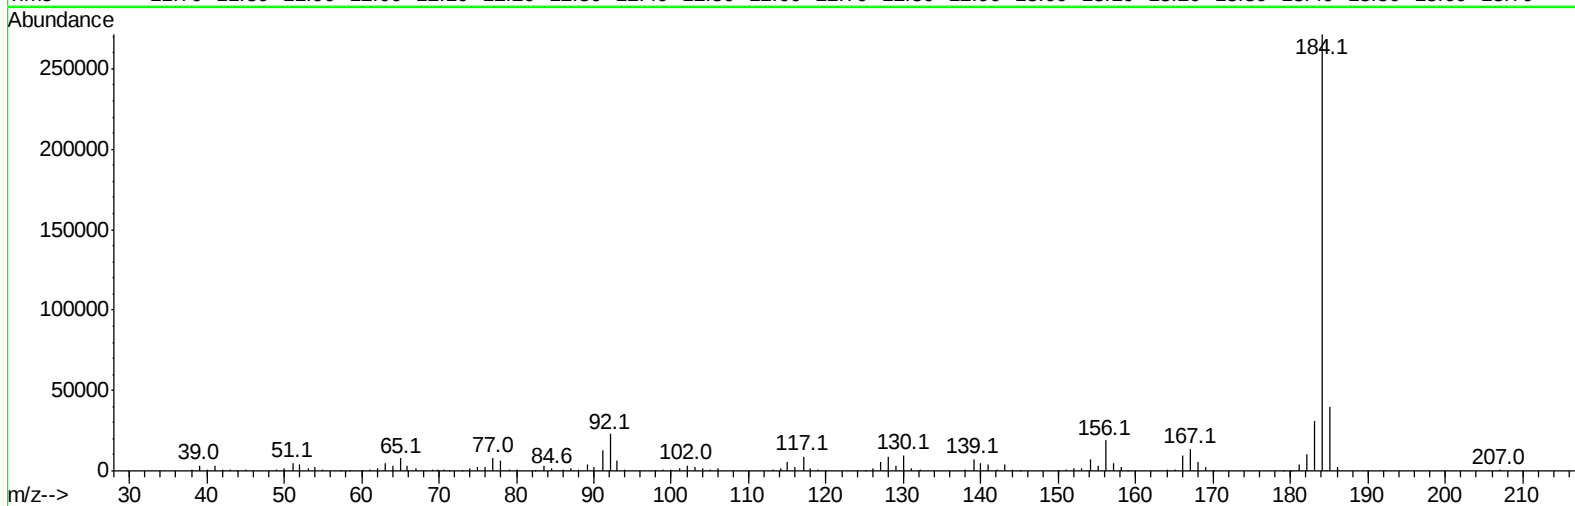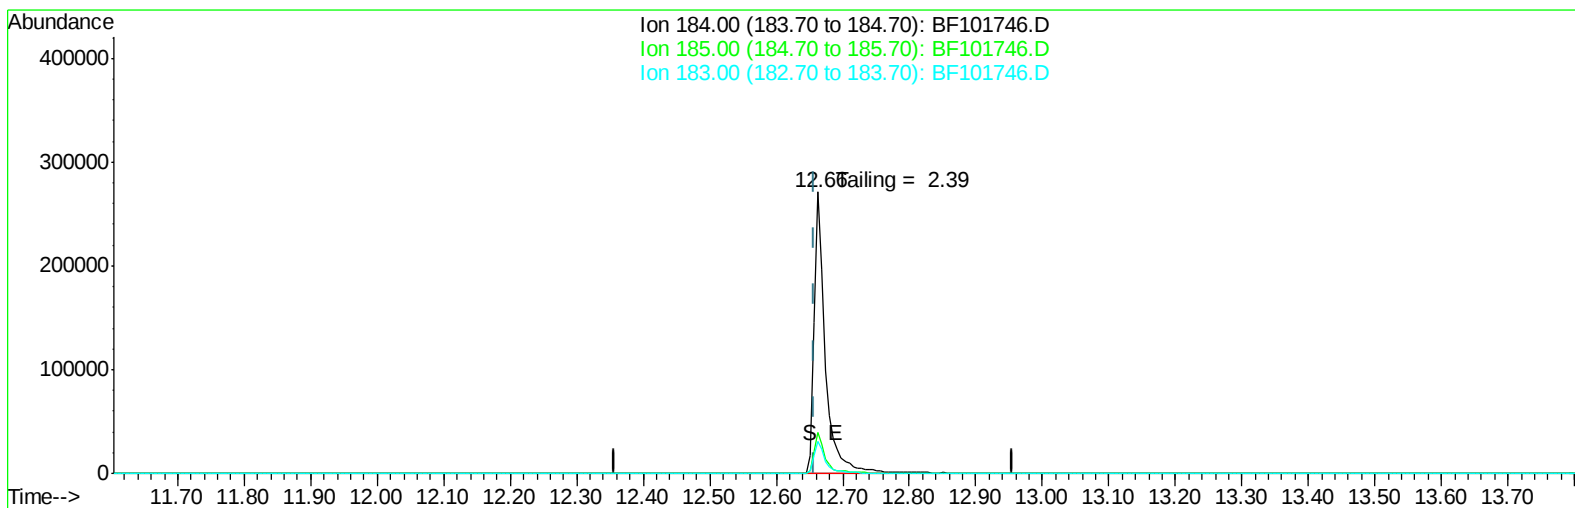

TIC: BF101746.D

(76) Benzidine

12.663min (+0.006) 0.00ng

response 325475

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.53
183.00	11.60	11.47
0.00	0.00	0.00