

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122617\
 Data File : BF101757.D
 Acq On : 27 Dec 2017 11:50
 Operator : SJ/JU
 Sample : I7010-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 122017-TIDO-F-U-B

Quant Time: Dec 27 12:18:41 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 10:48:01 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	143391	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	532181	20.00	ng	0.00
38) Acenaphthene-d10	9.83	164	199319	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	315548	20.00	ng	0.00
75) Chrysene-d12	13.97	240	305074	20.00	ng	0.00
86) Perylene-d12	15.44	264	251426	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	280273	29.12	ng	0.02
7) Phenol-d6	6.45	99	222237	18.55	ng	0.01
23) Nitrobenzene-d5	7.36	82	795268	83.18	ng	0.00
41) 2,4,6-Tribromophenol	10.62	330	129130	67.23	ng	0.00
44) 2-Fluorobiphenyl	9.15	172	1226748	95.47	ng	0.00
78) Terphenyl-d14	12.90	244	891980	70.49	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122617\
Data File : BF101757.D
Acq On : 27 Dec 2017 11:50
Operator : SJ/JU
Sample : I7010-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
122017-TIDO-F-U-B

Quant Time: Dec 27 12:18:41 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration




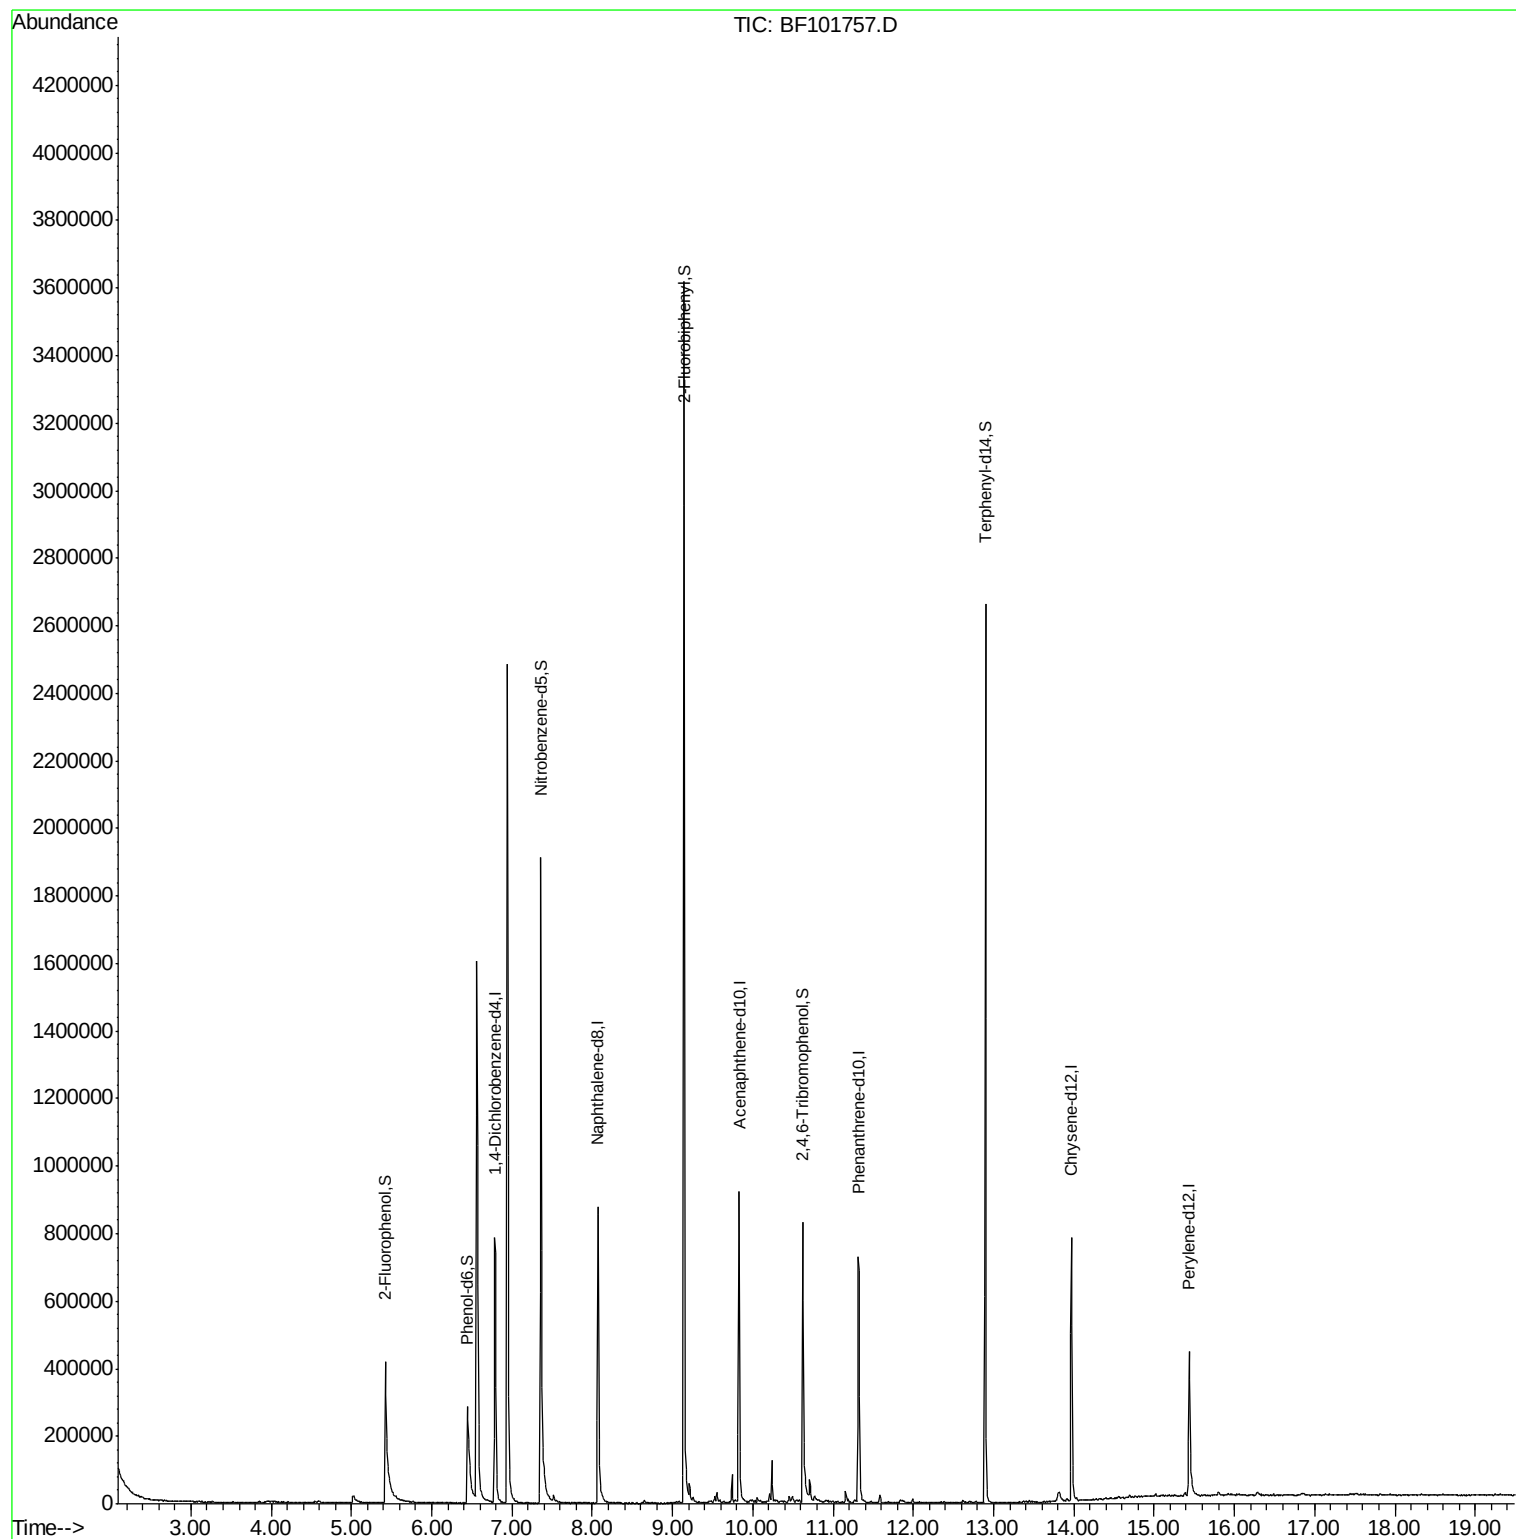


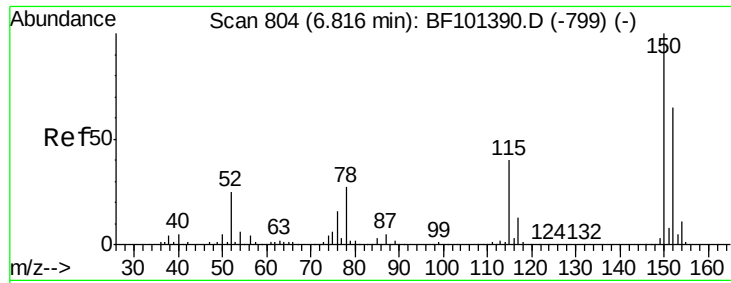

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.79 min Scan# 800
 Delta R.T. 0.01 min
 Lab File: BF101757.D
 Acq: 27 Dec 2017 11:50




Instrument :
 BNA_F
 ClientSampleId :
 122017-TIDO-F-U-B


Tgt Ion:152 Resp: 143391
 Ion Ratio Lower Upper
 152 100
 150 153.7 124.6 186.8
 115 60.3 50.1 75.1

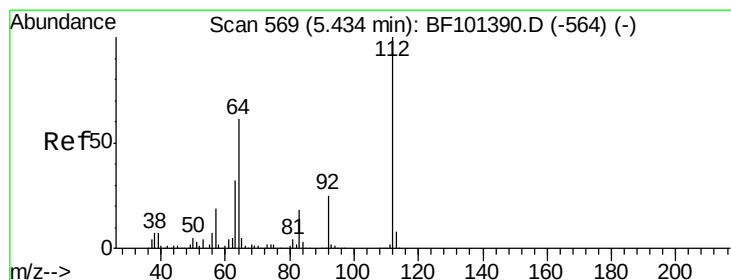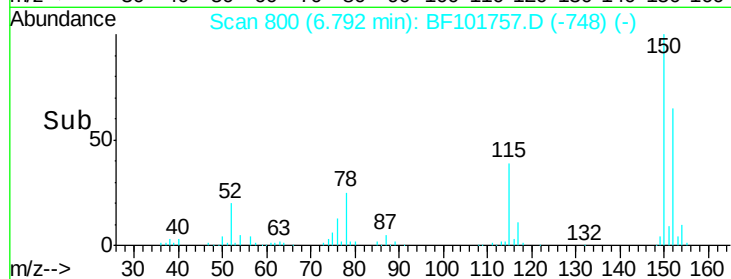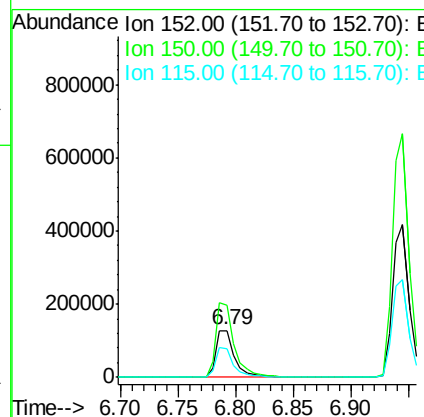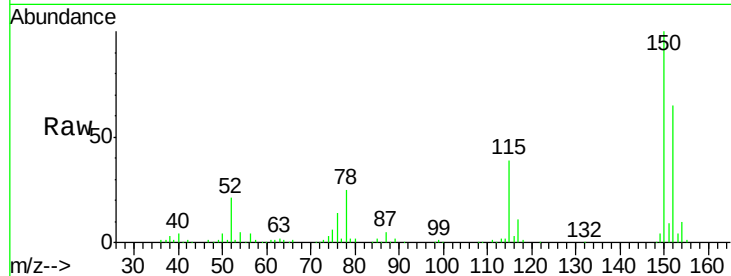

#5
 2-Fluorophenol
 Concen: 29.115 ng
 RT: 5.42 min Scan# 567
 Delta R.T. 0.02 min
 Lab File: BF101757.D
 Acq: 27 Dec 2017 11:50

Tgt Ion:112 Resp: 280273
 Ion Ratio Lower Upper
 112 100
 64 59.1 47.9 71.9
 63 31.2 23.7 35.5

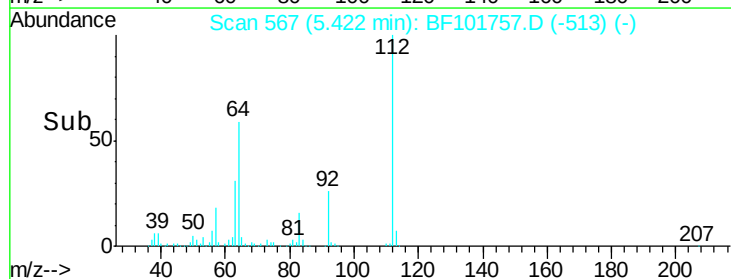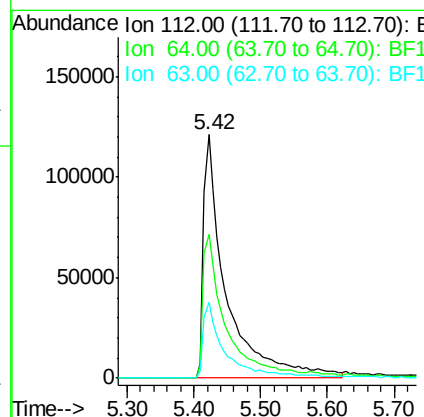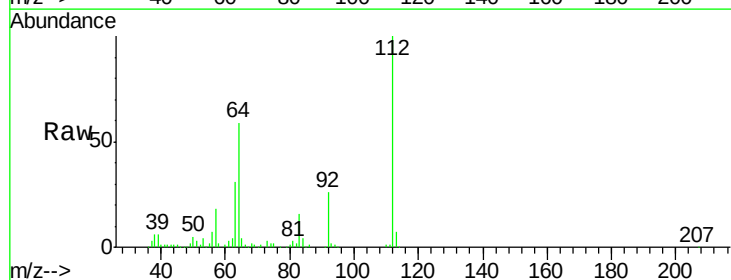

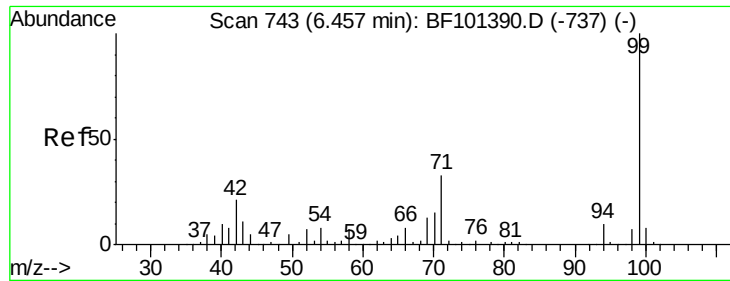

#7

Phenol-d6

Concen: 18.550 ng

RT: 6.45 min Scan# 741

Delta R.T. 0.01 min

Lab File: BF101757.D

Acq: 27 Dec 2017 11:50

Instrument :

BNA_F

ClientSampleId :

122017-TIDO-F-U-B


Tgt Ion: 99 Resp: 222237

Ion Ratio Lower Upper

99 100

42 18.7 14.5 21.7




71 30.3 25.4 38.0

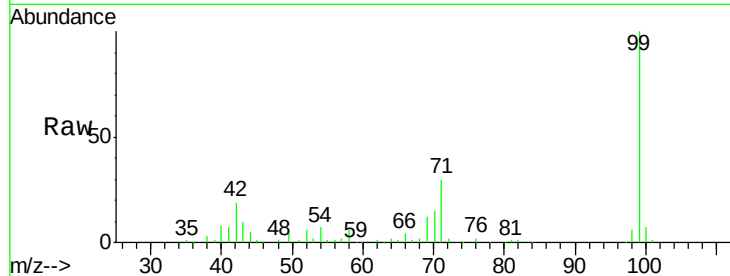

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

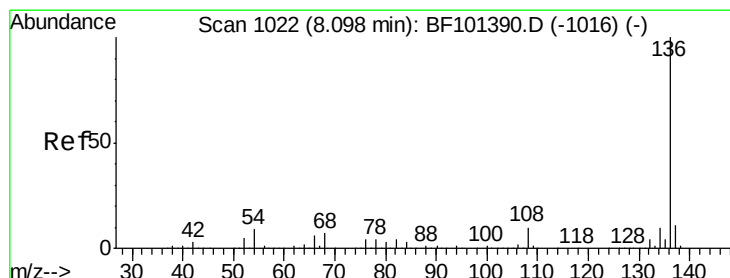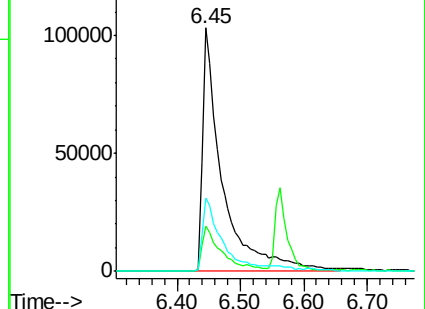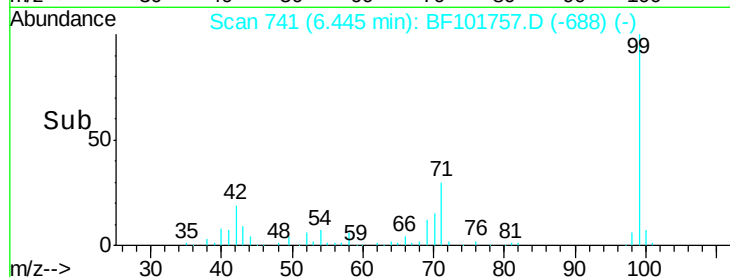

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1017

Delta R.T. -0.00 min

Lab File: BF101757.D

Acq: 27 Dec 2017 11:50

Tgt Ion: 136 Resp: 532181


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 9.4 6.6 9.8

68 7.1 5.0 7.4


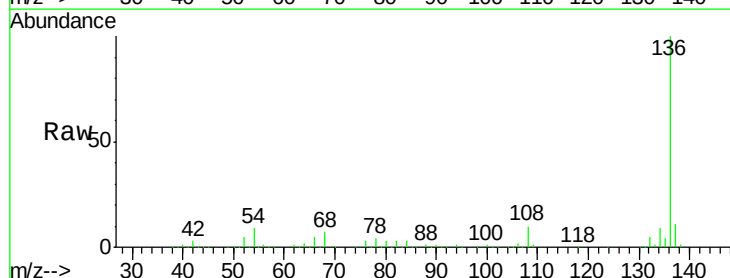



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

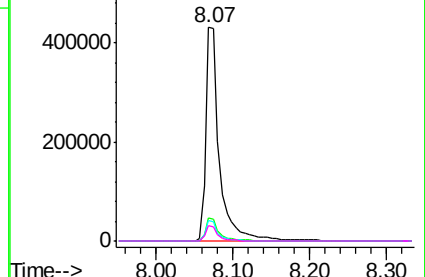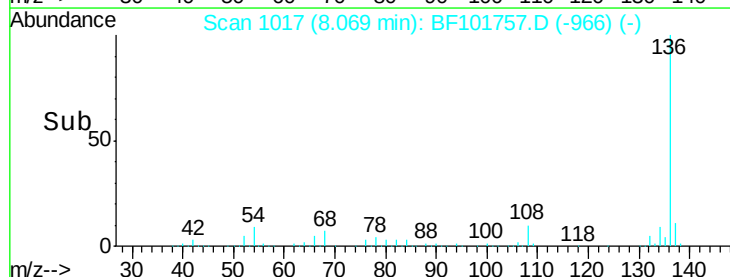


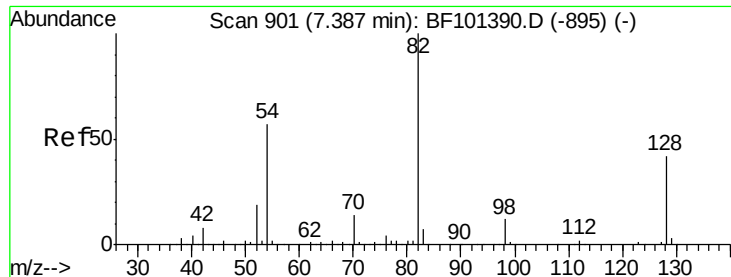




#23
 Nitrobenzene-d5
 Concen: 83.185 ng
 RT: 7.36 min Scan# 897
 Delta R.T. -0.00 min
 Lab File: BF101757.D
 Acq: 27 Dec 2017 11:50

Instrument :
 BNA_F
 ClientSampleId :
 122017-TIDO-F-U-B

Tgt Ion: 82 Resp: 795268
 Ion Ratio Lower Upper
 82 100
 128 45.9 36.1 54.1
 54 54.3 41.4 62.2

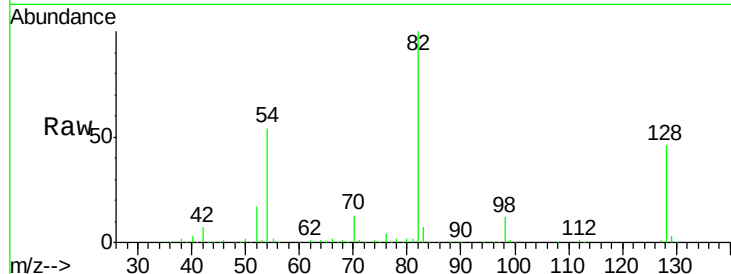


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

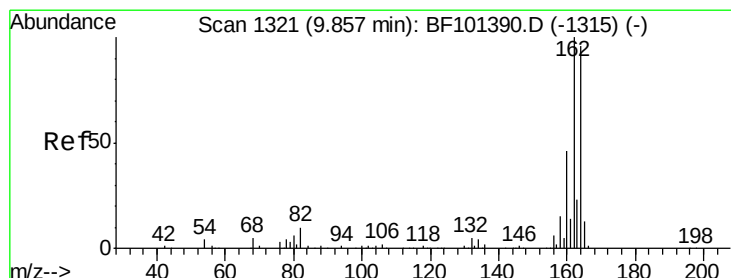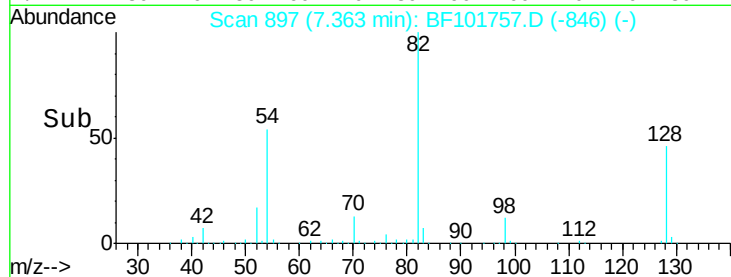
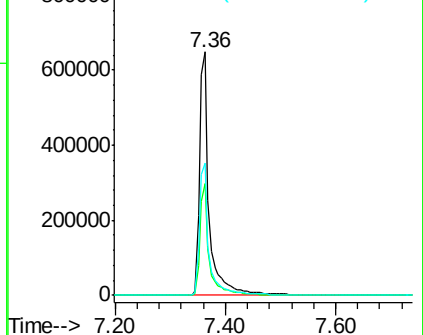



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.83 min Scan# 1316
 Delta R.T. -0.00 min
 Lab File: BF101757.D
 Acq: 27 Dec 2017 11:50

Tgt Ion: 164 Resp: 199319
 Ion Ratio Lower Upper
 164 100
 162 104.9 86.1 129.1
 160 48.9 38.3 57.5

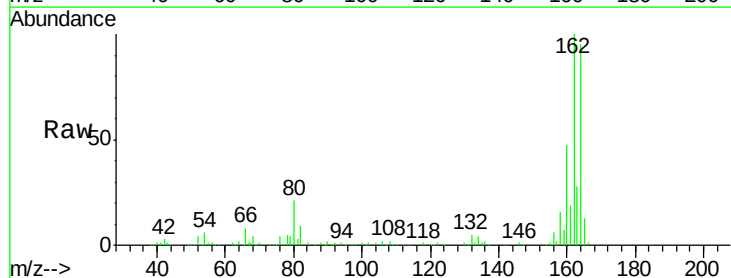

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

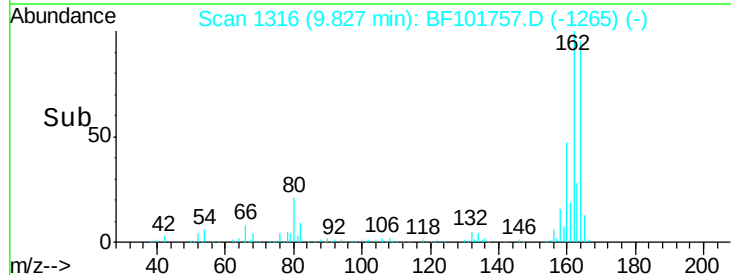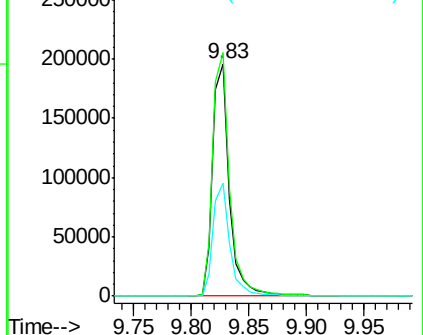


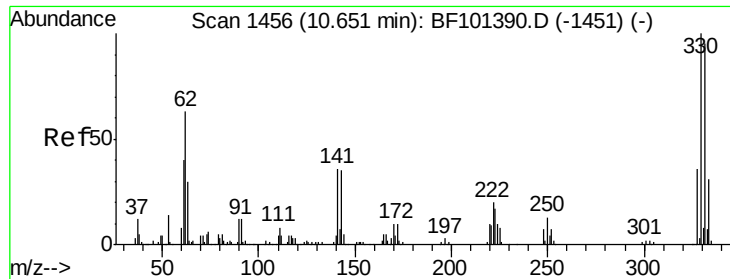




#41
 2,4,6-Tribromophenol
 Concen: 67.234 ng
 RT: 10.62 min Scan# 1451
 Delta R.T. -0.00 min
 Lab File: BF101757.D
 Acq: 27 Dec 2017 11:50

Instrument :
 BNA_F
 ClientSampleId :
 122017-TIDO-F-U-B

Tgt Ion	Ratio	Lower	Upper
330	100		
332	94.7	77.0	115.6
141	34.2	29.9	44.9

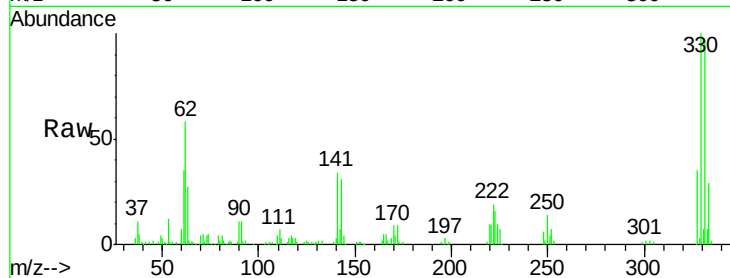


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

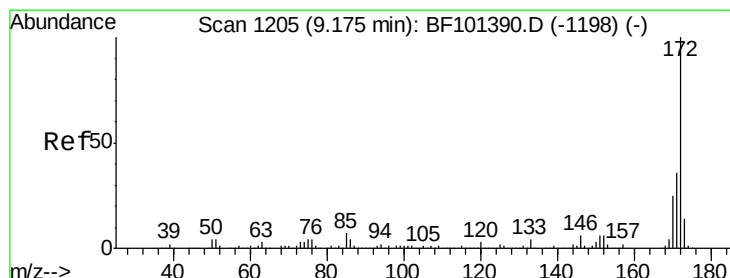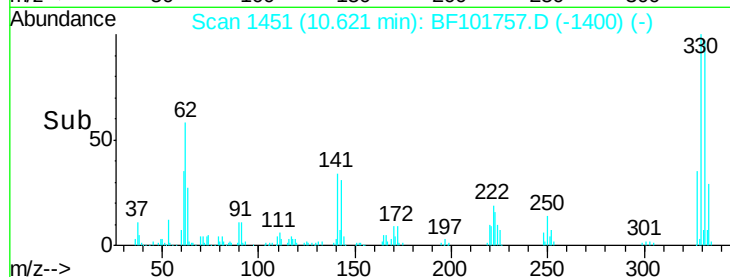
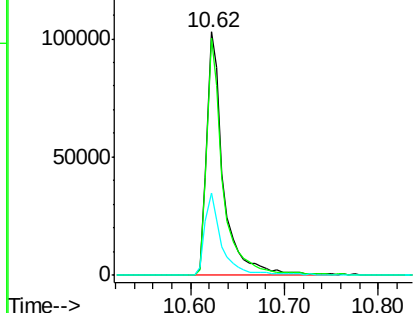



#44
 2-Fluorobiphenyl
 Concen: 95.474 ng
 RT: 9.15 min Scan# 1200
 Delta R.T. -0.00 min
 Lab File: BF101757.D
 Acq: 27 Dec 2017 11:50

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.7	44.5
170	24.9	19.6	29.4

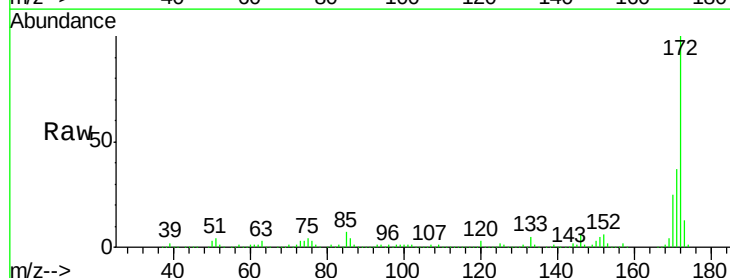

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

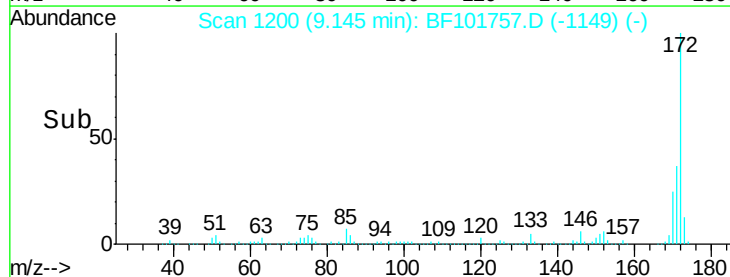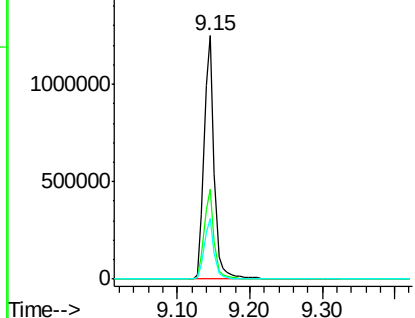

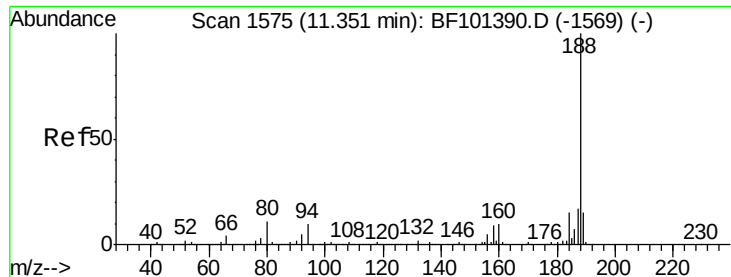

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.32 min Scan# 1569

Delta R.T. -0.00 min

Lab File: BF101757.D

Acq: 27 Dec 2017 11:50

Instrument :

BNA_F

ClientSampleId :

122017-TIDO-F-U-B


Tgt Ion:188 Resp: 315548

Ion Ratio Lower Upper

188 100

94 11.8 8.5 12.7




80 12.9 9.2 13.8

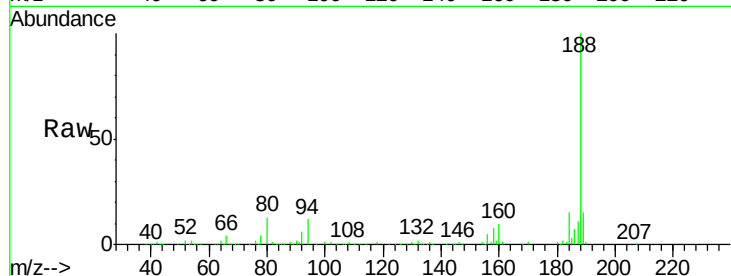

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

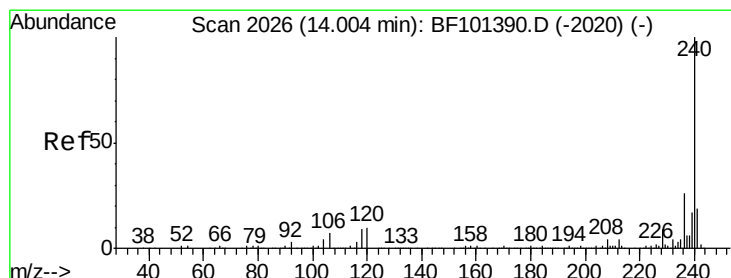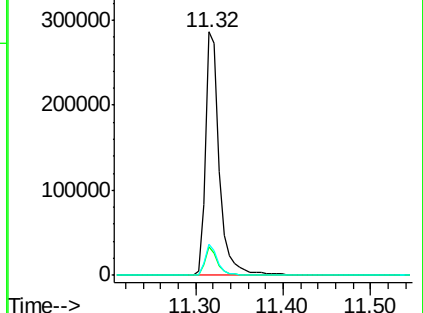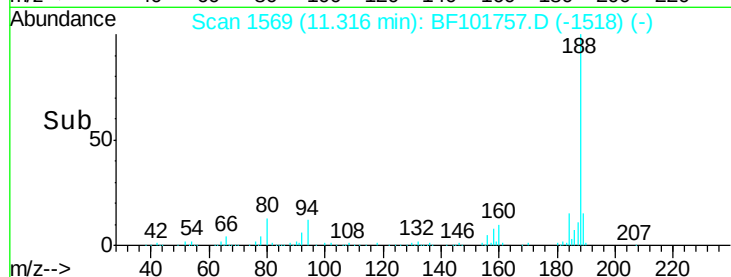

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.97 min Scan# 2020

Delta R.T. -0.00 min

Lab File: BF101757.D

Acq: 27 Dec 2017 11:50


Tgt Ion:240 Resp: 305074

Ion Ratio Lower Upper

240 100

120 12.2 9.5 14.3



236 25.0 20.7 31.1

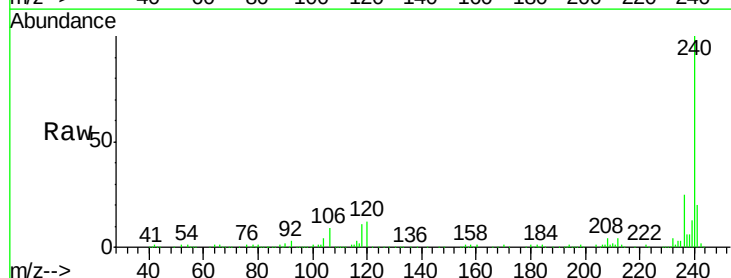


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

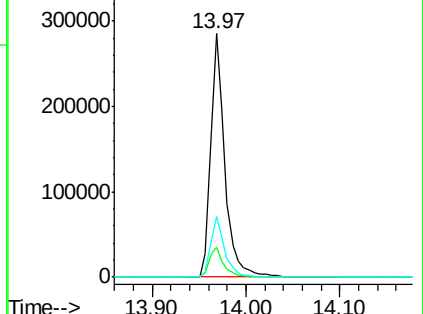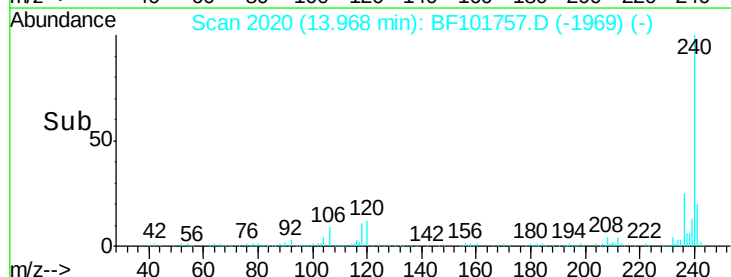

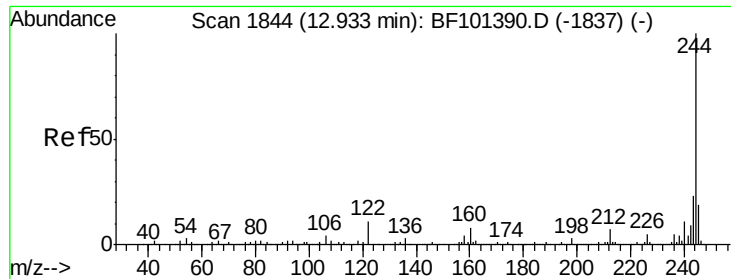

#78

Terphenyl-d14

Concen: 70.486 ng

RT: 12.90 min Scan# 1838

Delta R.T. -0.00 min

Lab File: BF101757.D

Acq: 27 Dec 2017 11:50

Instrument :

BNA_F

ClientSampleId :

122017-TIDO-F-U-B


Tgt Ion:244 Resp: 891980

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 11.8 11.0 16.4

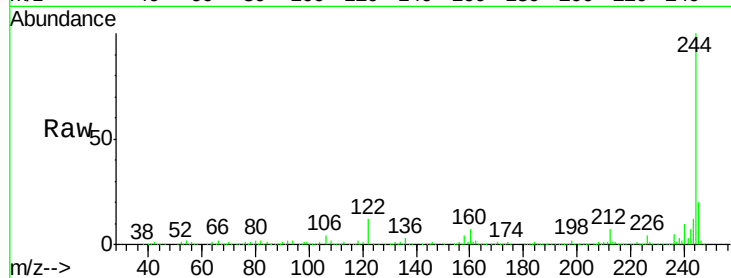

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

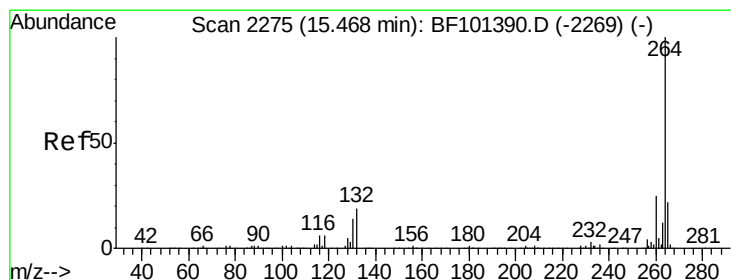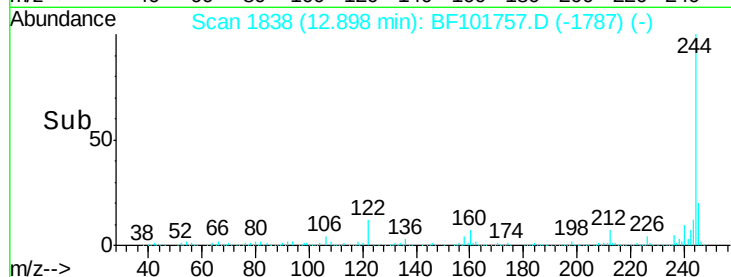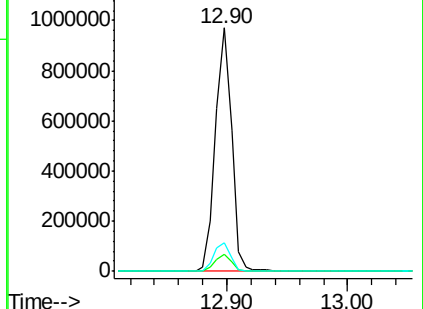

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2270

Delta R.T. 0.01 min

Lab File: BF101757.D

Acq: 27 Dec 2017 11:50


Tgt Ion:264 Resp: 251426

Ion Ratio Lower Upper

264 100

260 22.3 19.2 28.8

265 21.2 17.5 26.3

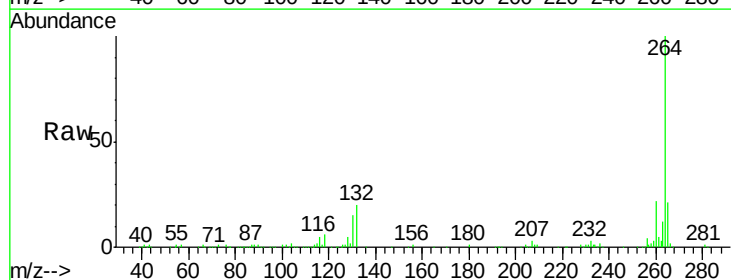

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

