


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122617\
 Data File : BF101702.D
 Acq On : 26 Dec 2017 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 29 13:21:45 2017

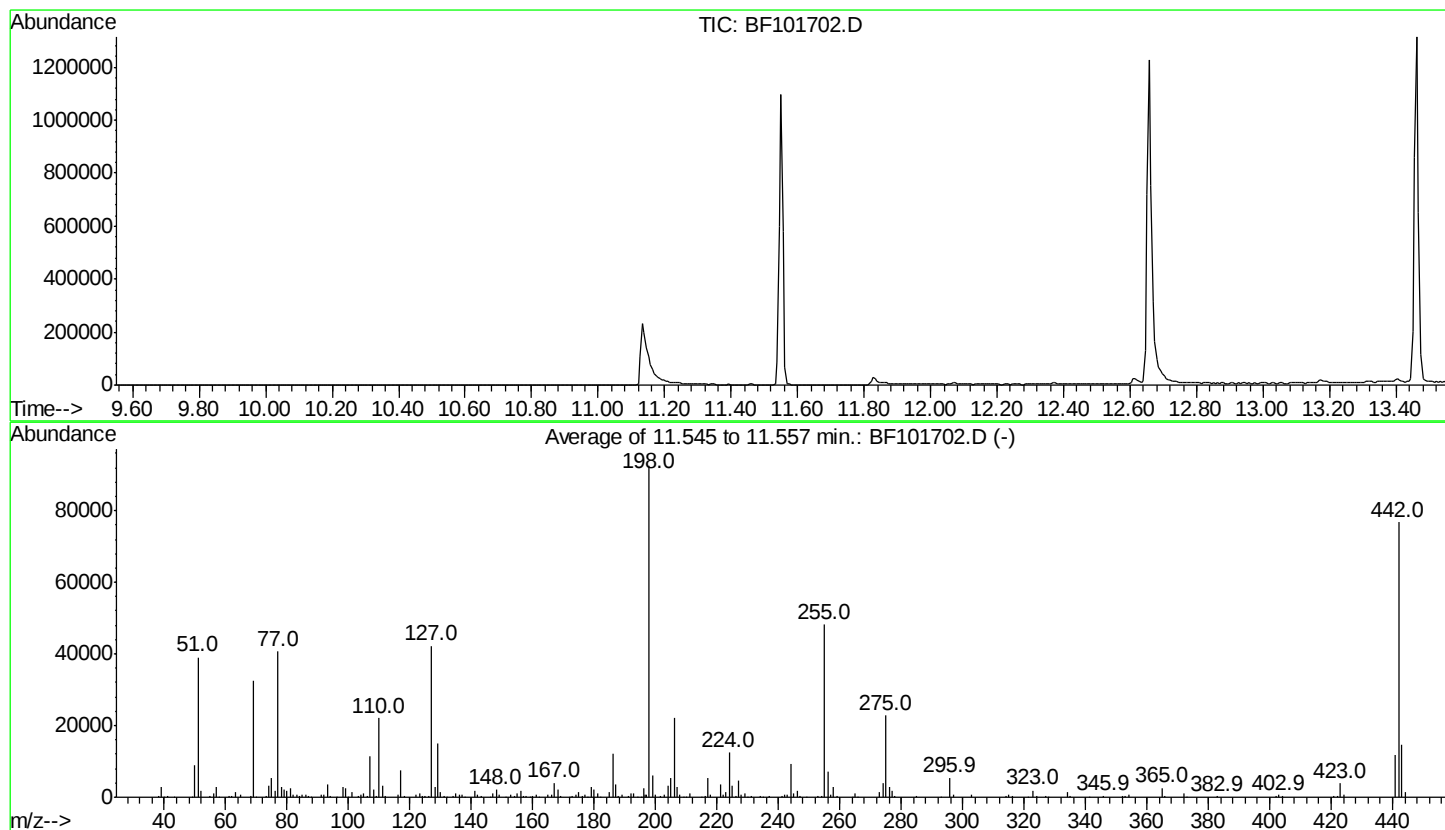

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	39077	PASS
68	69	0.00	2	1.6	521	PASS
69	198	0.00	100	35.0	32392	PASS
70	69	0.00	2	0.4	119	PASS
127	198	10	80	45.6	42234	PASS
197	198	0.00	2	0.8	710	PASS
198	198	100	100	100.0	92560	PASS
199	198	5	9	6.5	6055	PASS
275	198	10	60	24.5	22713	PASS
365	198	1	100	2.9	2673	PASS
441	443	0.01	100	79.6	11689	PASS
442	198	50	100	82.8	76656	PASS
443	442	15	24	19.2	14691	PASS