
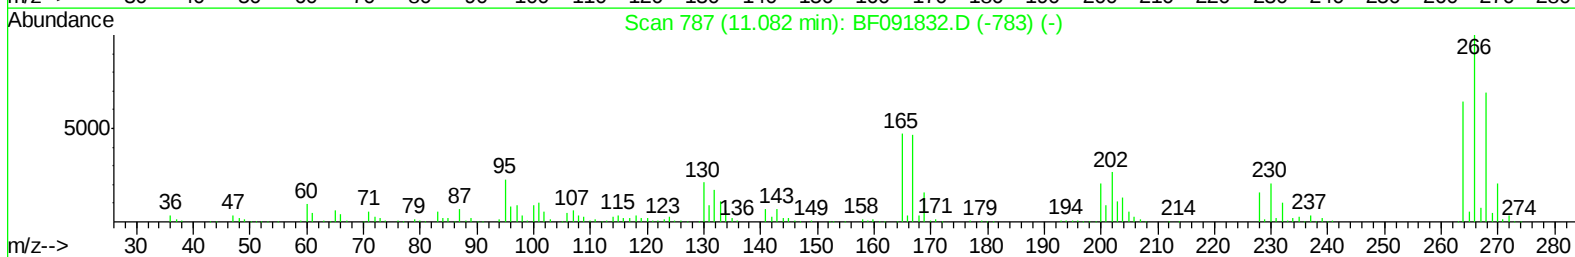
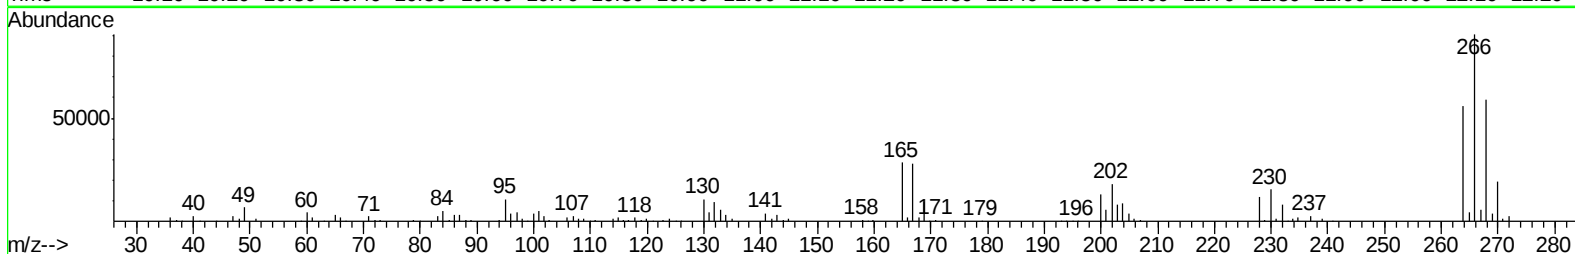


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122716\
Data File : BF091961.D
Acq On : 27 Dec 2016 12:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:40:58 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 16:17:51 2016
Response via : Initial Calibration

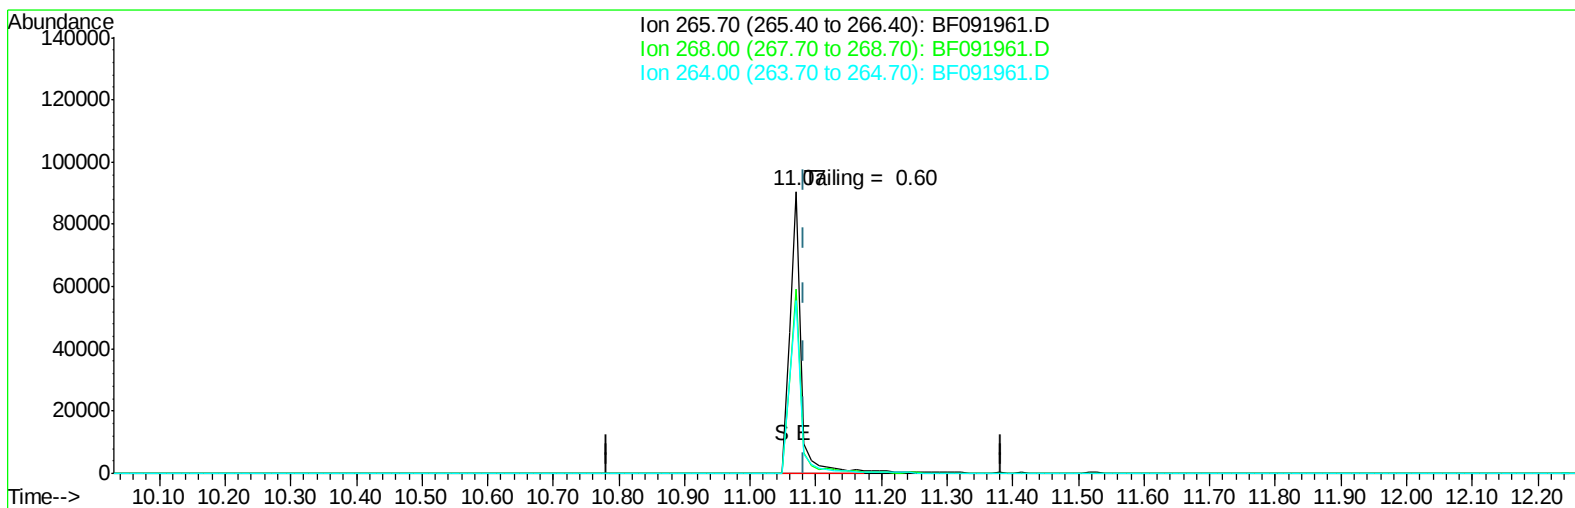

TIC: BF091961.D

(69) Pentachlorophenol (C)




11.071min (-0.012) 92031.42ng

response 112471

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.48
264.00	62.90	61.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122716\
Data File : BF091961.D
Acq On : 27 Dec 2016 12:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:40:58 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 16:17:51 2016
Response via : Initial Calibration

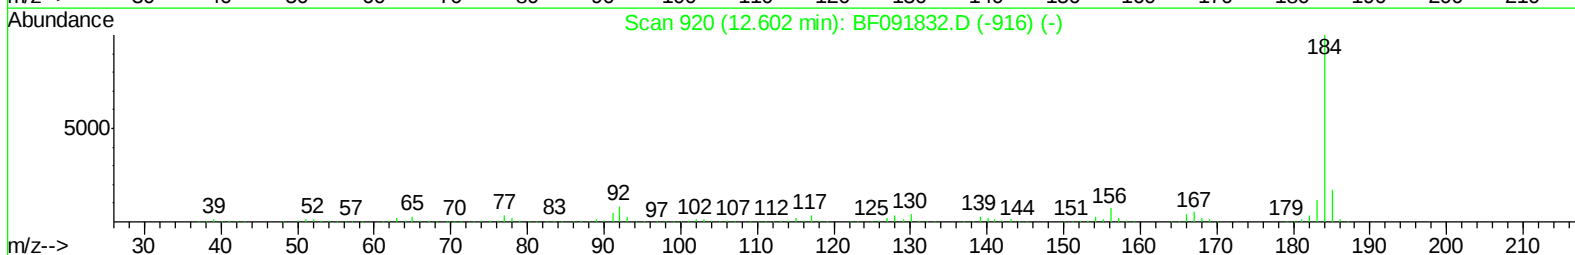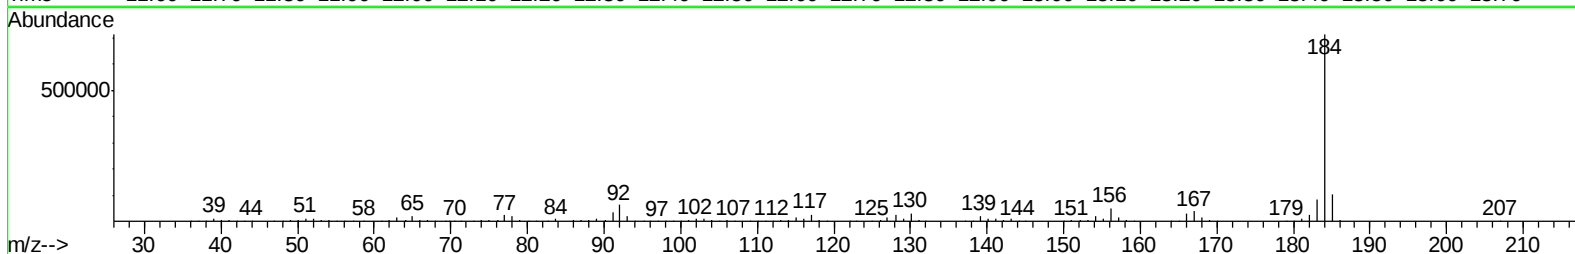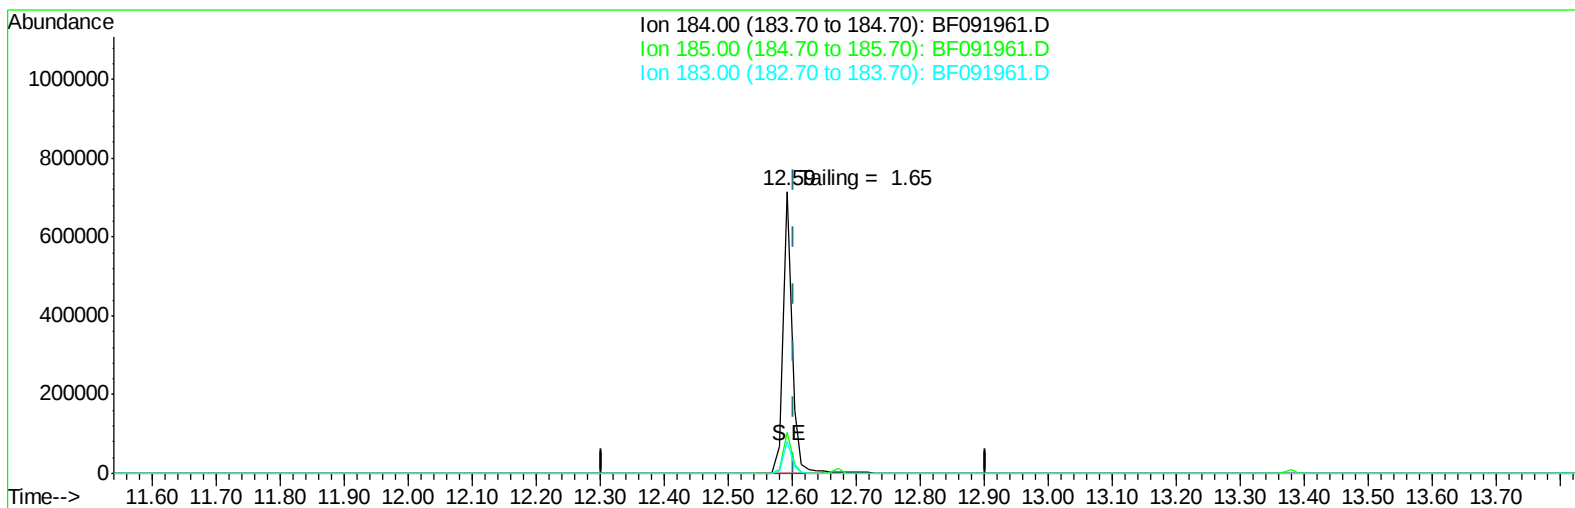

TIC: BF091961.D

(76) Benzidine

12.591min (-0.011) -20.00ng

response 699486

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.63
183.00	11.50	11.60
0.00	0.00	0.00