

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122716\
 Data File : BF091988.D
 Acq On : 28 Dec 2016 2:41
 Operator : UM/SJ
 Sample : H6236-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 122216-DSDC-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.876	242	244	252	rBV	639953	698594	9.02%	1.649%
2	5.344	283	285	299	rVB	1832915	1867504	24.11%	4.408%
3	6.396	374	377	384	rBV	1171340	1229564	15.88%	2.902%
4	6.499	384	386	389	rBV	2703498	3047688	39.35%	7.194%
5	6.727	403	406	408	rBV	1405568	1320983	17.06%	3.118%
6	6.887	417	420	422	rBV	5284555	5660141	73.08%	13.360%
7	7.299	453	456	459	rBV	3834127	4220510	54.49%	9.962%
8	8.019	516	519	521	rBV	1792130	1868333	24.12%	4.410%
9	9.105	610	614	616	rBV	5579535	7744806	100.00%	18.280%
10	9.493	646	648	651	rBV	200009	173213	2.24%	0.409%
11	9.768	670	672	675	rBV	2122553	1872148	24.17%	4.419%
12	10.556	739	741	744	rBV	1956752	2160771	27.90%	5.100%
13	11.253	799	802	804	rBV	2015048	1854813	23.95%	4.378%
14	12.842	938	941	944	rBV	5102464	6081157	78.52%	14.354%
15	13.882	1030	1032	1035	rBV	1077108	1442082	18.62%	3.404%
16	15.288	1152	1155	1158	rBV	932664	1124641	14.52%	2.655%


Sum of corrected areas: 42366948

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122716\
Data File : BF091988.D
Acq On : 28 Dec 2016 2:41
Operator : UM/SJ
Sample : H6236-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
122216-DSDC-E-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

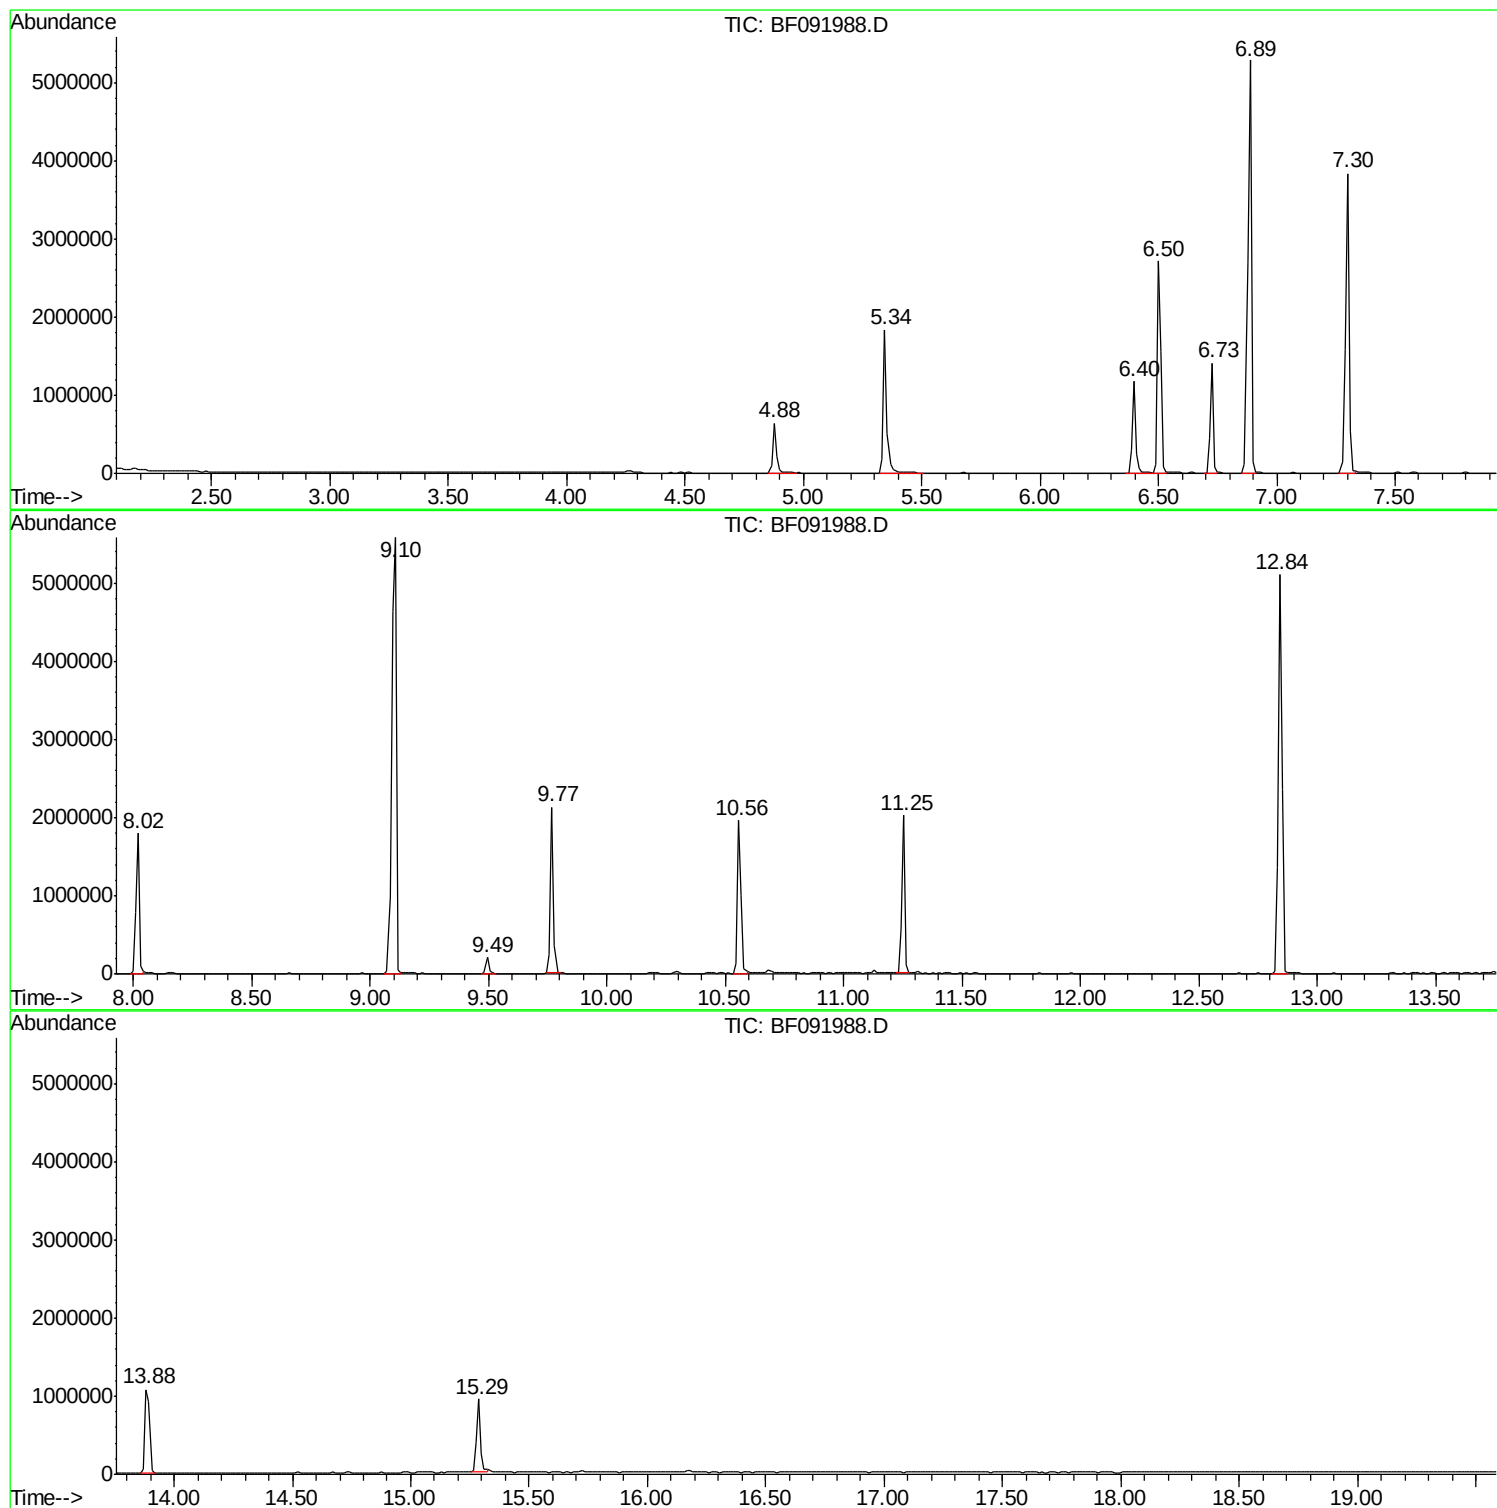

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122716\
Data File : BF091988.D
Acq On : 28 Dec 2016 2:41
Operator : UM/SJ
Sample : H6236-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
122216-DSDC-E-U-M










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.88	10.58 ng	698594	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Propane, 2-methyl-2-(1-methylethoxy)-	116	C7H16O	017348-59-3	36
3		Acetic acid, cyano-, 1,1-dimethyl-	141	C7H11NO2	001116-98-9	23
4		5-Hexen-2-one	98	C6H10O	000109-49-9	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

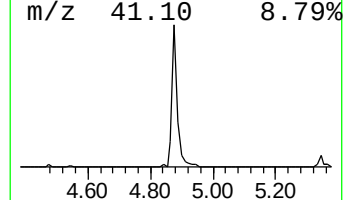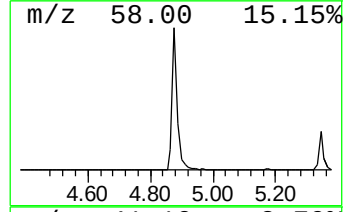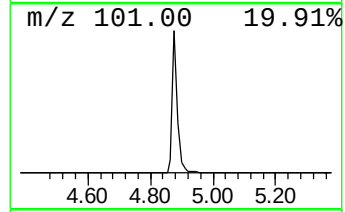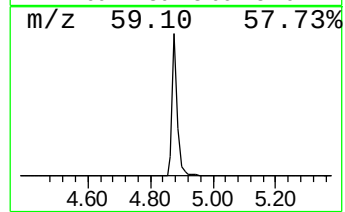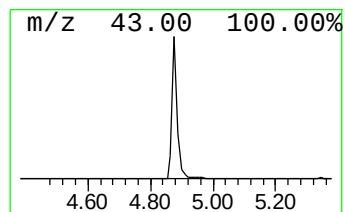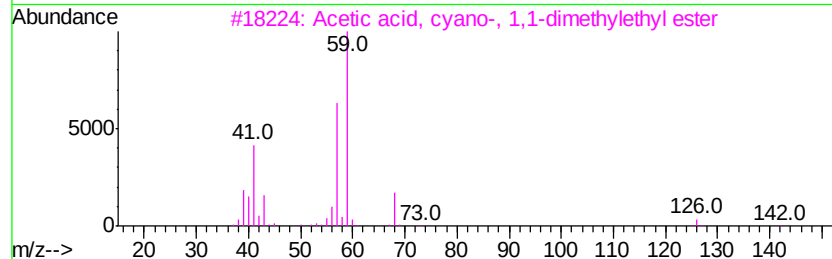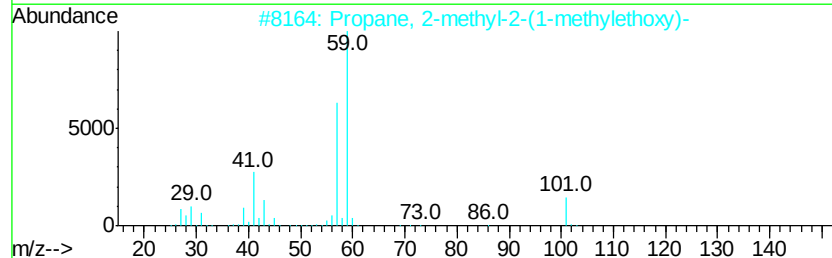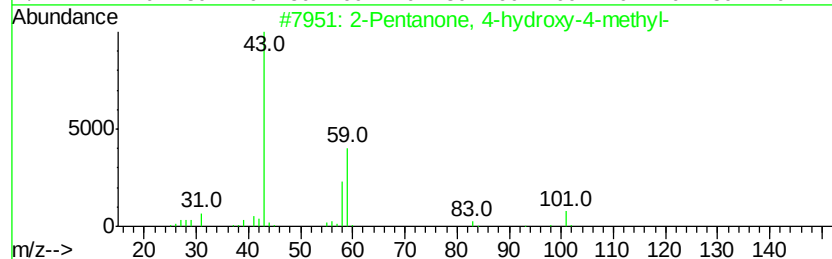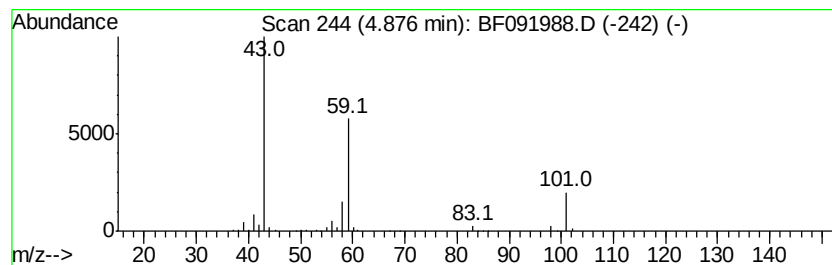

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122716\
Data File : BF091988.D
Acq On : 28 Dec 2016 2:41
Operator : UM/SJ
Sample : H6236-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
122216-DSDC-E-U-M










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.50 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	46.14 ng	3047690	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	12
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

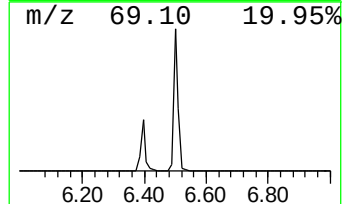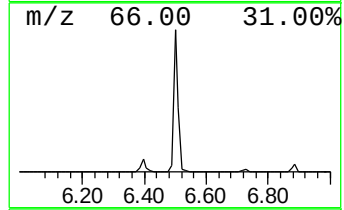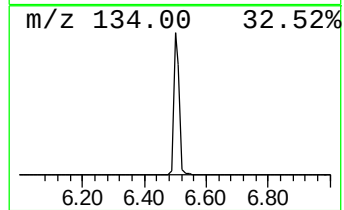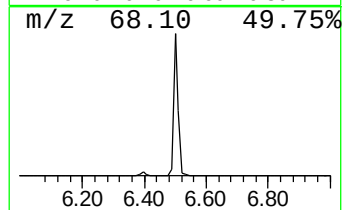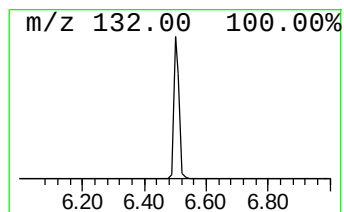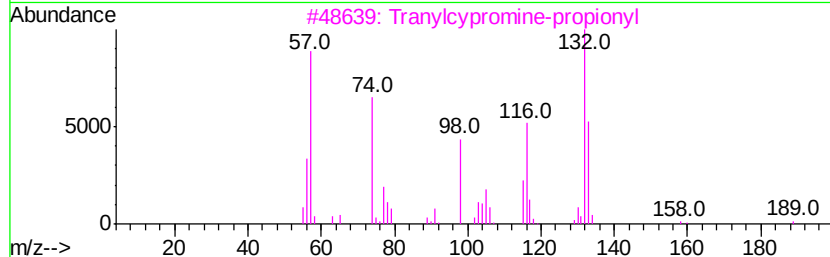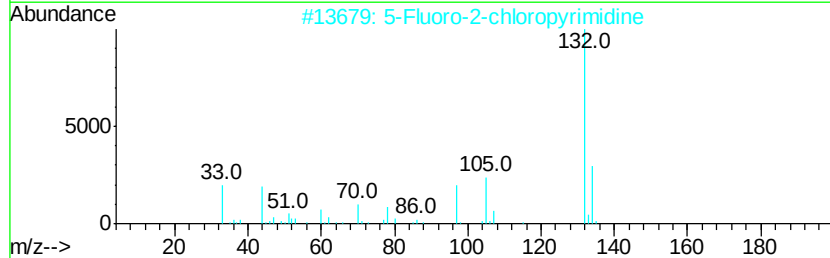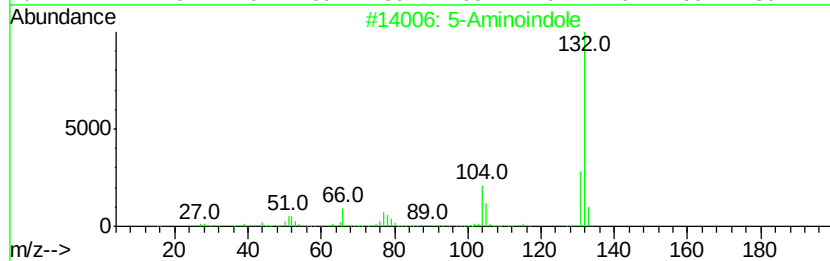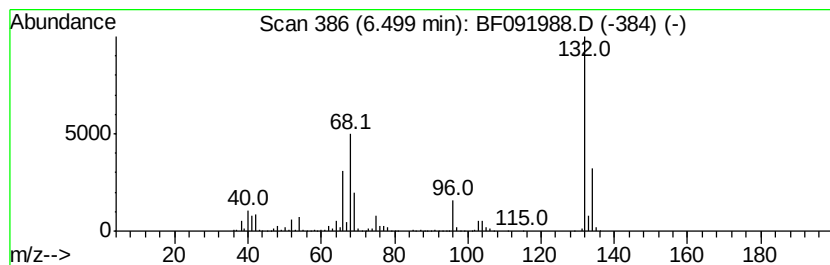

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122716\
Data File : BF091988.D
Acq On : 28 Dec 2016 2:41
Operator : UM/SJ
Sample : H6236-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
122216-DSDC-E-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.88	10.6	ng	698594	1	6.73	1320980	20.0
unknown6.50	6.50	46.1	ng	3047690	1	6.73	1320980	20.0