


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122716\
 Data File : BF091985.D
 Acq On : 27 Dec 2016 23:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 16:17:51 2016

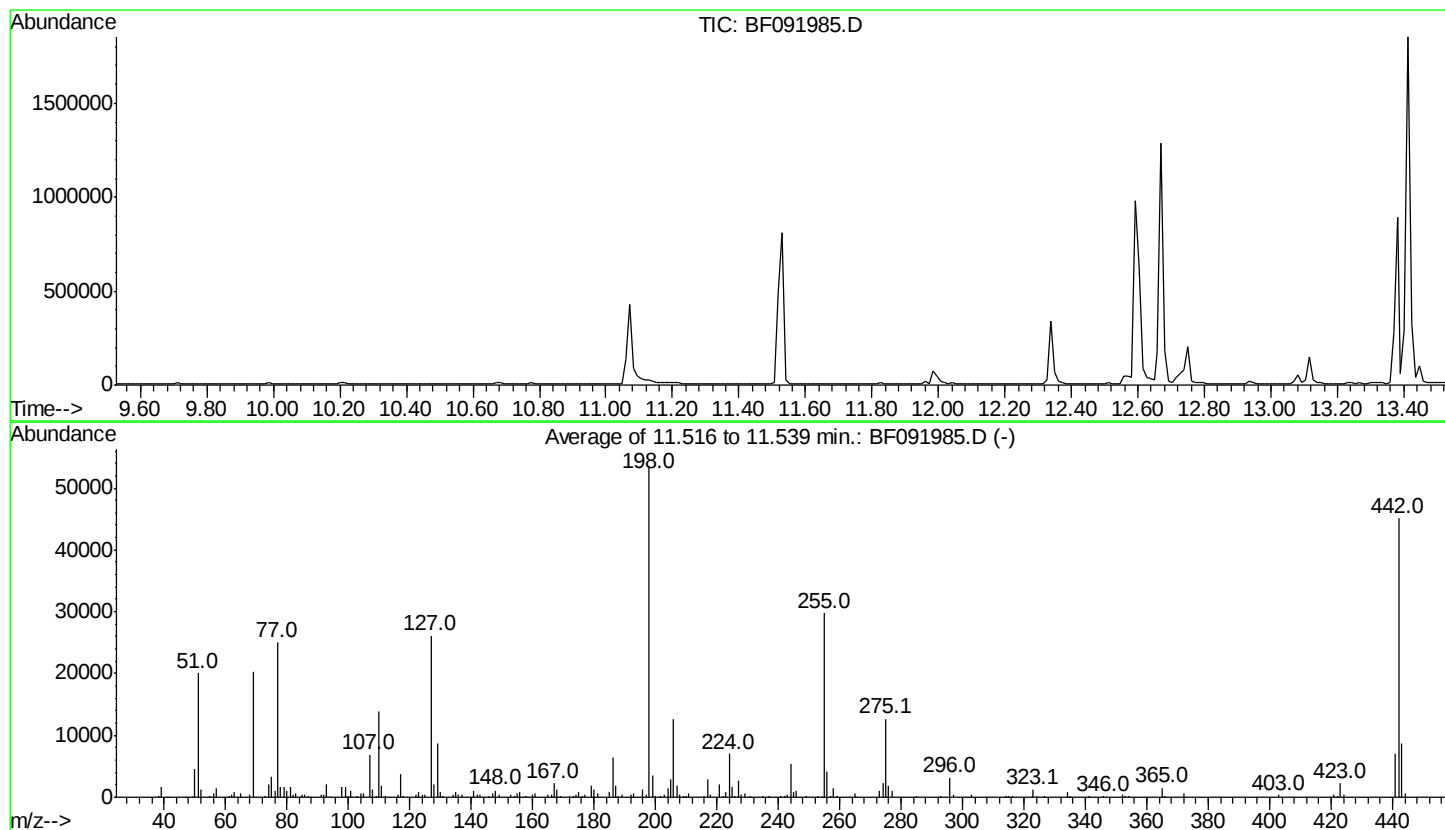

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	20029	PASS
68	69	0.00	2	1.7	351	PASS
69	198	0.00	100	38.0	20383	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	26157	PASS
197	198	0.00	2	0.6	327	PASS
198	198	100	100	100.0	53629	PASS
199	198	5	9	6.6	3535	PASS
275	198	10	60	23.7	12696	PASS
365	198	1	100	2.8	1522	PASS
441	442	0.01	24	15.5	7010	PASS
442	198	50	100	84.1	45123	PASS
443	442	15	24	19.3	8689	PASS