
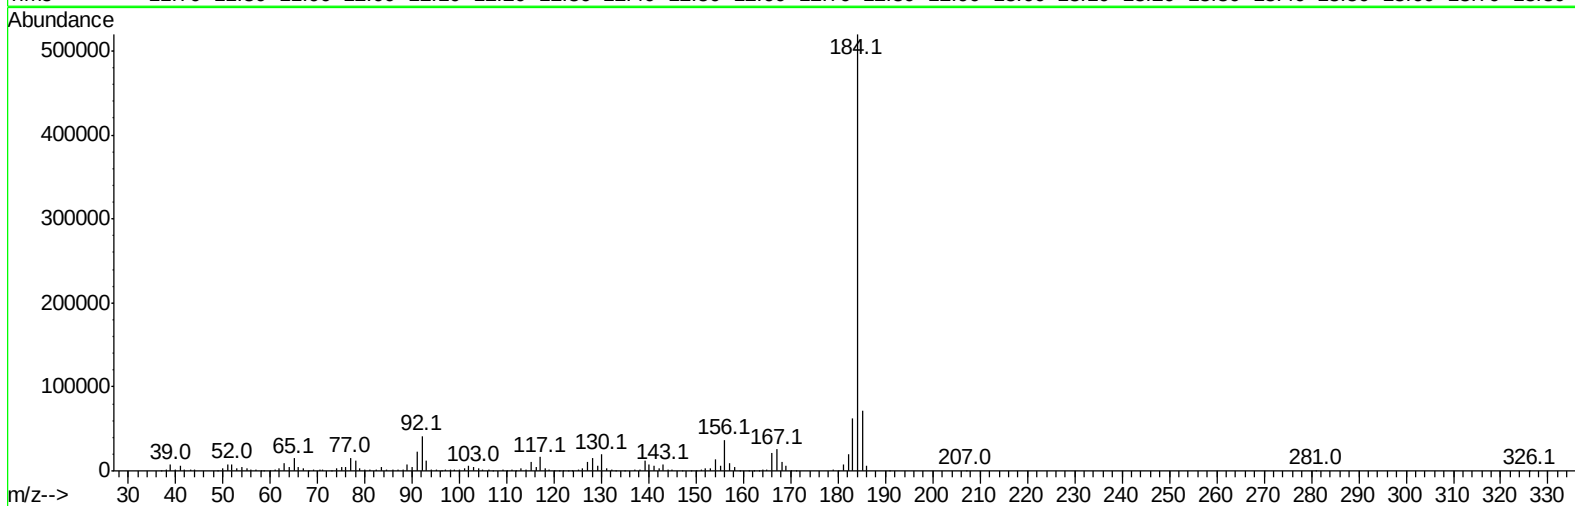


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122717\
Data File : BF101760.D
Acq On : 27 Dec 2017 13:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:57:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

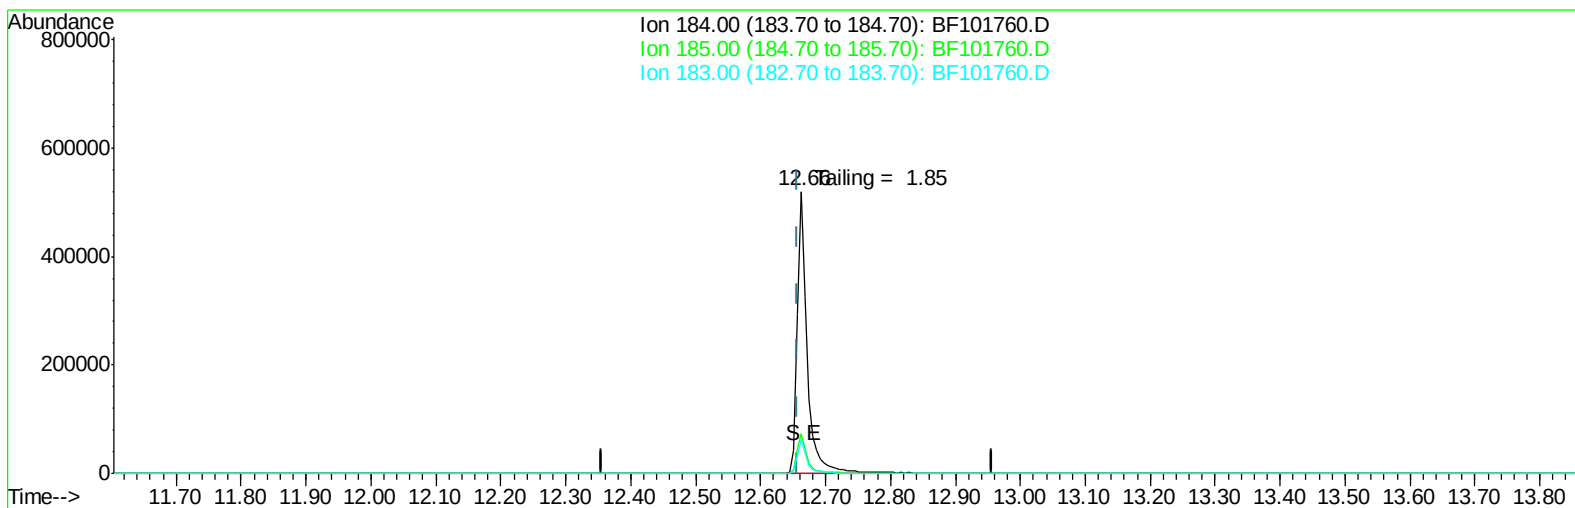

TIC: BF101760.D

(76) Benzidine



12.663min (+0.006) 53156.78ng

response 554536

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.93
183.00	11.60	11.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122717\
Data File : BF101760.D
Acq On : 27 Dec 2017 13:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:57:28 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

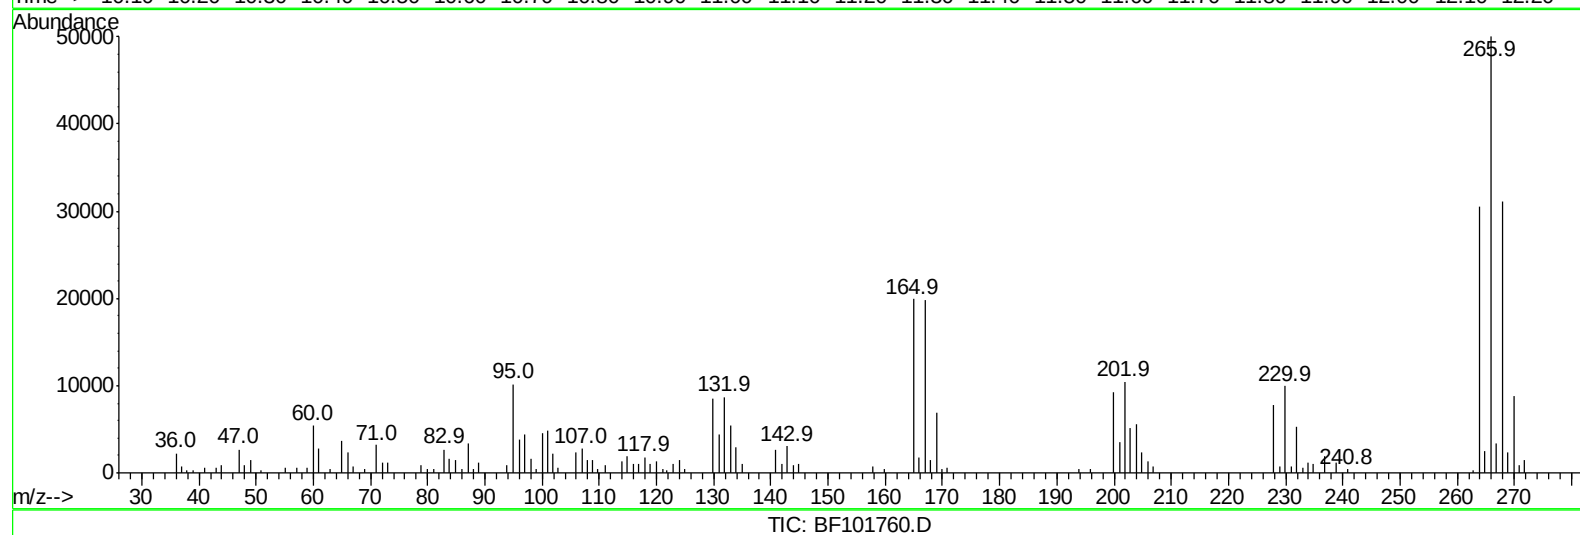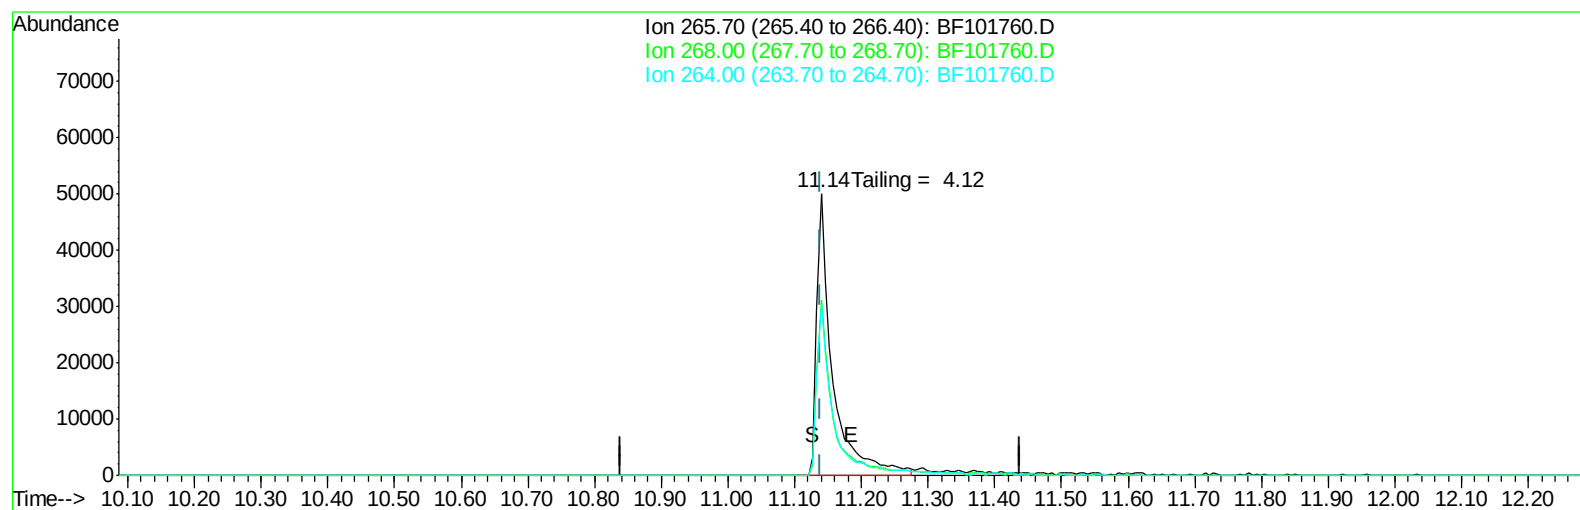

(69) Pentachlorophenol (C)

11.139min (+0.000) 42863.16ng

response 80310

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.15
264.00	61.90	61.00
0.00	0.00	0.00