


Data Path : Z:\HPCHEM1\BNA F\Data\BF122717\
 Data File : BF101760.D
 Acq On : 27 Dec 2017 13:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 26 10:48:01 2017

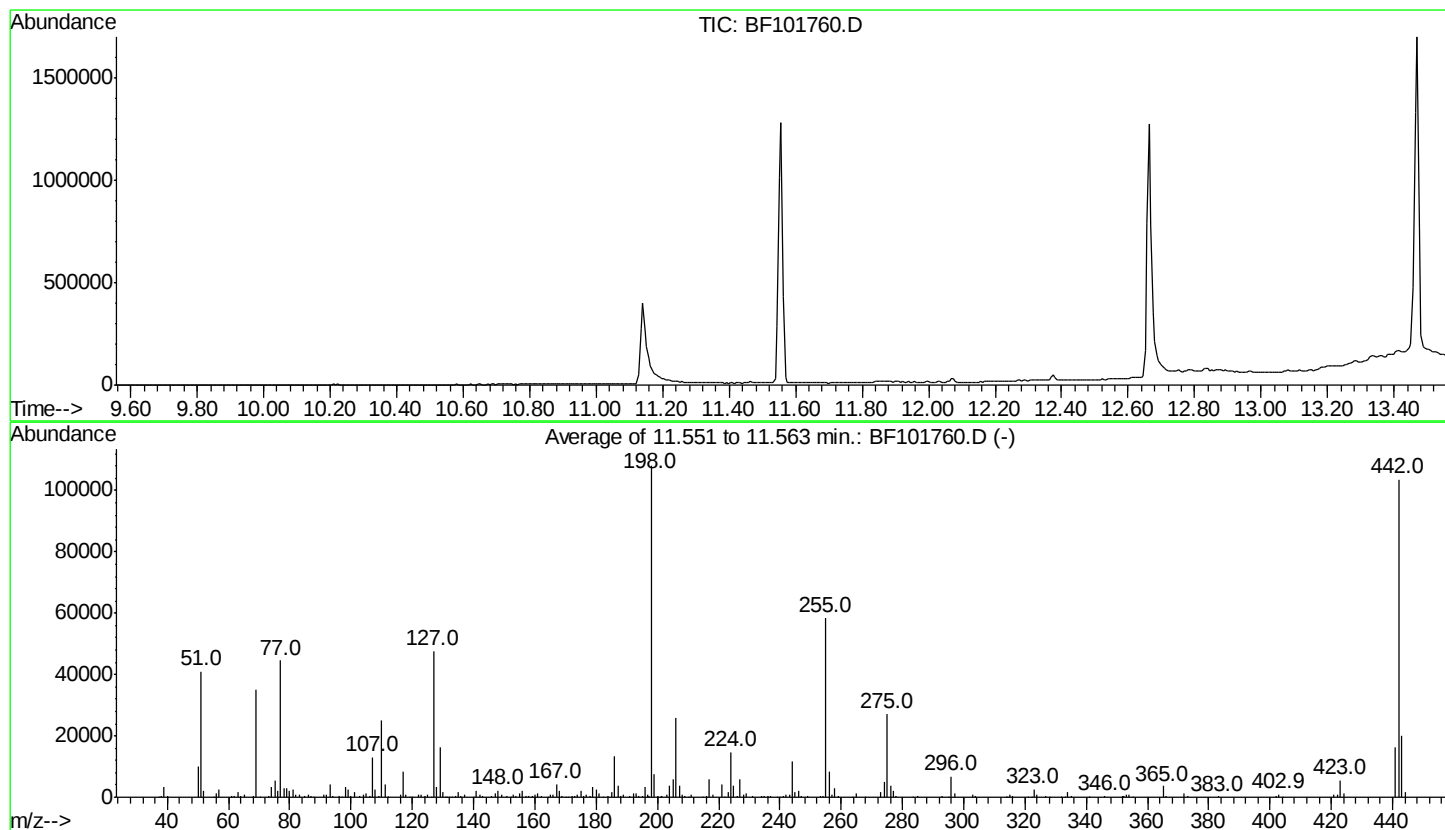

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	41038	PASS
68	69	0.00	2	1.7	610	PASS
69	198	0.00	100	32.3	34943	PASS
70	69	0.00	2	0.4	131	PASS
127	198	10	80	44.2	47772	PASS
197	198	0.00	2	0.6	693	PASS
198	198	100	100	100.0	108144	PASS
199	198	5	9	6.9	7455	PASS
275	198	10	60	25.2	27224	PASS
365	198	1	100	3.3	3612	PASS
441	443	0.01	100	81.3	16249	PASS
442	198	50	100	95.8	103632	PASS
443	442	15	24	19.3	19984	PASS