


Data Path : Z:\HPCHEM1\BNA F\Data\BF122717\
 Data File : BF101785.D
 Acq On : 28 Dec 2017 2:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 26 10:48:01 2017

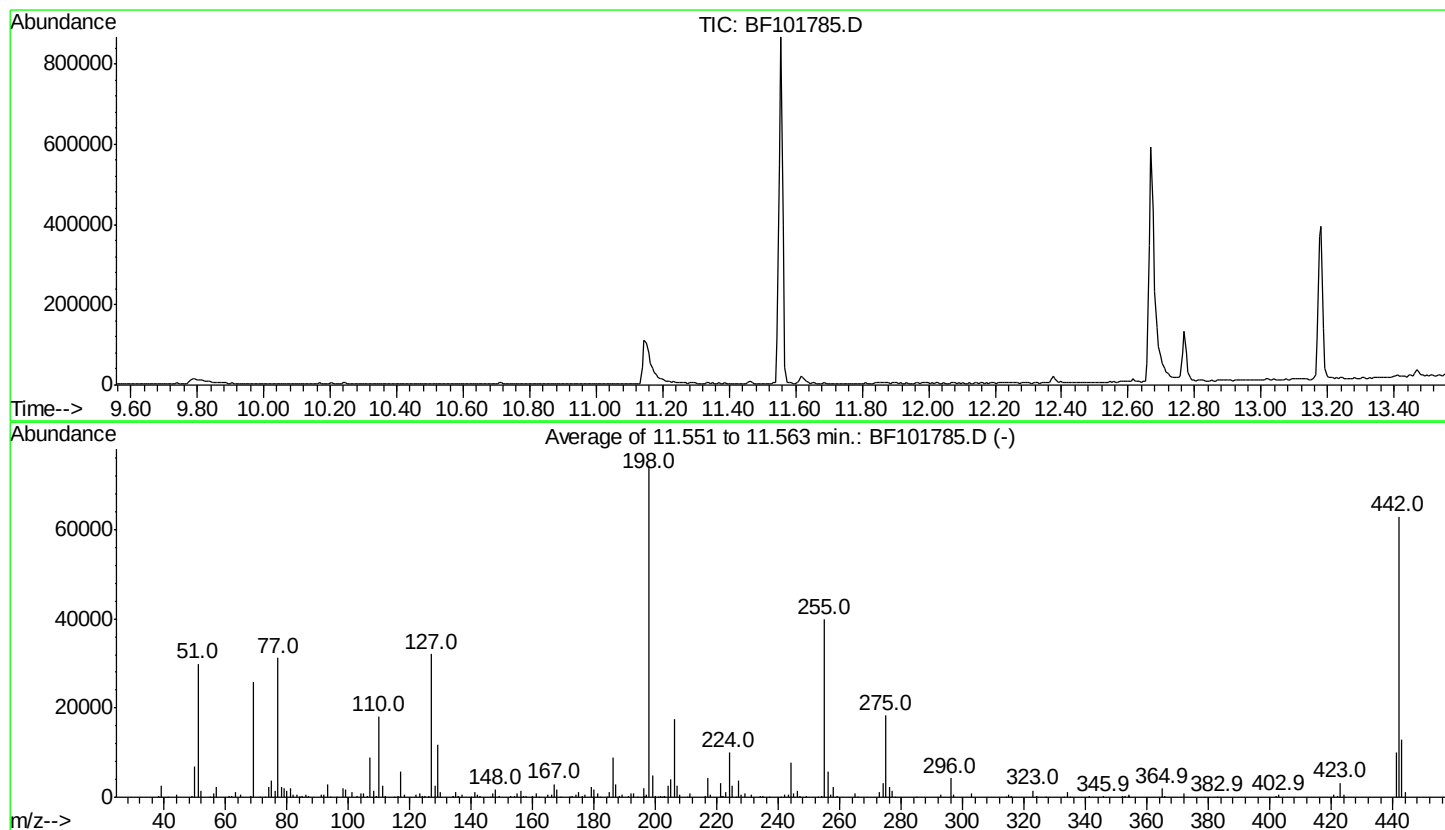

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	29933	PASS
68	69	0.00	2	1.6	417	PASS
69	198	0.00	100	34.7	25768	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	32106	PASS
197	198	0.00	2	0.6	450	PASS
198	198	100	100	100.0	74352	PASS
199	198	5	9	6.5	4824	PASS
275	198	10	60	24.6	18255	PASS
365	198	1	100	2.6	1962	PASS
441	443	0.01	100	77.7	9972	PASS
442	198	50	100	84.7	62944	PASS
443	442	15	24	20.4	12827	PASS