
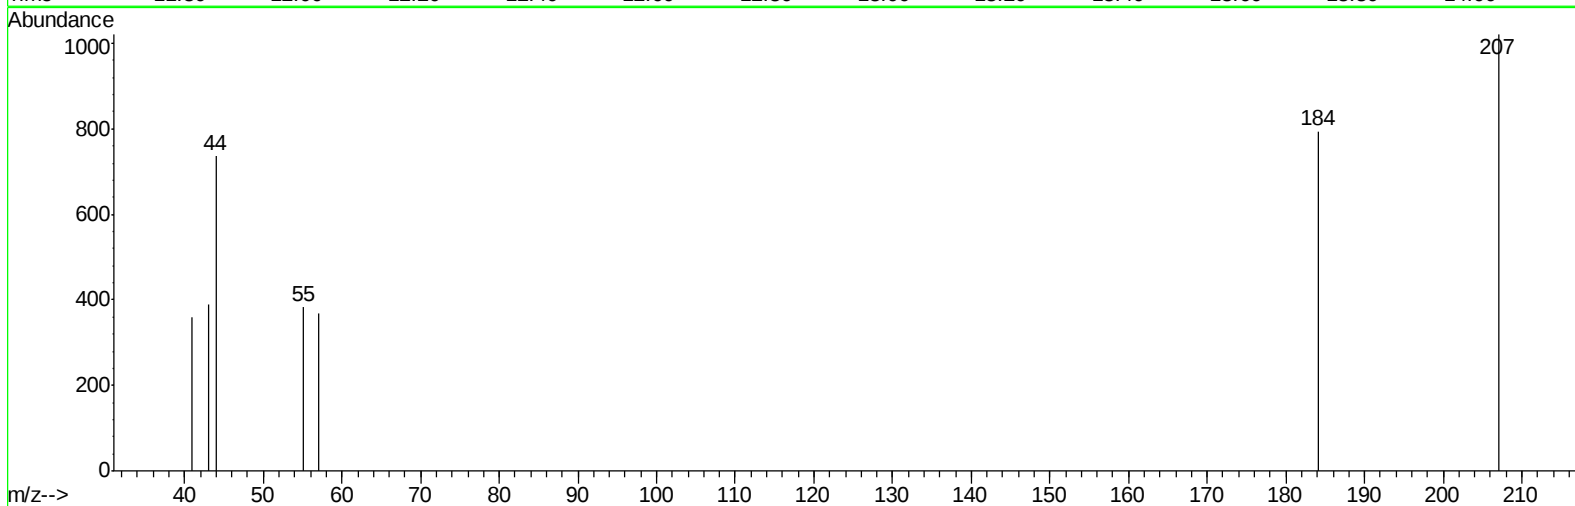


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF122719\
 Data File : BF118333.D
 Acq On : 27 Dec 2019 11:57
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:13:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 15:58:52 2019
 Response via : Initial Calibration

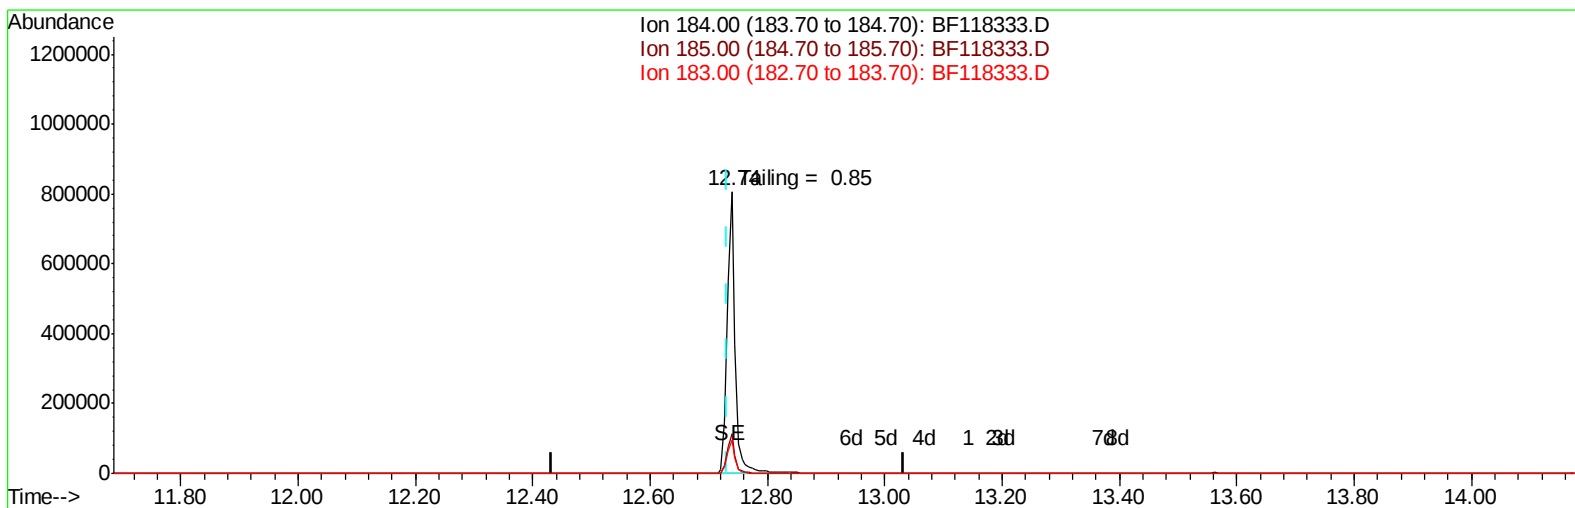

TIC: BF118333.D

(77) Benzidine



13.145min (+0.412) 367.93ng

response 1361

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	0.00#
183.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF122719\
Data File : BF118333.D
Acq On : 27 Dec 2019 11:57
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:13:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 15:58:52 2019
Response via : Initial Calibration

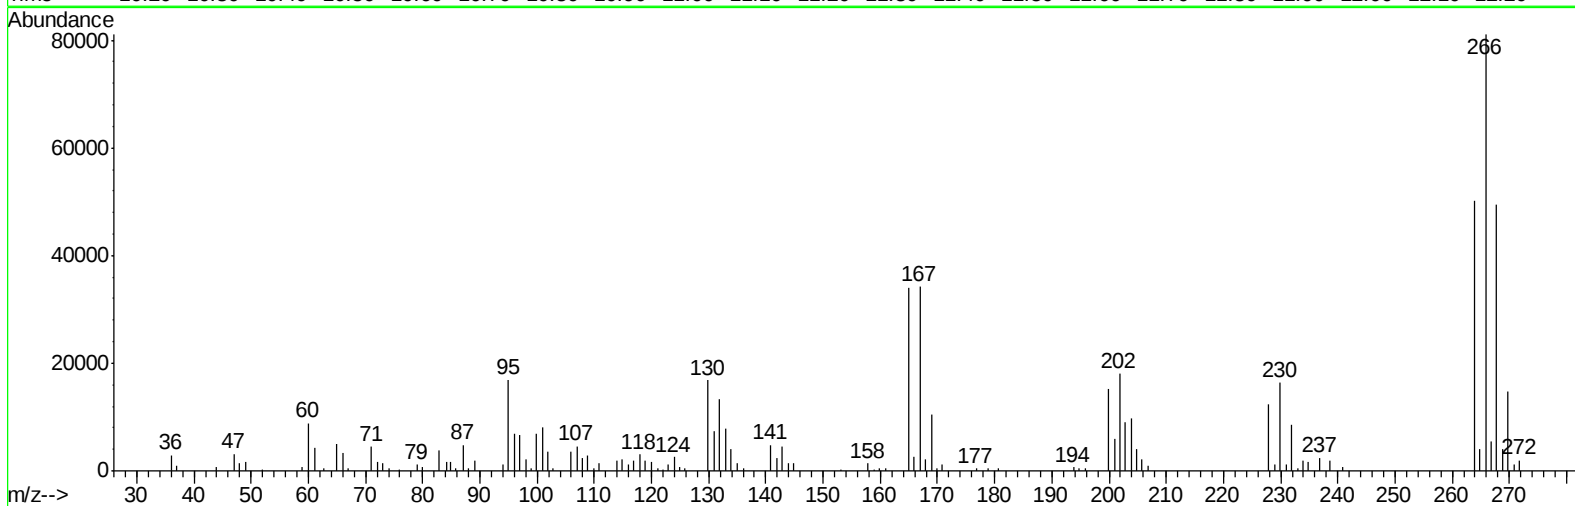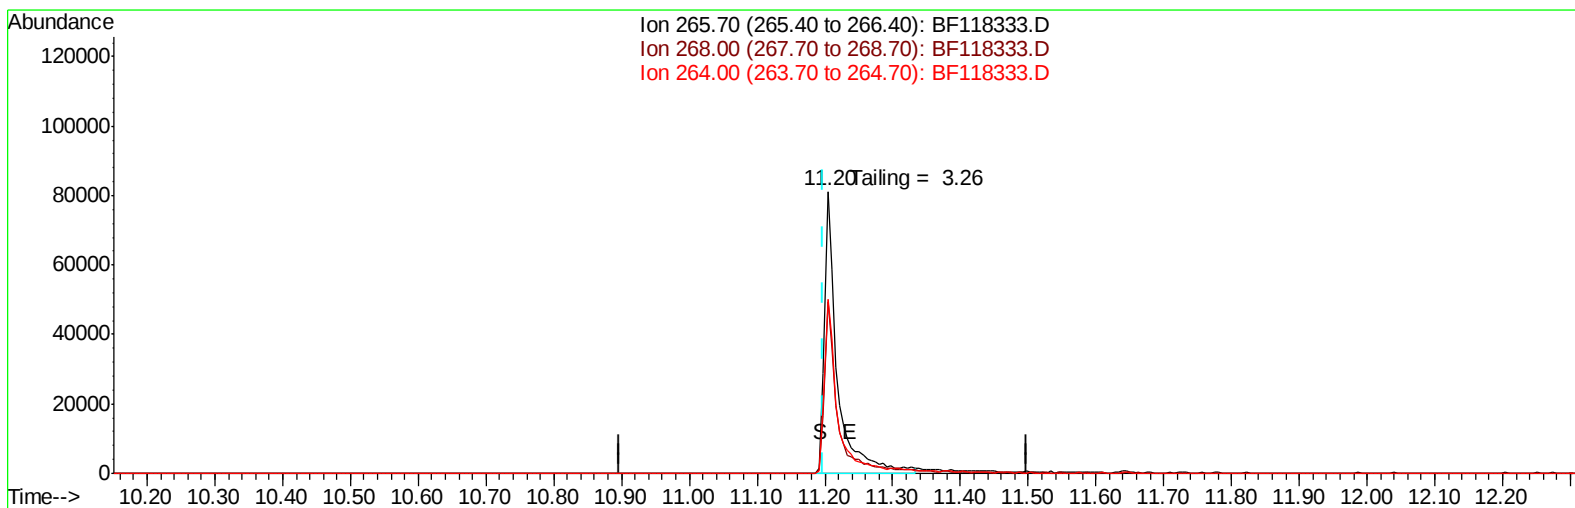

TIC: BF118333.D

(70) Pentachlorophenol (C)

11.204min (+0.006) 33034.17ng

response 103268

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	61.00
264.00	62.40	61.86
0.00	0.00	0.00