

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
 Data File : BF136749.D
 Acq On : 27 Dec 2023 10:13
 Operator : CG\JU
 Sample : PB158018BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB158018BL

Quant Time: Dec 27 10:58:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.787	152	82175	20.000	ng	0.00
21) Naphthalene-d8	8.057	136	315153	20.000	ng	-0.01
39) Acenaphthene-d10	9.816	164	159503	20.000	ng	-0.01
64) Phenanthrene-d10	11.310	188	288734	20.000	ng	0.00
76) Chrysene-d12	13.963	240	166101	20.000	ng	0.00
86) Perylene-d12	15.445	264	163583	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.440	112	662671	125.824	ng	0.01
7) Phenol-d6	6.434	99	830226	121.657	ng	0.00
23) Nitrobenzene-d5	7.345	82	509819	82.779	ng	-0.01
42) 2,4,6-Tribromophenol	10.616	330	207591	110.509	ng	0.00
45) 2-Fluorobiphenyl	9.139	172	987954	83.308	ng	-0.01
79) Terphenyl-d14	12.910	244	909711	76.537	ng	0.00
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.345	70	68279	16.505	ng	# 75
25) Isophorone	7.345	82	508153	45.344	ng	# 65
50) Dimethylphthalate	9.816	163	30090	2.583	ng	# 1
51) 2,6-Dinitrotoluene	9.816	165	19914	7.531	ng	# 30
57) 2,4-Dinitrotoluene	9.816	165	19914	5.802	ng	# 21
67) 4-Bromophenyl-phenylether	10.616	248	12246	3.819	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
Data File : BF136749.D
Acq On : 27 Dec 2023 10:13
Operator : CG\JU
Sample : PB158018BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158018BL

Quant Time: Dec 27 10:58:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration



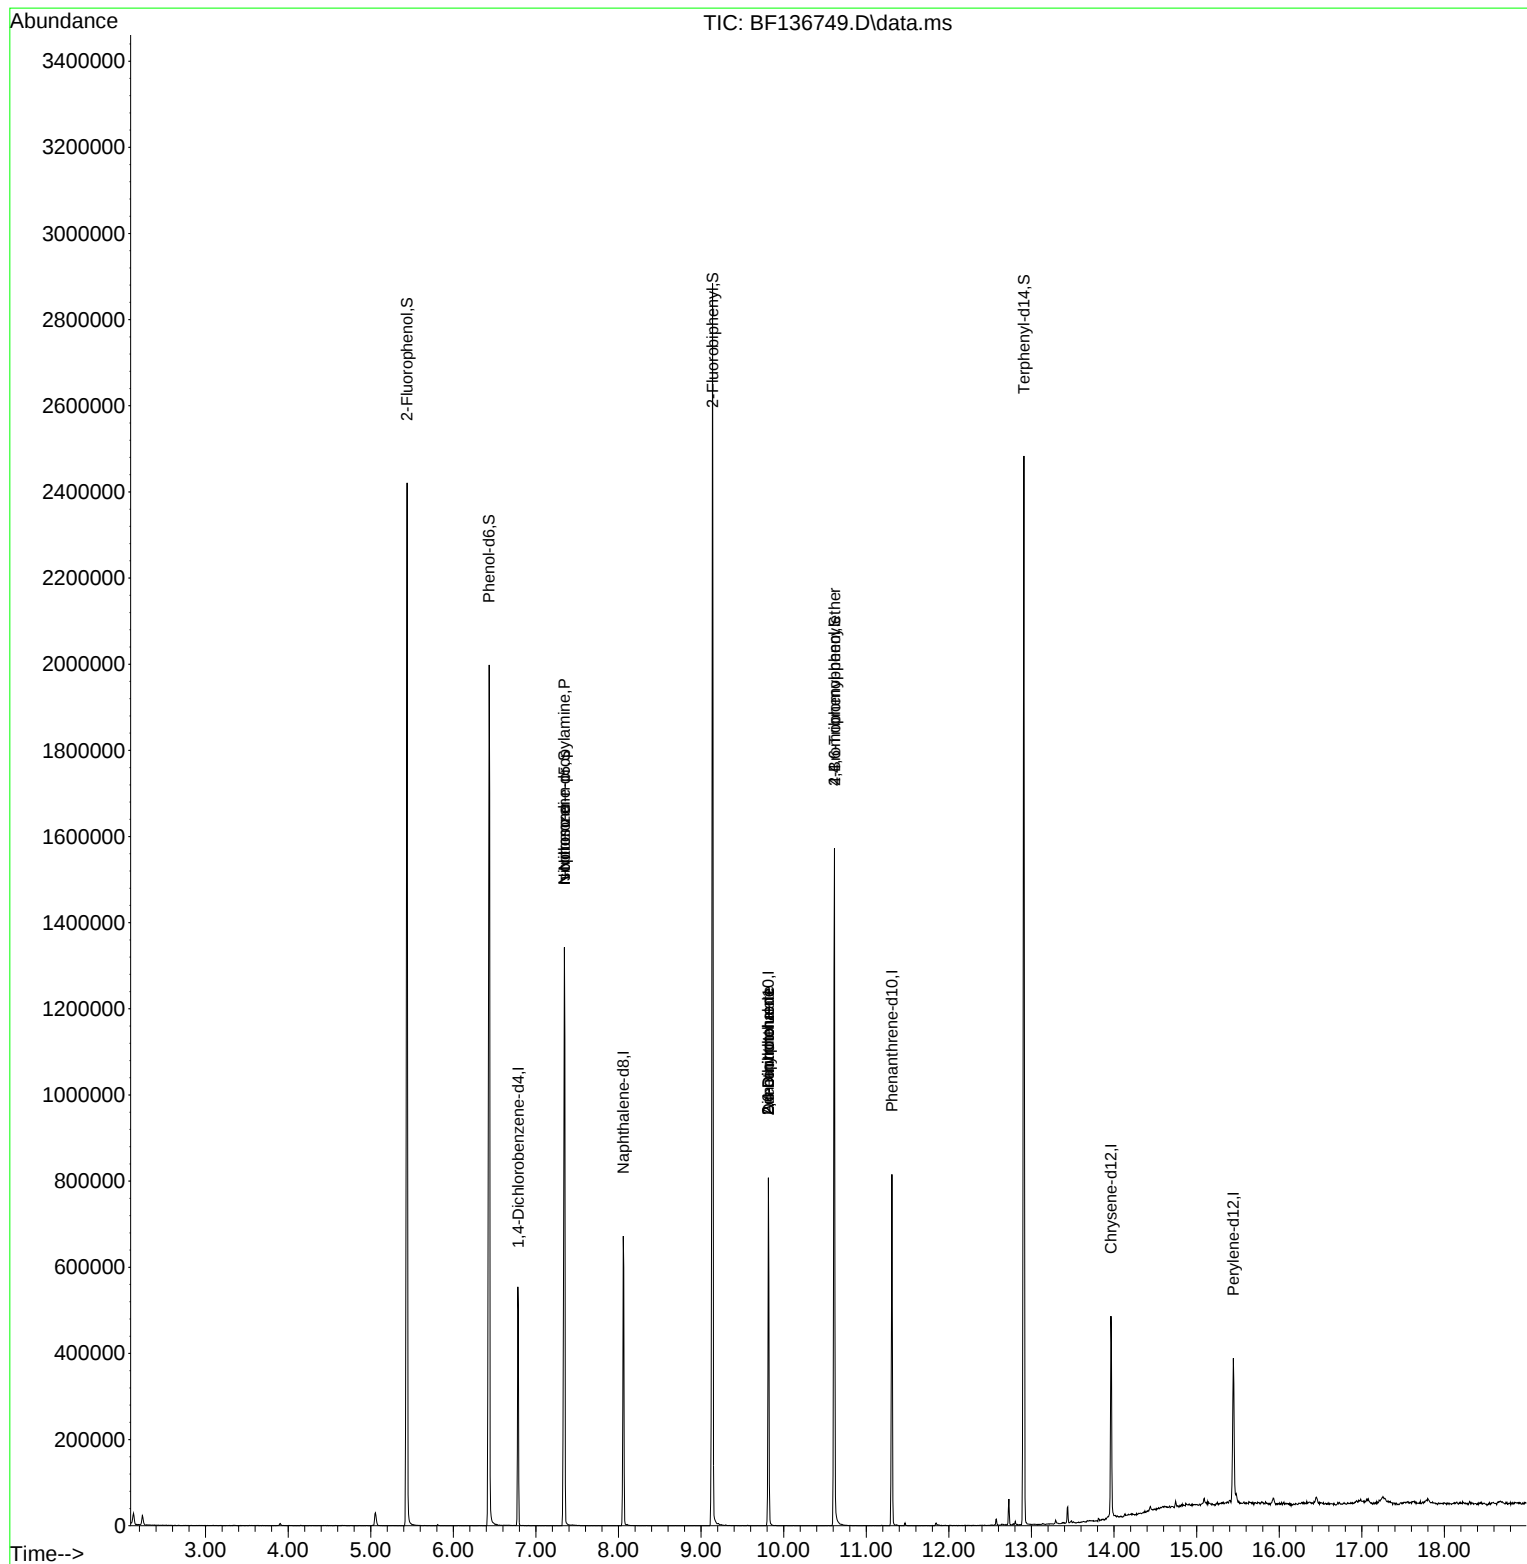




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.787 min Scan# 71
 Delta R.T. -0.005 min
 Lab File: BF136749.D
 Acq: 27 Dec 2023 10:13




Instrument :
 BNA_F
 ClientSampleId :
 PB158018BL


Tgt Ion:152 Resp: 82175
 Ion Ratio Lower Upper
 152 100
 150 154.5 127.0 190.6
 115 56.0 49.0 73.4

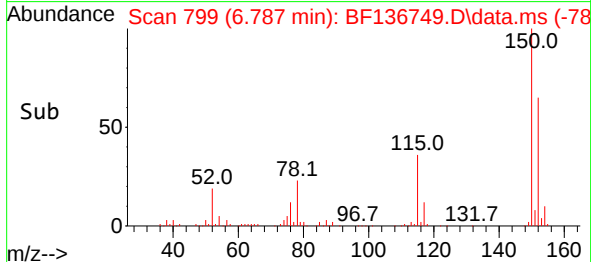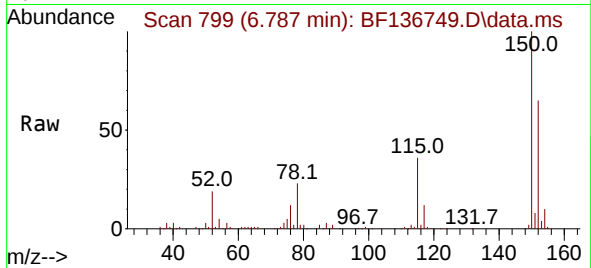

#5
 2-Fluorophenol
 Concen: 125.824 ng
 RT: 5.440 min Scan# 570
 Delta R.T. 0.012 min
 Lab File: BF136749.D
 Acq: 27 Dec 2023 10:13

Tgt Ion:112 Resp: 662671
 Ion Ratio Lower Upper
 112 100
 64 63.0 51.1 76.7
 63 31.8 26.1 39.1


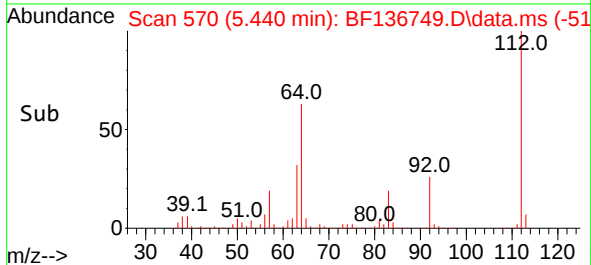

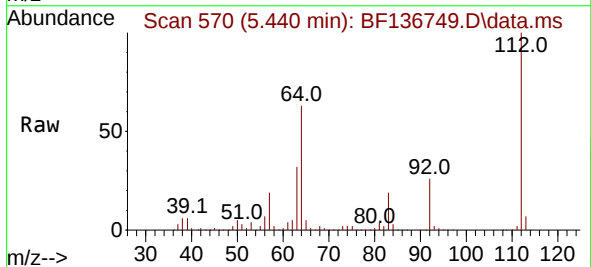


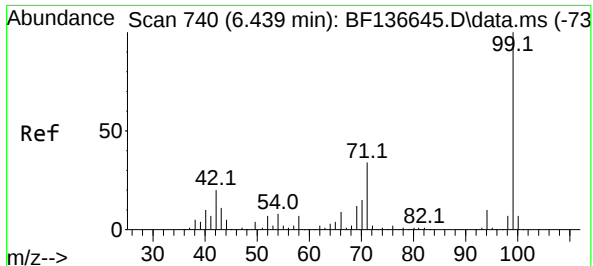

#7
Phenol-d6
Concen: 121.657 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13




Instrument :
BNA_F
ClientSampleId :
PB158018BL


Tgt Ion: 99 Resp: 830226
Ion Ratio Lower Upper
99 100
42 20.2 16.1 24.1
71 33.2 27.4 41.2

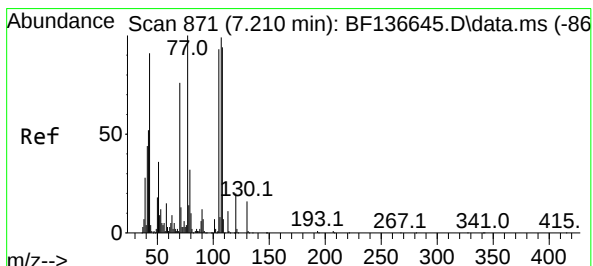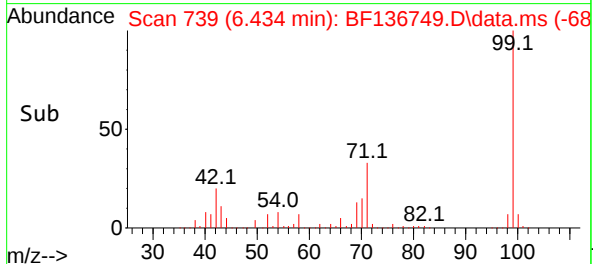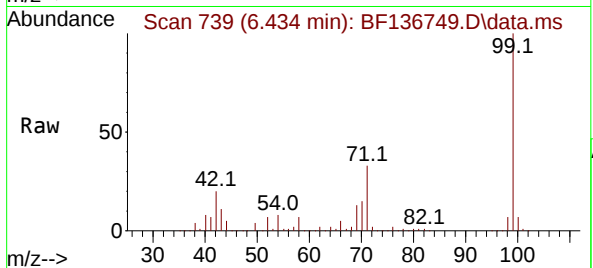

#19
n-Nitroso-di-n-propylamine
Concen: 16.505 ng
RT: 7.345 min Scan# 894
Delta R.T. 0.135 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Tgt Ion: 70 Resp: 68279
Ion Ratio Lower Upper
70 100
42 51.3 54.2 81.4#
101 0.0 7.6 11.4#
130 2.3 17.1 25.7#

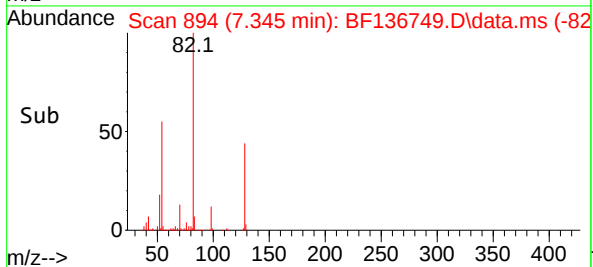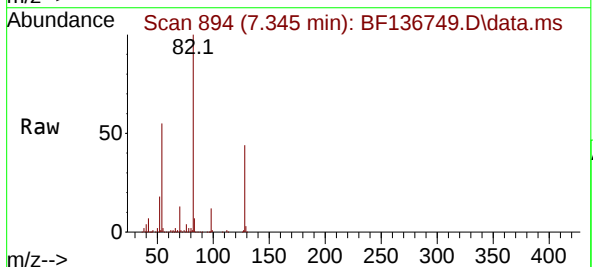



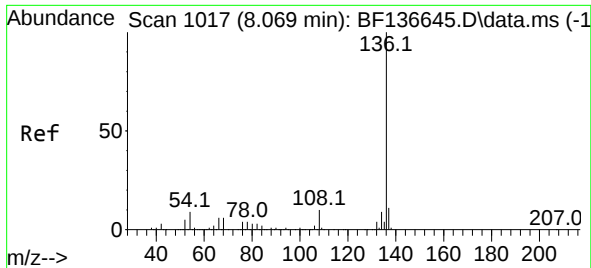


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 1017
Delta R.T. -0.012 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Instrument :
BNA_F
ClientSampleId :
PB158018BL

Tgt Ion:136 Resp: 315153




Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.0	13.4
54	9.0	7.2	10.8
68	6.0	4.9	7.3

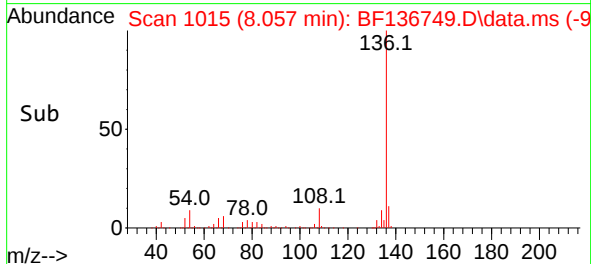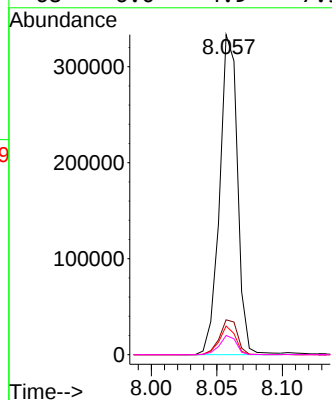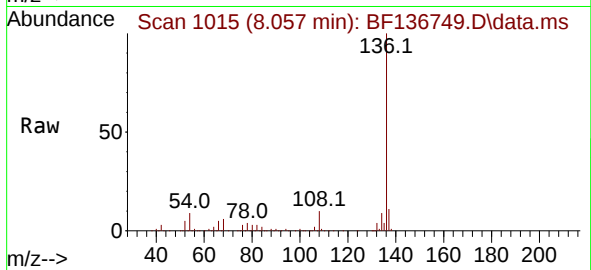

#23
Nitrobenzene-d5
Concen: 82.779 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.012 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Tgt Ion: 82 Resp: 509819

Ion	Ratio	Lower	Upper
82	100		
128	44.0	35.3	52.9
54	55.3	44.5	66.7


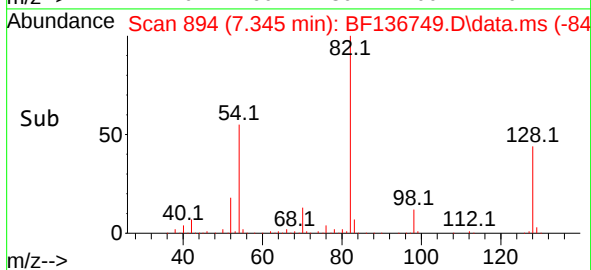
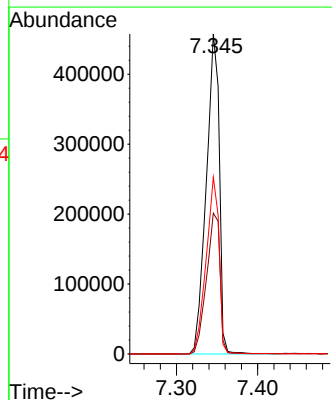
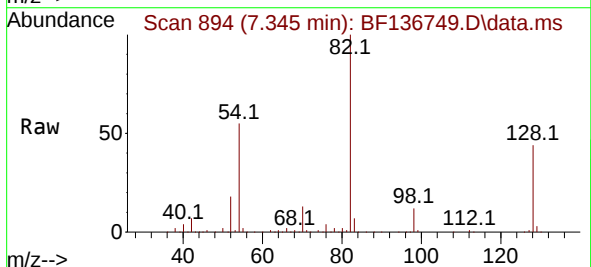




#25
Isophorone
Concen: 45.344 ng
RT: 7.345 min Scan# 894
Delta R.T. -0.270 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13




Instrument :
BNA_F
ClientSampleId :
PB158018BL

Tgt Ion: 82 Resp: 508153
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 14.5 21.7#

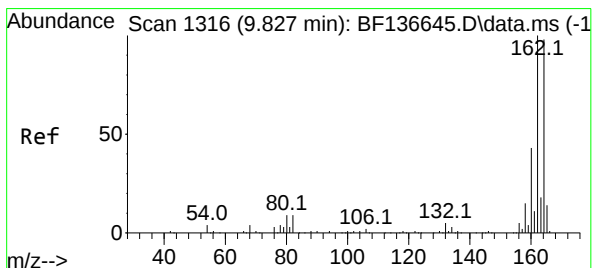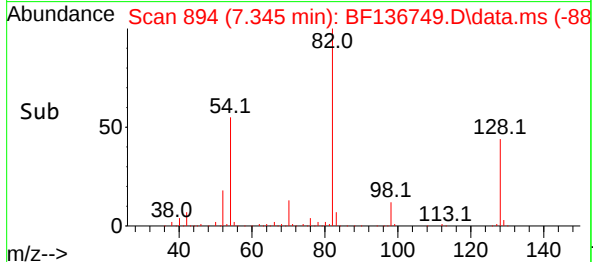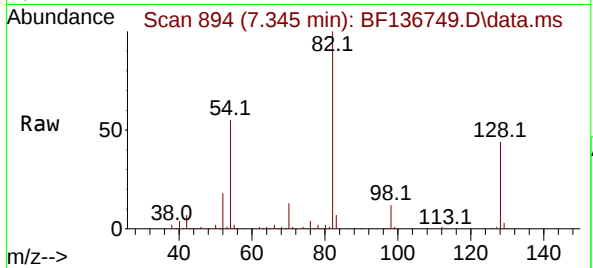

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.816 min Scan# 1314
Delta R.T. -0.012 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Tgt Ion:164 Resp: 159503
Ion Ratio Lower Upper
164 100
162 101.6 81.6 122.4
160 46.4 34.9 52.3

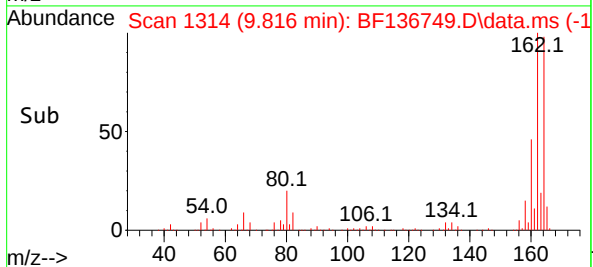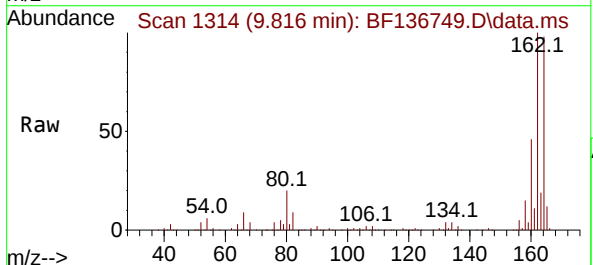



#42

2,4,6-Tribromophenol

Concen: 110.509 ng

RT: 10.616 min Scan# 1451

Delta R.T. -0.006 min

Lab File: BF136749.D

Acq: 27 Dec 2023 10:13

Instrument :

BNA_F

ClientSampleId :

PB158018BL




Tgt Ion:330 Resp: 207591

Ion Ratio Lower Upper

330 100

332 97.6 77.4 116.0

141 28.7 23.4 35.2

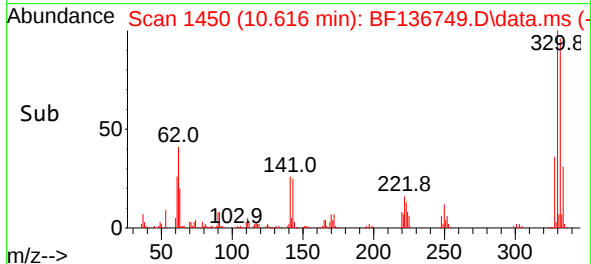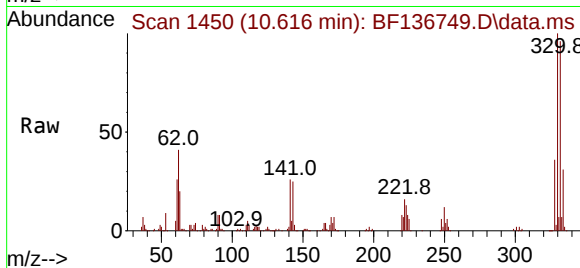

#45

2-Fluorobiphenyl

Concen: 83.308 ng

RT: 9.139 min Scan# 1199

Delta R.T. -0.012 min

Lab File: BF136749.D

Acq: 27 Dec 2023 10:13




Tgt Ion:172 Resp: 987954

Ion Ratio Lower Upper

172 100

171 36.0 29.0 43.6

170 23.3 19.0 28.4

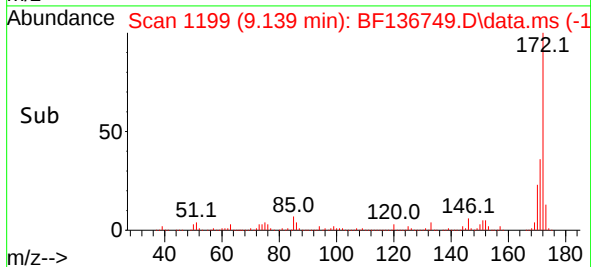

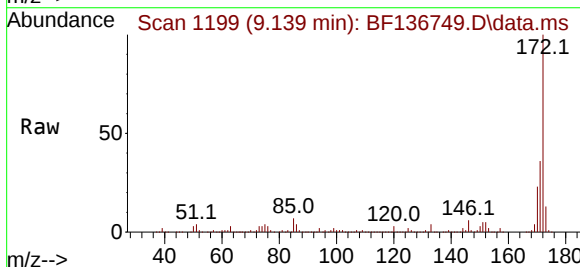




#50
Dimethylphthalate
Concen: 2.583 ng
RT: 9.816 min Scan# 11
Delta R.T. 0.259 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13




Instrument :
BNA_F
ClientSampleId :
PB158018BL

Tgt Ion:163 Resp: 30090
Ion Ratio Lower Upper
163 100
194 0.0 3.3 4.9#
164 509.2 7.8 11.6#

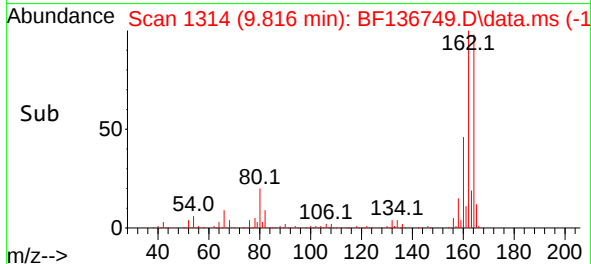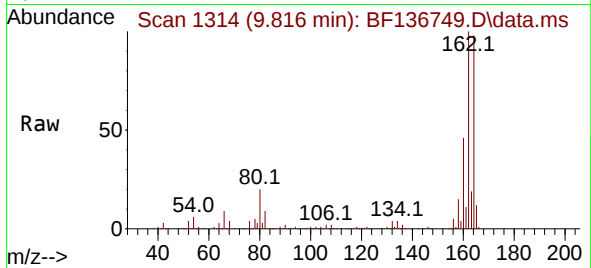

#51
2,6-Dinitrotoluene
Concen: 7.531 ng
RT: 9.816 min Scan# 1314
Delta R.T. 0.194 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Tgt Ion:165 Resp: 19914
Ion Ratio Lower Upper
165 100
63 1.3 39.8 59.6#
89 1.1 38.8 58.2#


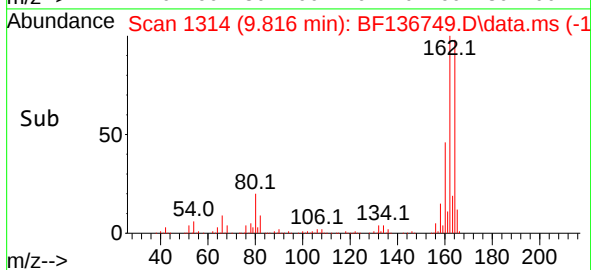

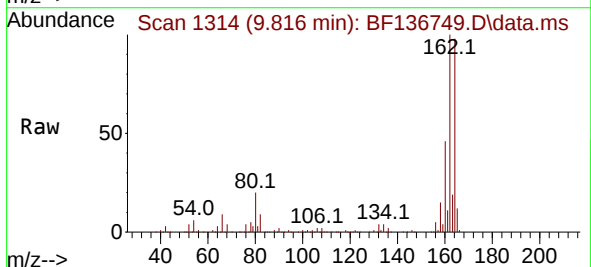




#57
2,4-Dinitrotoluene
Concen: 5.802 ng
RT: 9.816 min Scan# 11
Delta R.T. -0.206 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13




Instrument :
BNA_F
ClientSampleId :
PB158018BL


Tgt Ion:165	Resp:	19914
Ion Ratio	Lower	Upper
165	100	
63	1.3	41.0 61.6#
89	1.1	59.9 89.9#
182	0.0	2.0 3.0#

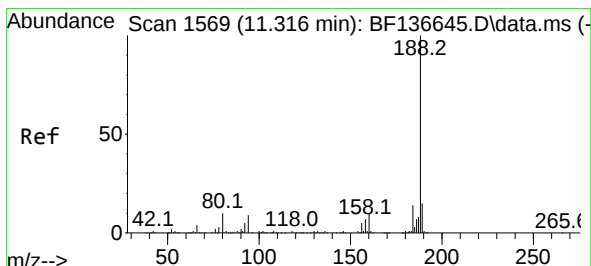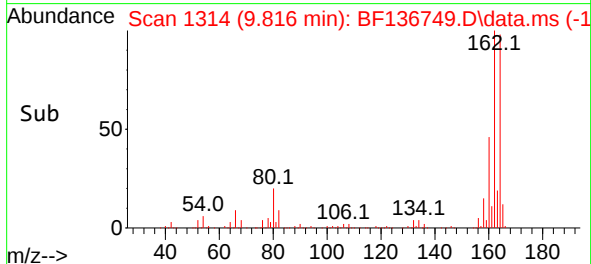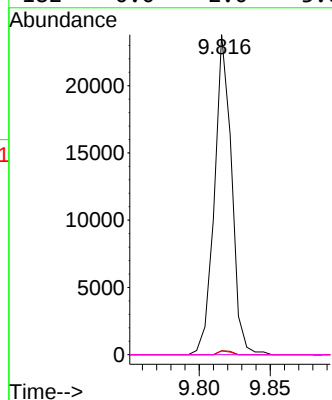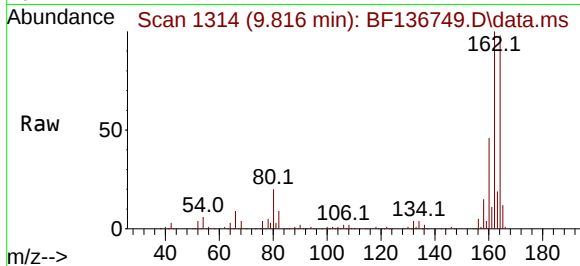

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Tgt Ion:188	Resp:	288734
Ion Ratio	Lower	Upper
188	100	
94	9.1	7.5 11.3
80	9.6	8.1 12.1


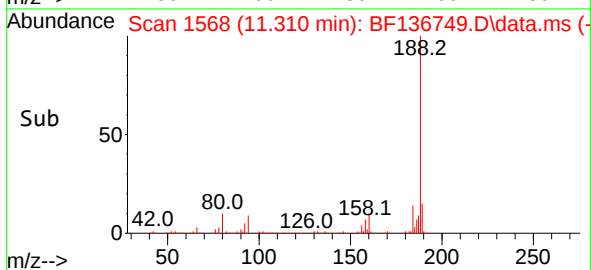
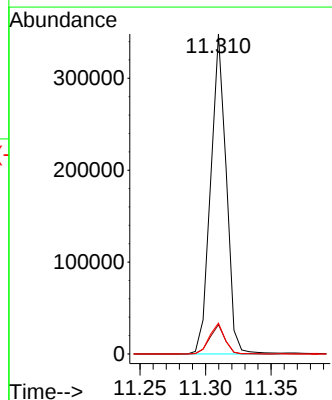
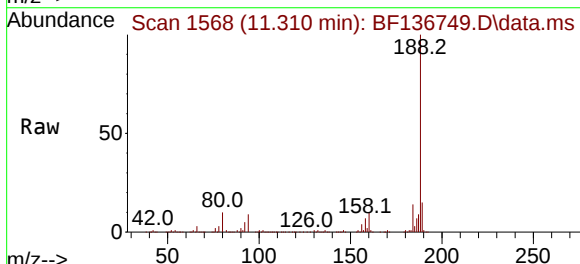


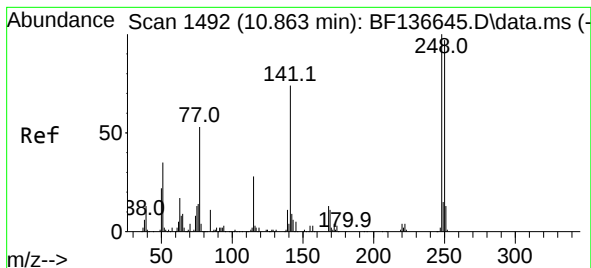

#67
4-Bromophenyl-phenylether
Concen: 3.819 ng
RT: 10.616 min Scan# 1492
Delta R.T. -0.247 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13




Instrument :
BNA_F
ClientSampleId :
PB158018BL


Tgt Ion:248 Resp: 12246
Ion Ratio Lower Upper
248 100
250 210.2 77.8 116.6#
141 455.1 59.2 88.8#

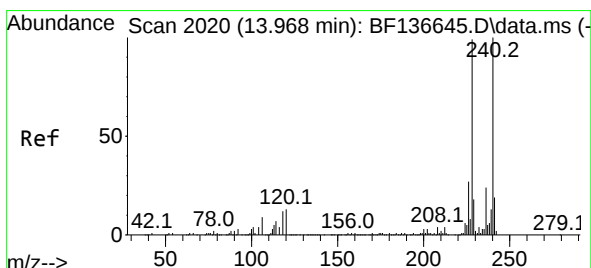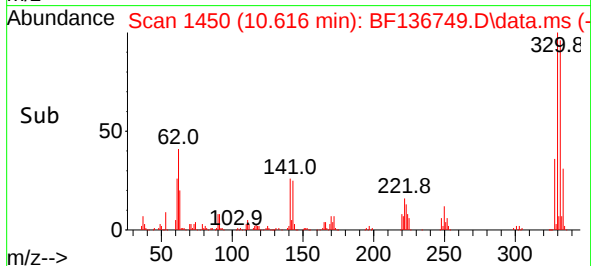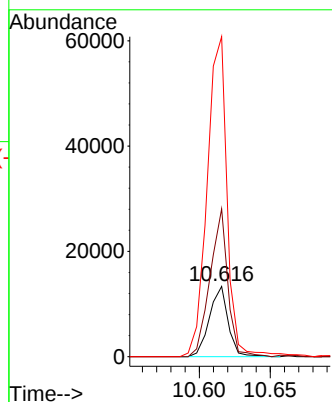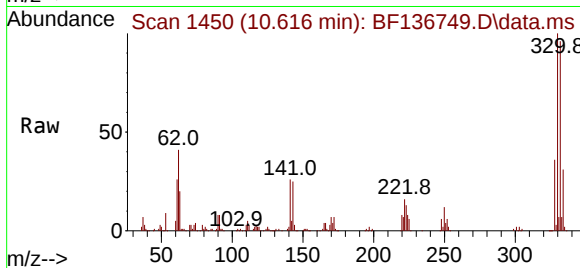

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.963 min Scan# 2019
Delta R.T. -0.006 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13


Tgt Ion:240 Resp: 166101
Ion Ratio Lower Upper
240 100
120 11.2 10.3 15.5
236 24.4 19.4 29.2

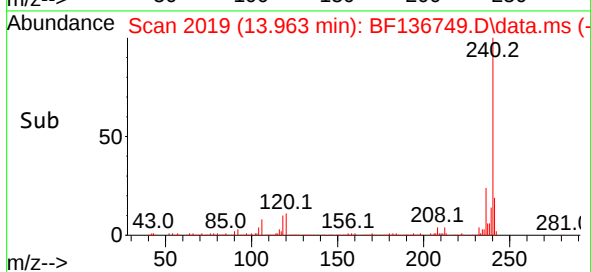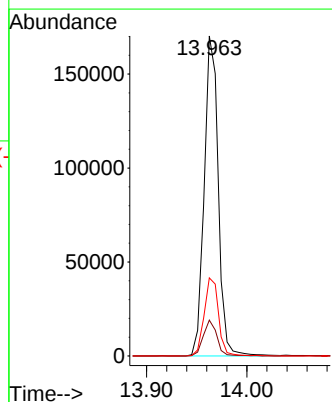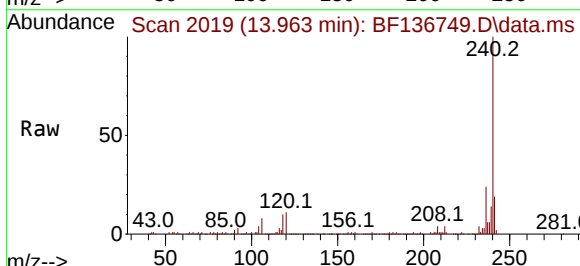



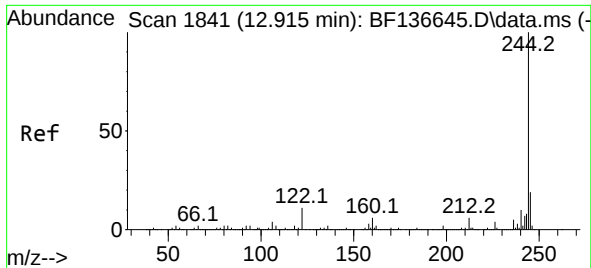


#79
Terphenyl-d14
Concen: 76.537 ng
RT: 12.910 min Scan# 1841
Delta R.T. -0.006 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Instrument :
BNA_F
ClientSampleId :
PB158018BL

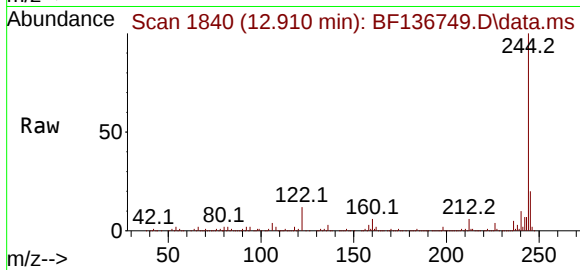

Tgt Ion:244 Resp: 909711
Ion Ratio Lower Upper
244 100
212 6.3 5.0 7.4
122 11.6 9.0 13.4

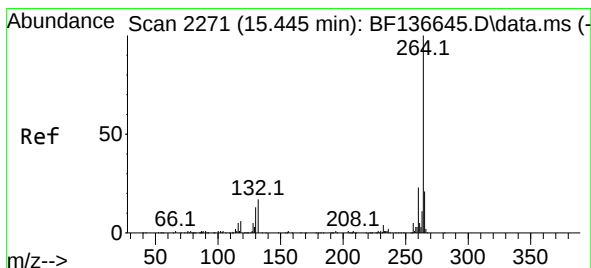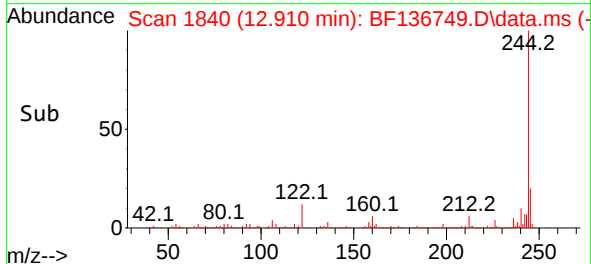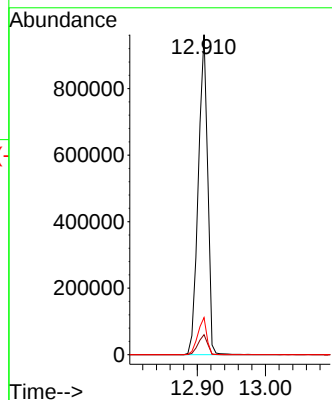

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.445 min Scan# 2271
Delta R.T. 0.000 min
Lab File: BF136749.D
Acq: 27 Dec 2023 10:13

Tgt Ion:264 Resp: 163583
Ion Ratio Lower Upper
264 100
260 23.4 18.3 27.5
265 20.9 17.0 25.6

