
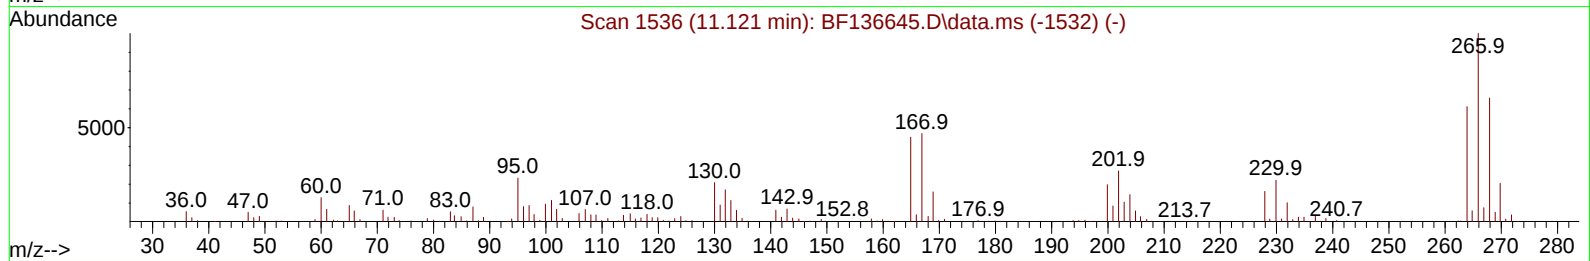
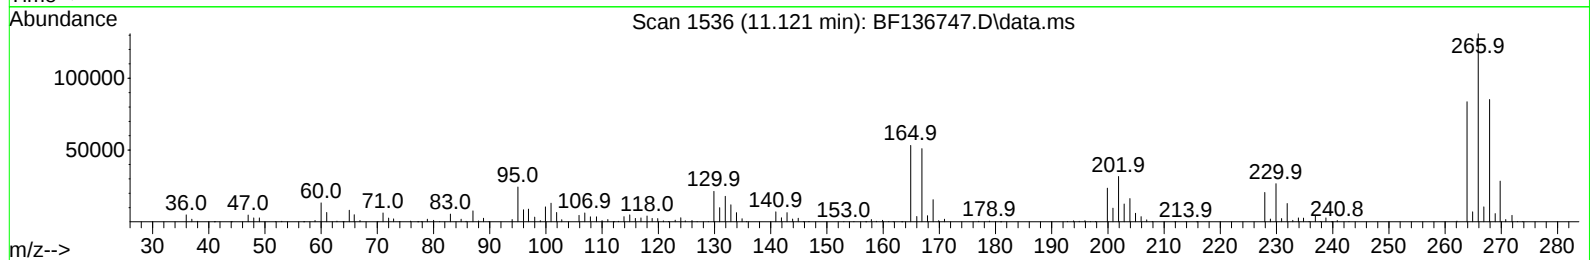


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
 Data File : BF136747.D
 Acq On : 27 Dec 2023 09:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 11:00:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

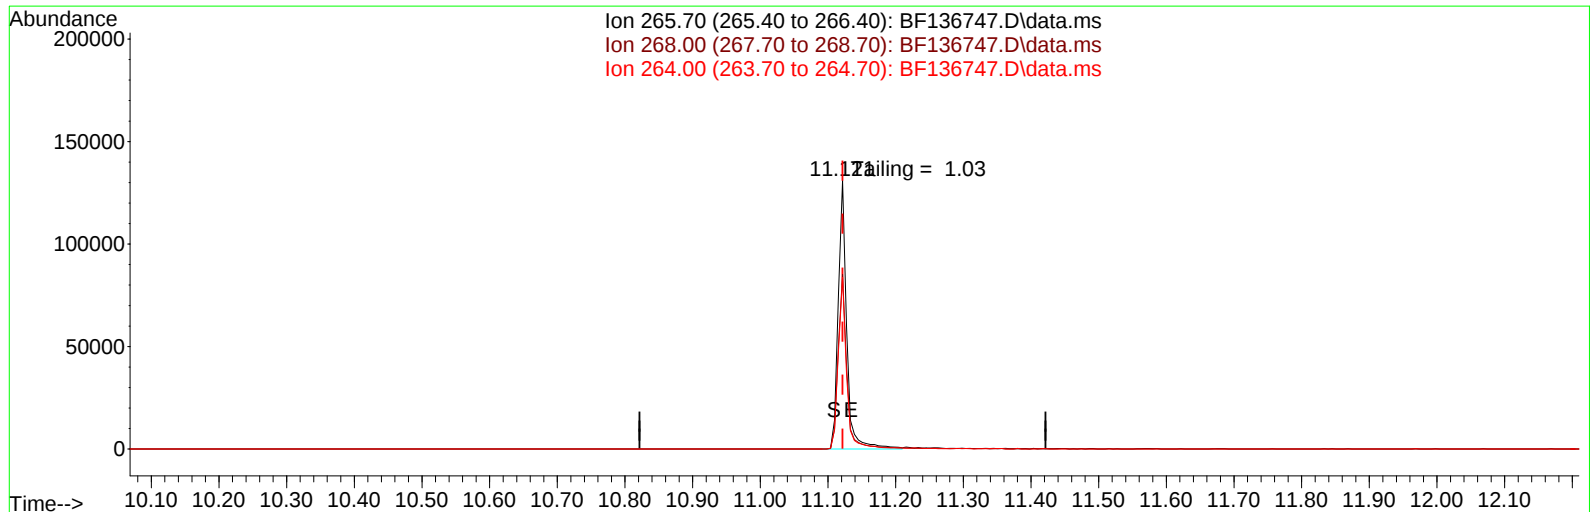

TIC: BF136747.D\data.ms

(70) Pentachlorophenol (C)




11.121min (-0.000) 38903.92 ng

response 114907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.03
264.00	61.20	63.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
Data File : BF136747.D
Acq On : 27 Dec 2023 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 11:00:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

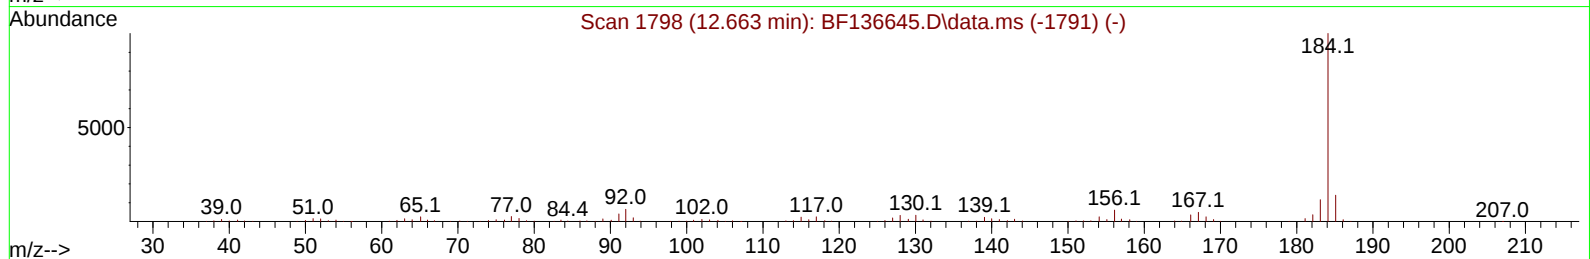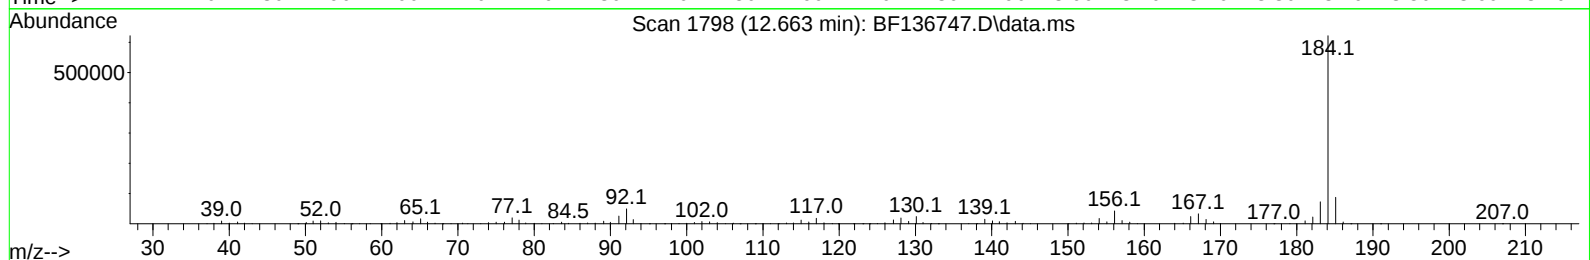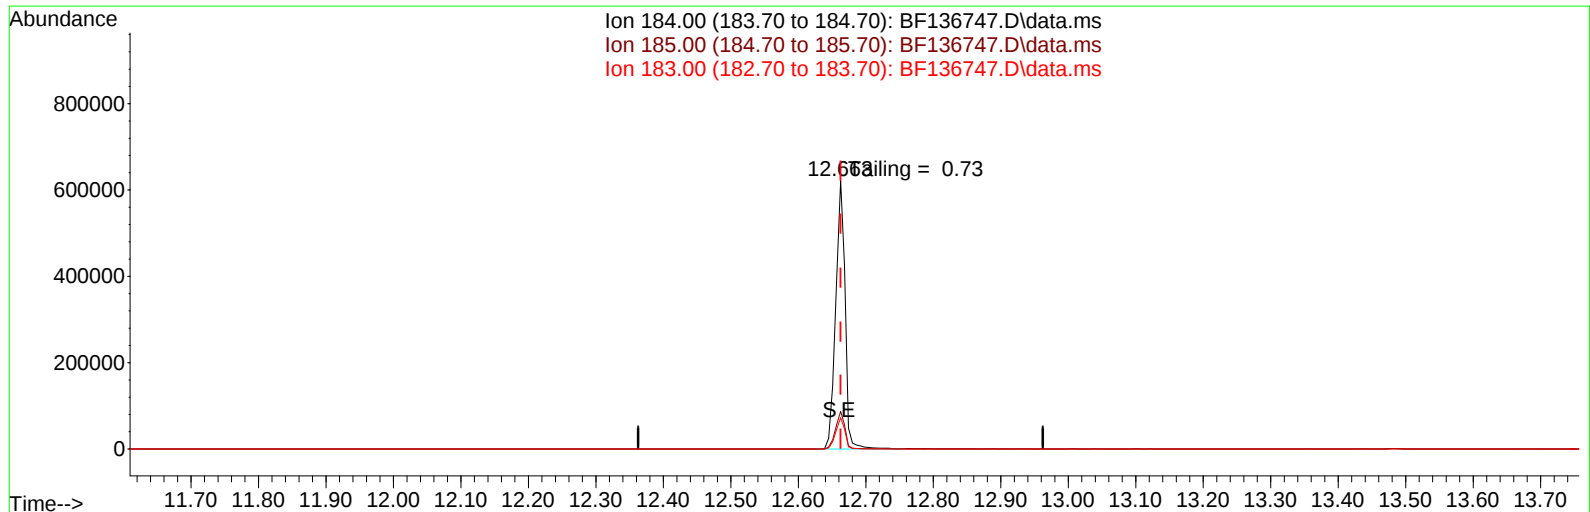

TIC: BF136747.D\data.ms

(77) Benzidine

12.663min (0.000) 347377.02 ng

response 604317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	11.60	11.69
0.00	0.00	0.00