
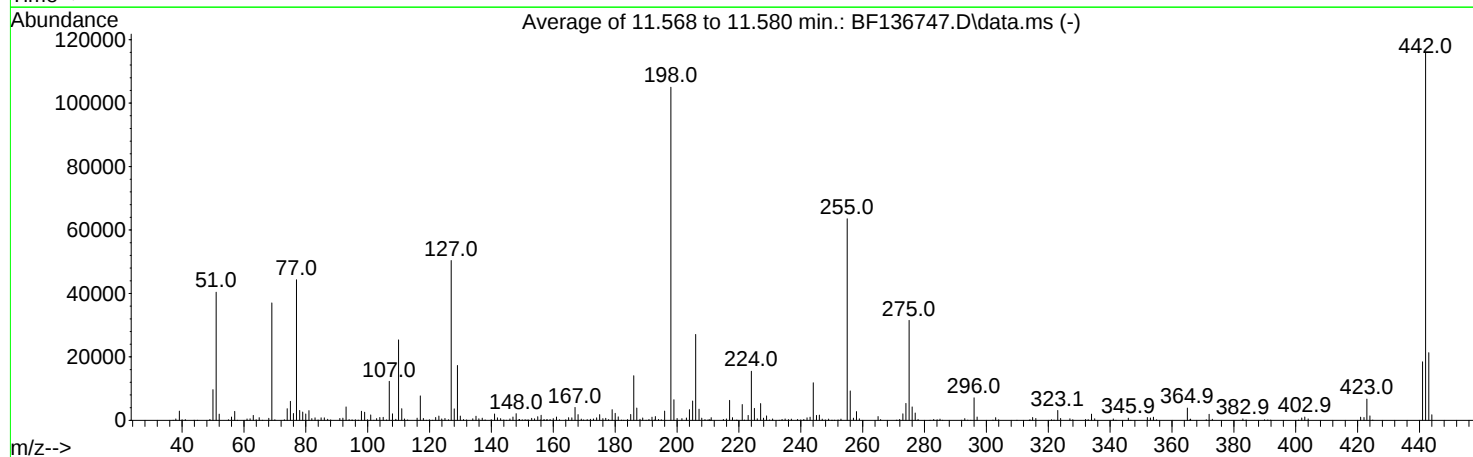


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
Data File : BF136747.D
Acq On : 27 Dec 2023 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

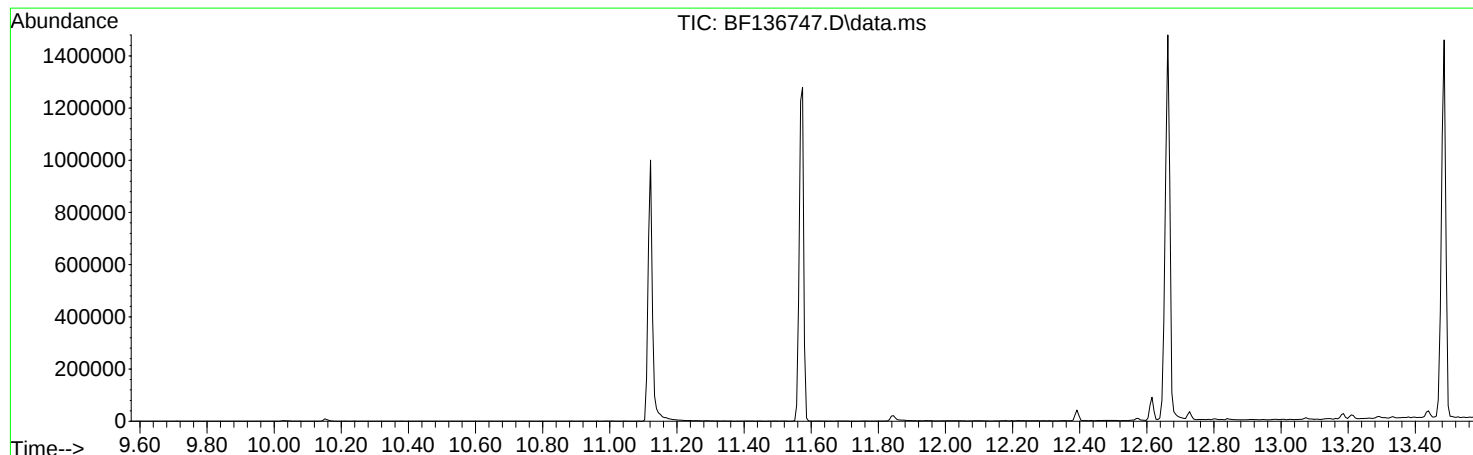




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	40407	PASS
68	69	0.00	2	1.7	639	PASS
69	198	0.00	100	35.3	37047	PASS
70	69	0.00	2	0.6	208	PASS
127	198	10	80	48.0	50411	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104981	PASS
199	198	5	9	6.2	6518	PASS
275	198	10	60	30.0	31517	PASS
365	198	1	100	3.7	3869	PASS
441	198	0.01	100	17.6	18444	PASS
442	442	50	100	100.0	115949	PASS
443	442	15	24	18.4	21351	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
Data File : BF136747.D
Acq On : 27 Dec 2023 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 11:00:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

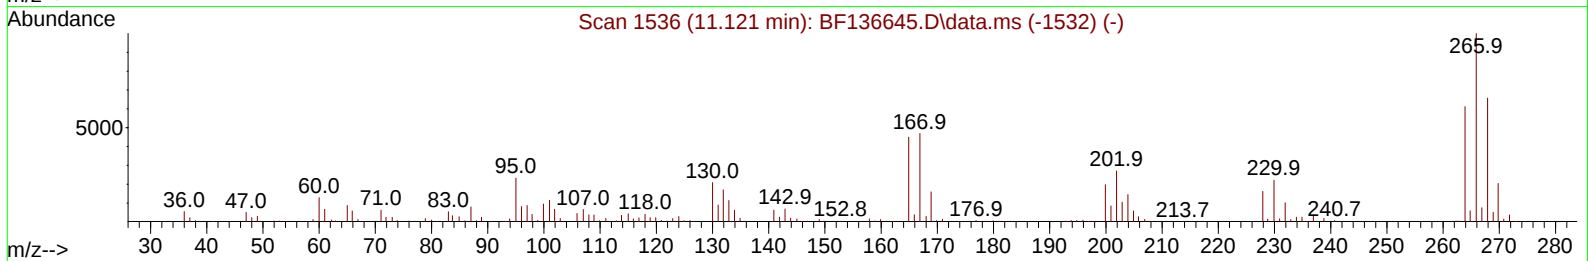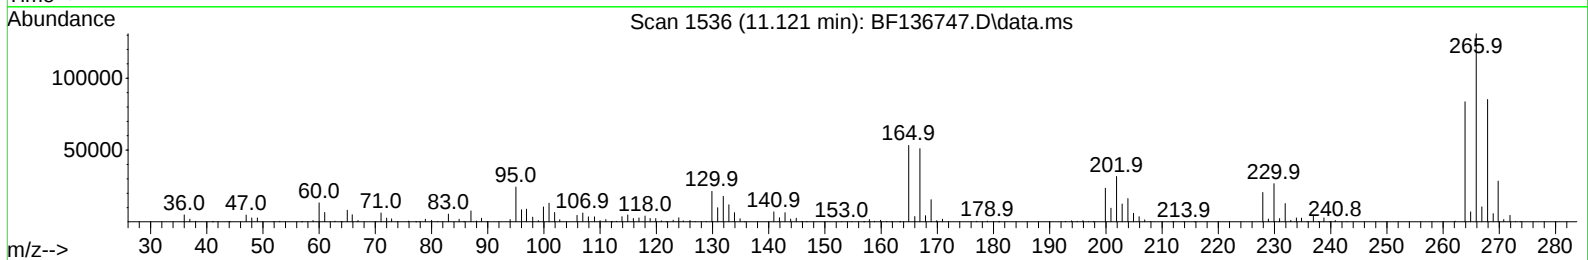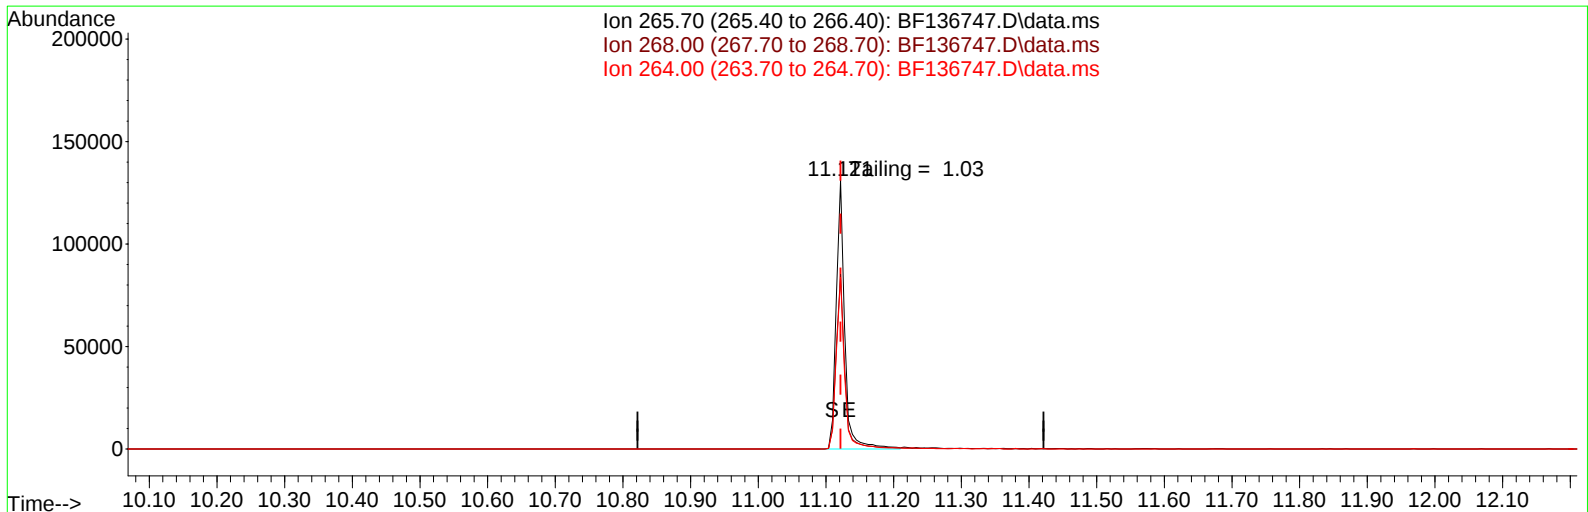

TIC: BF136747.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.000) 38903.92 ng




response 114907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.03
264.00	61.20	63.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
Data File : BF136747.D
Acq On : 27 Dec 2023 09:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 11:00:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

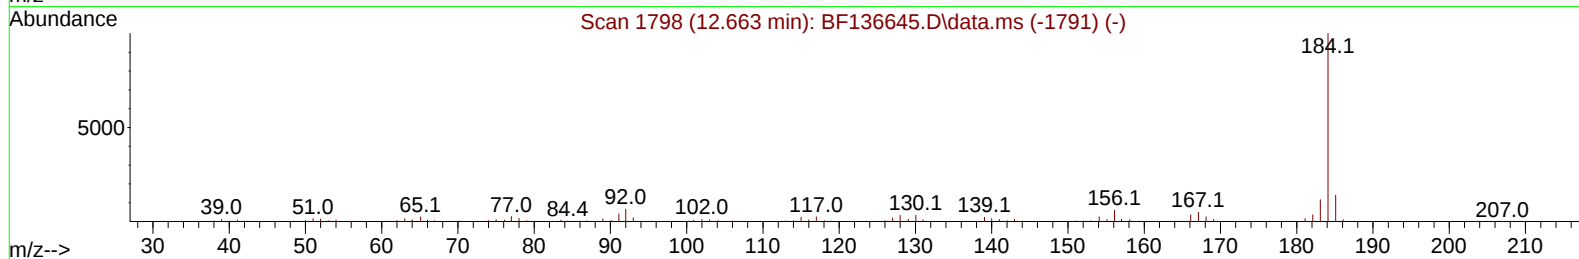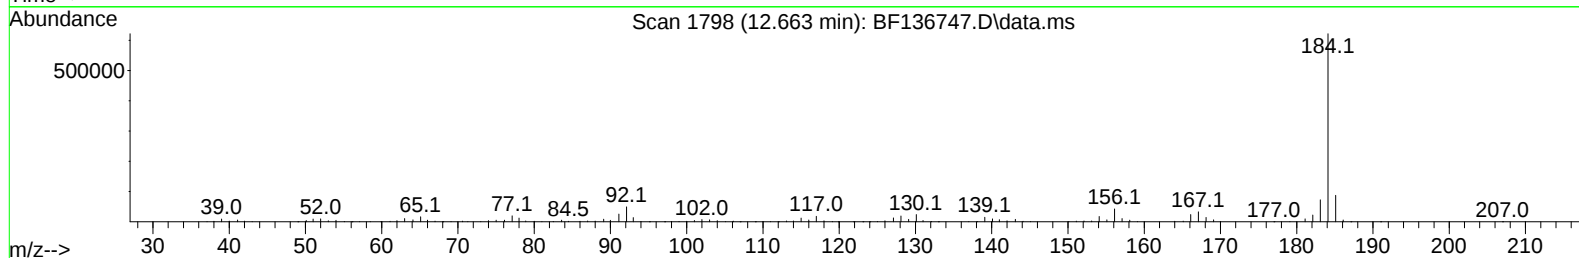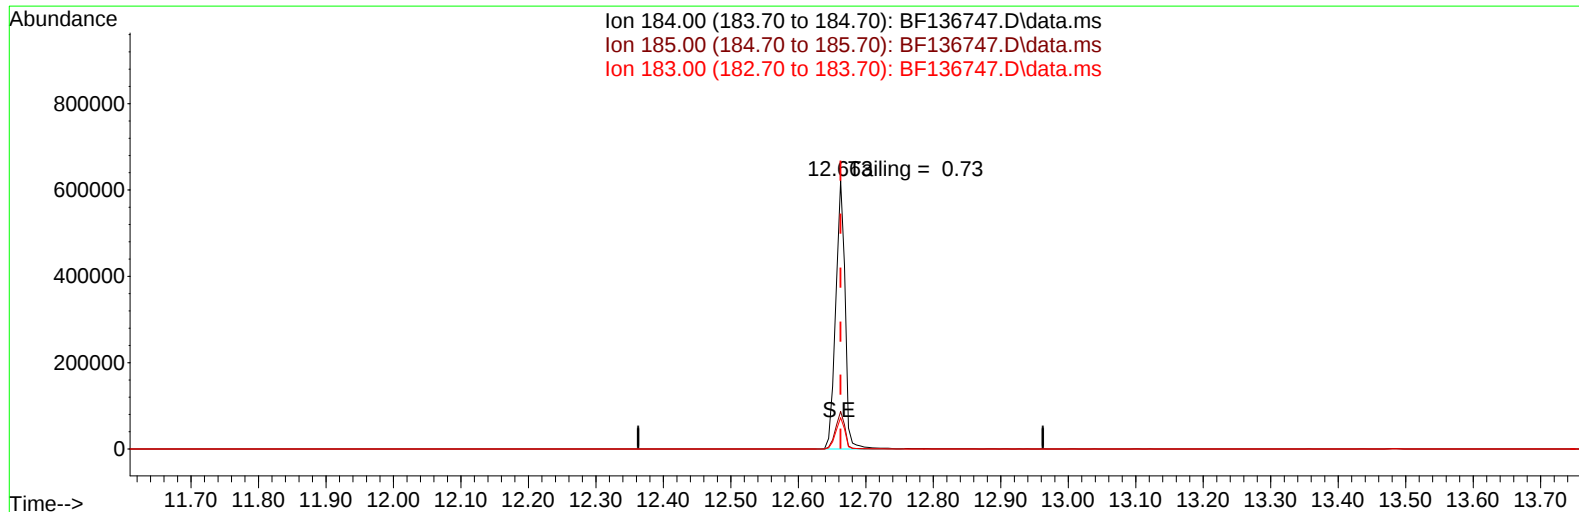

TIC: BF136747.D\data.ms

(77) Benzidine

12.663min (0.000) 347377.02 ng

response 604317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	11.60	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/27/2023	BNA_F	<u>BF136747.D</u>
Compound Name	Response	Retention Time
DDT	268342	13.486
DDD	7145	13.186
DDE	724	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7869	276211	2.85

Instrument :
BNA_F
ClientSampleId :
DFTPP