
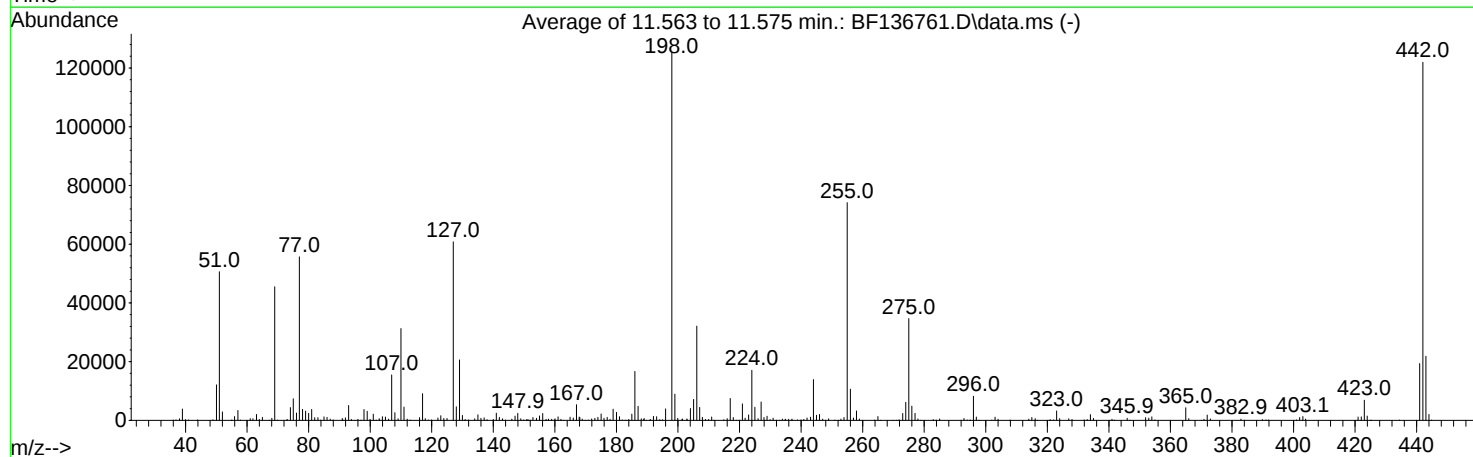


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
Data File : BF136761.D
Acq On : 27 Dec 2023 16:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

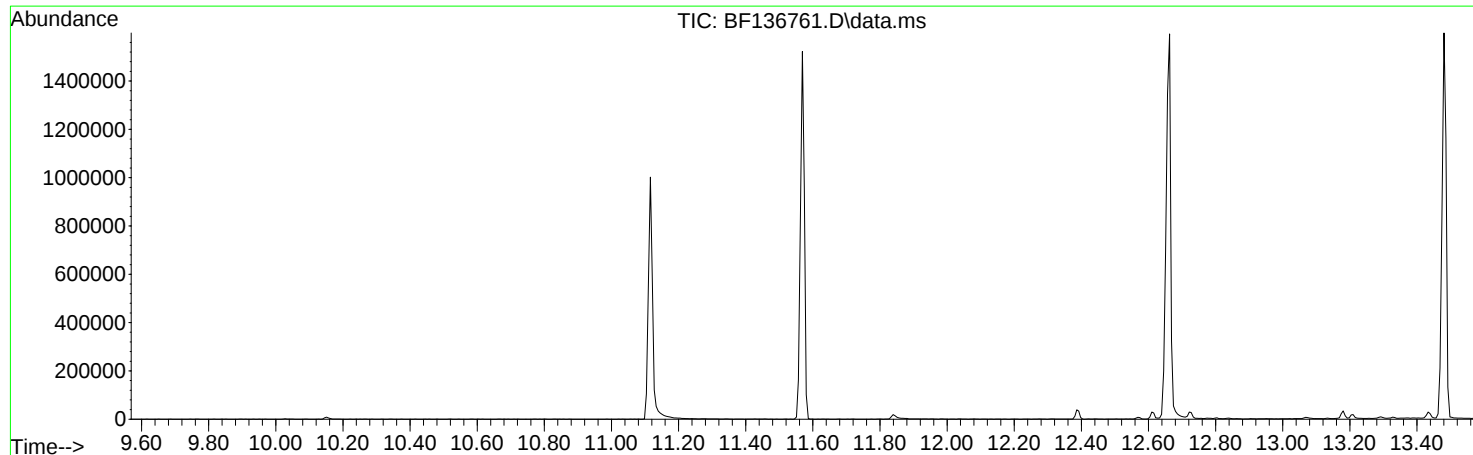




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	50629	PASS
68	69	0.00	2	1.5	702	PASS
69	198	0.00	100	36.3	45507	PASS
70	69	0.00	2	0.3	139	PASS
127	198	10	80	48.5	60816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125285	PASS
199	198	5	9	7.1	8917	PASS
275	198	10	60	27.7	34651	PASS
365	198	1	100	3.4	4308	PASS
441	198	0.01	100	15.4	19326	PASS
442	442	50	100	100.0	121933	PASS
443	442	15	24	17.9	21848	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
 Data File : BF136761.D
 Acq On : 27 Dec 2023 16:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 27 17:46:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

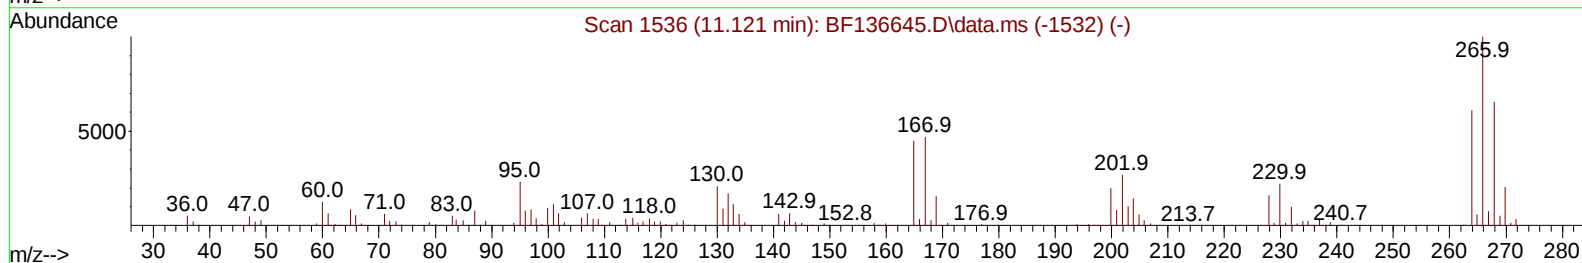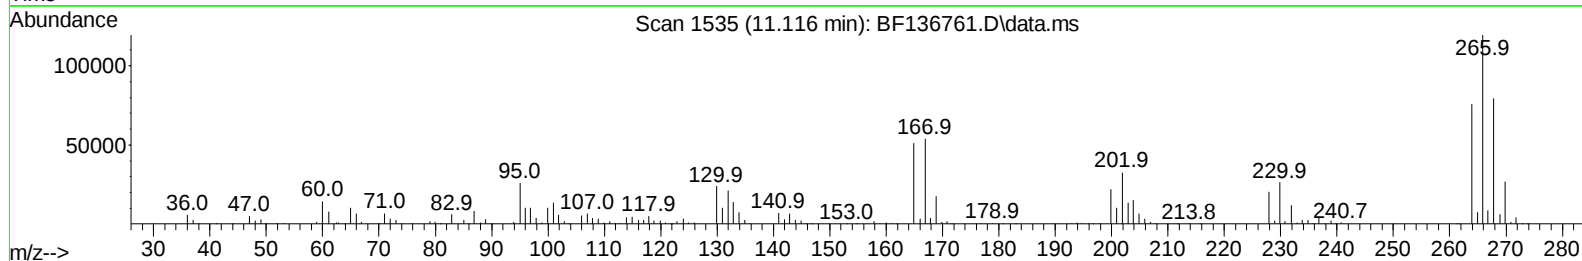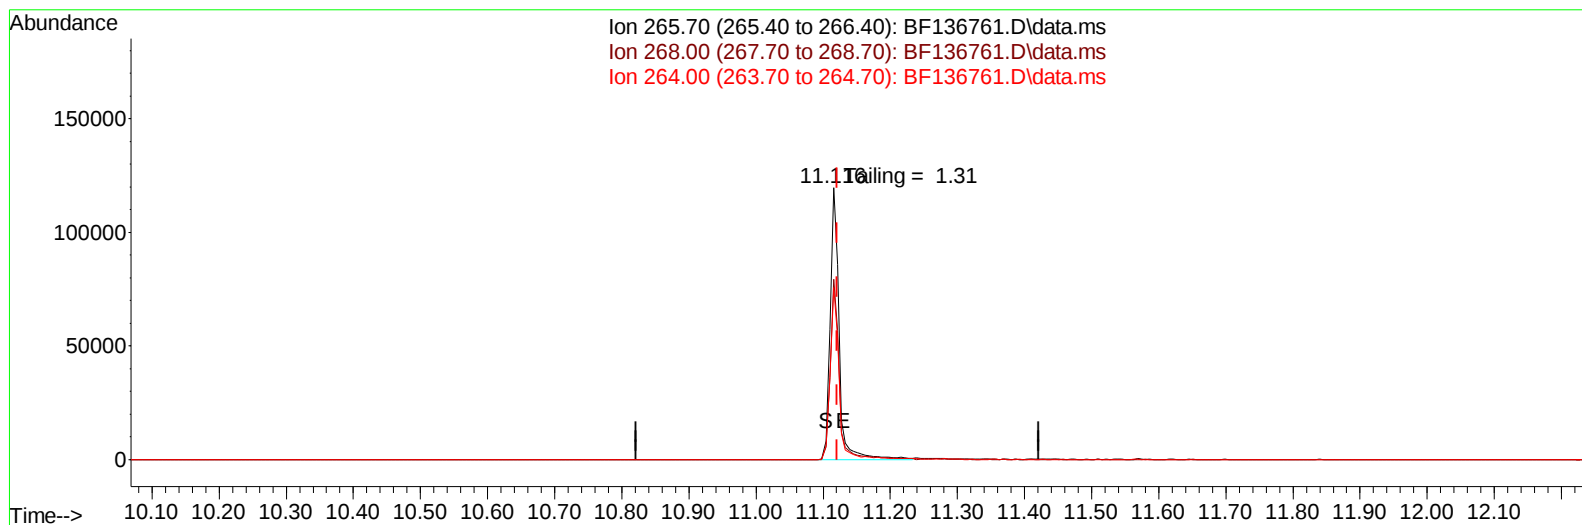

TIC: BF136761.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 35653.84 ng




response 113329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.35
264.00	61.20	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122723\
 Data File : BF136761.D
 Acq On : 27 Dec 2023 16:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 27 17:46:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

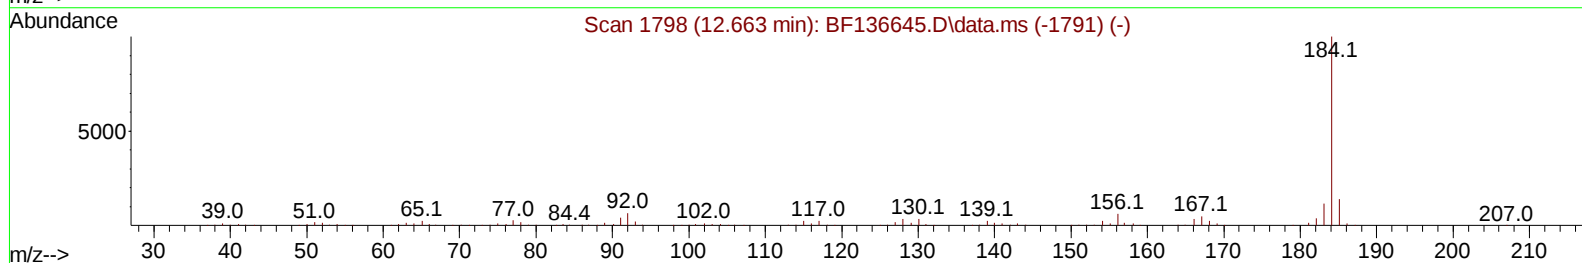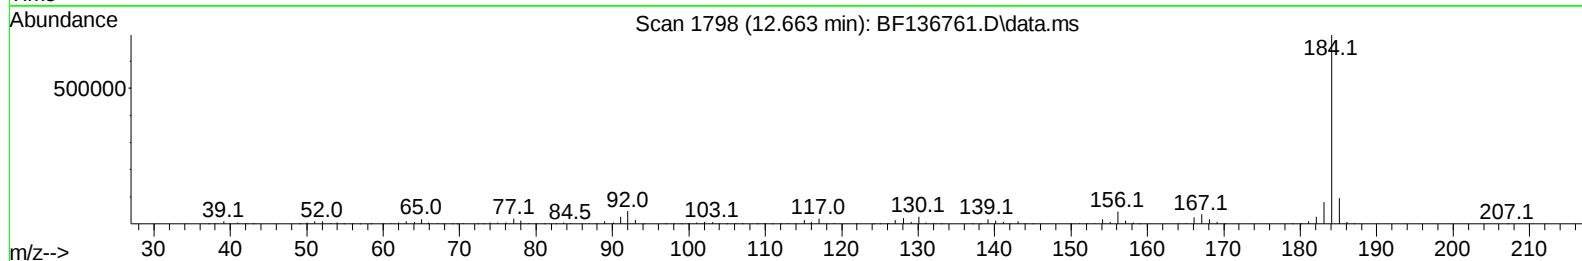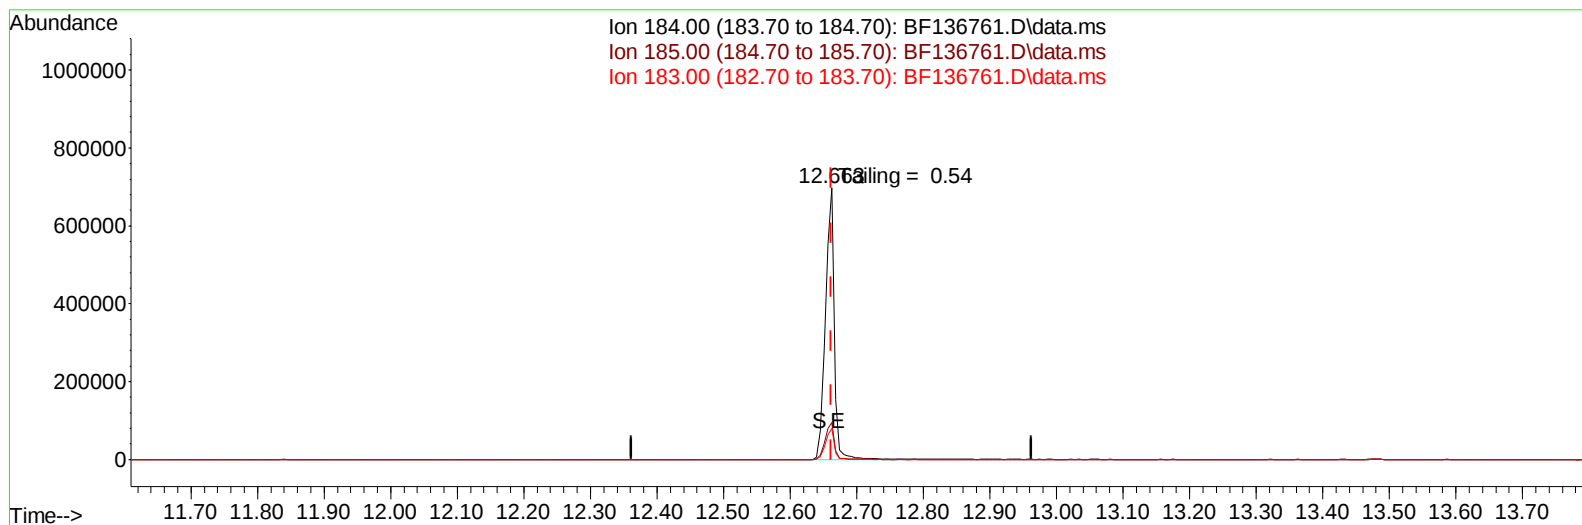

TIC: BF136761.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 0.00 ng

response 652094

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.47
183.00	11.60	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/27/2023	BNA_F	<u>BF136761.D</u>
Compound Name	Response	Retention Time
DDT	291854	13.48
DDD	9180	13.18
DDE	602	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9782	301636	3.24

Instrument :
BNA_F
ClientSampleId :
DFTPP