
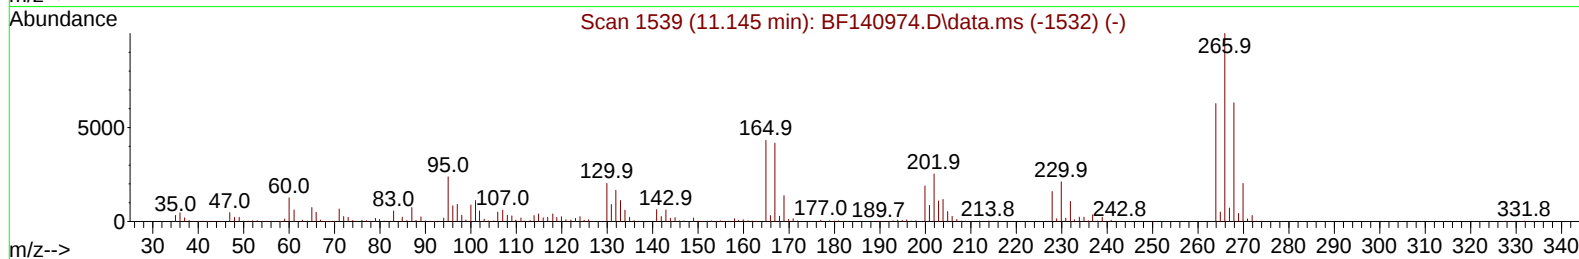
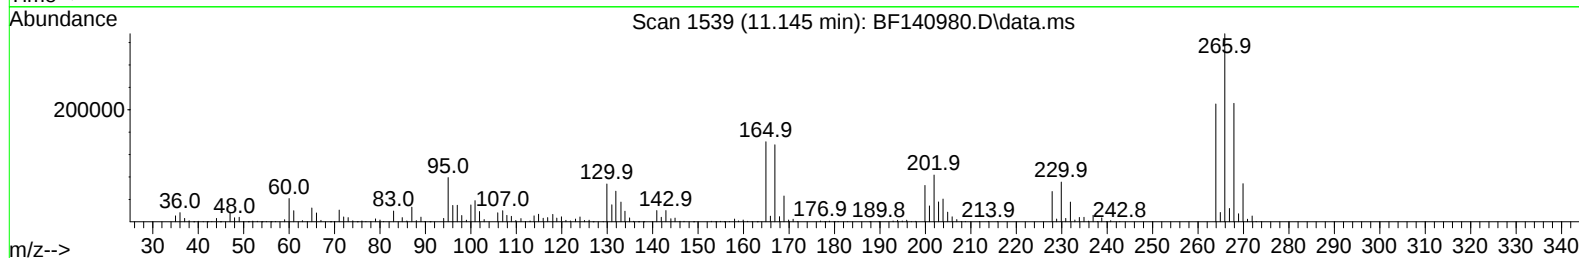


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140980.D
Acq On : 27 Dec 2024 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 10:40:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

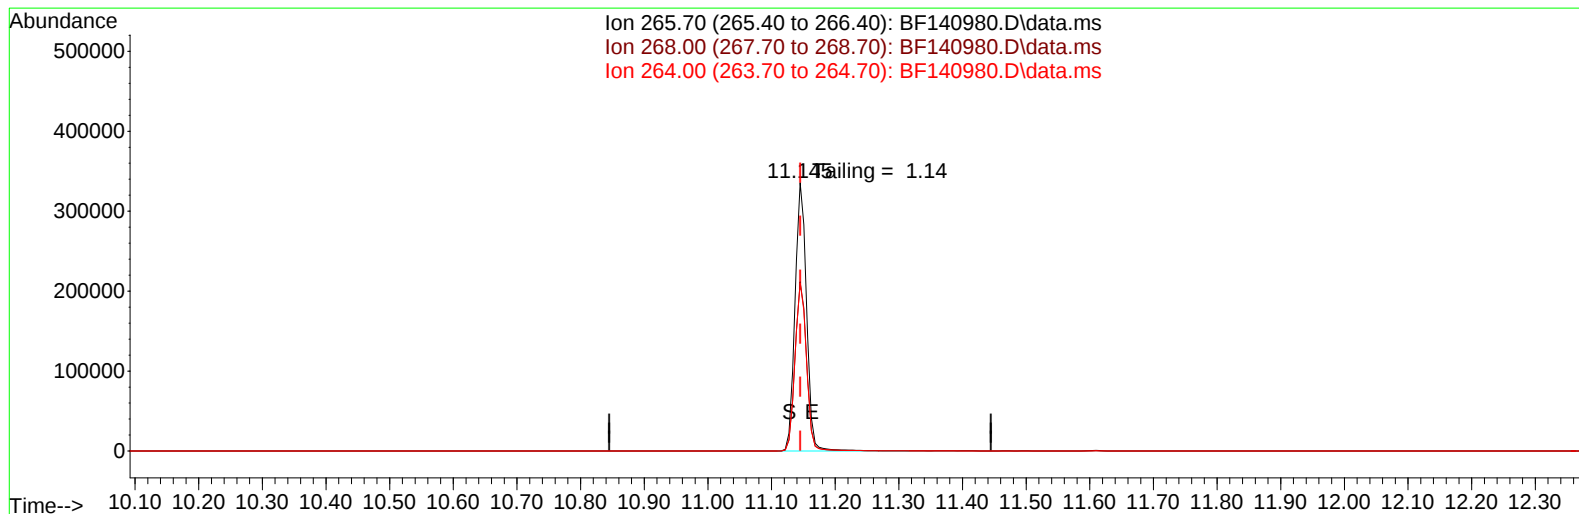

TIC: BF140980.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.000) 34975.88 ng

response 426475

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.00
264.00	62.80	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140980.D
Acq On : 27 Dec 2024 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 10:40:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

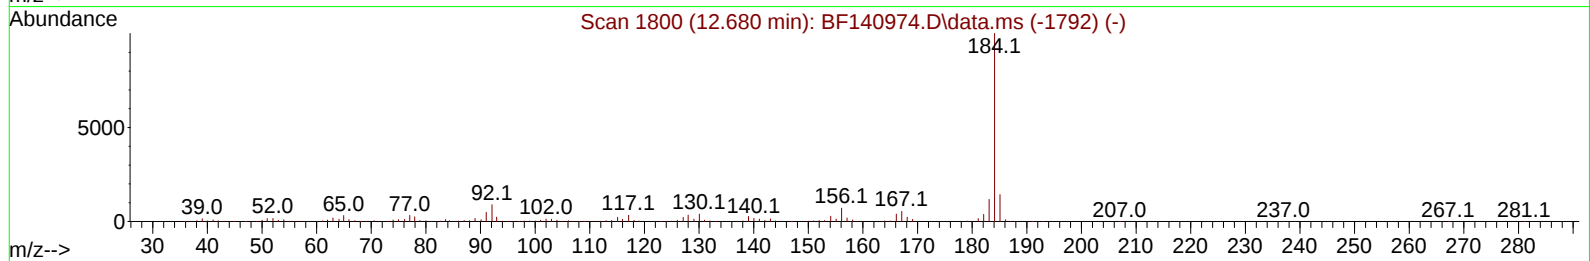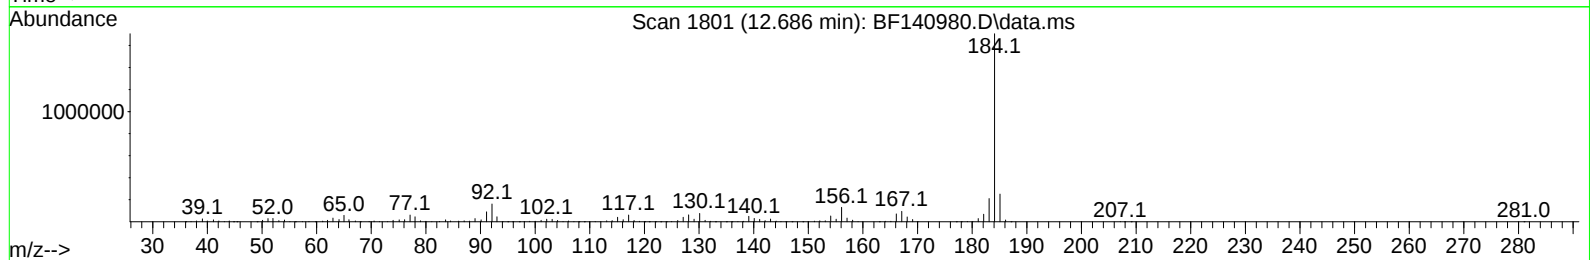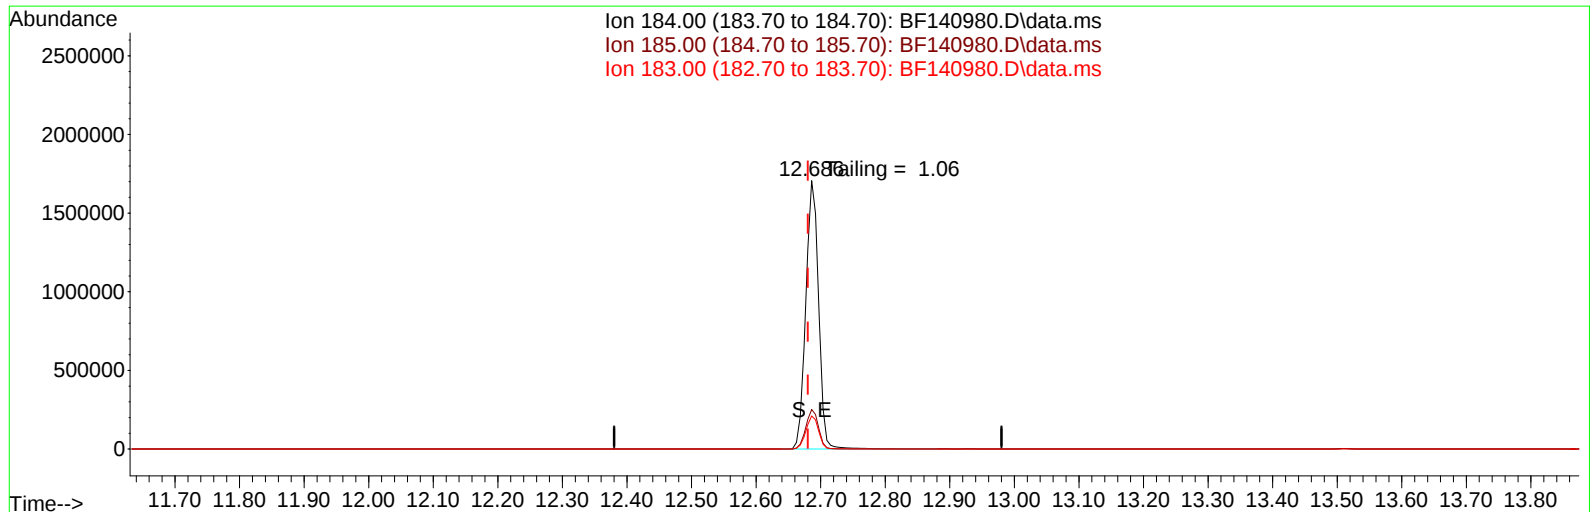

TIC: BF140980.D\data.ms

(77) Benzidine**12.686min (+ 0.006) 38443.56 ng****response 2340716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.75
183.00	11.70	12.36
0.00	0.00	0.00