
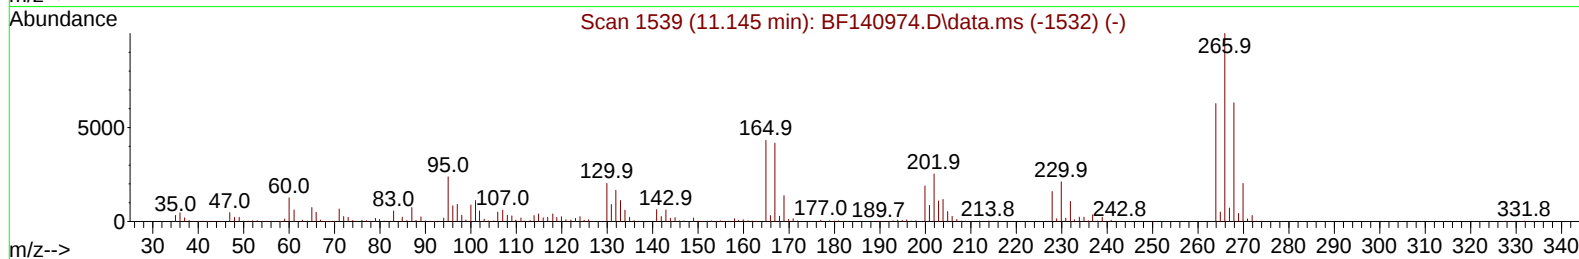
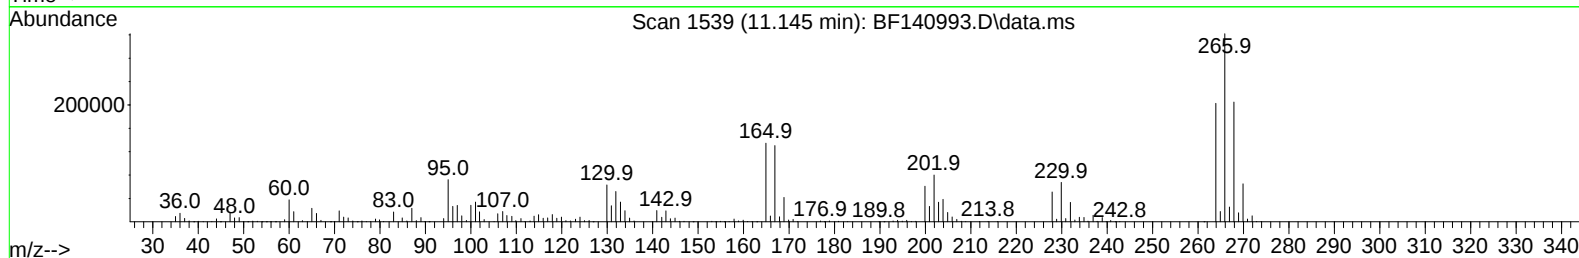


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140993.D
Acq On : 27 Dec 2024 13:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 14:11:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

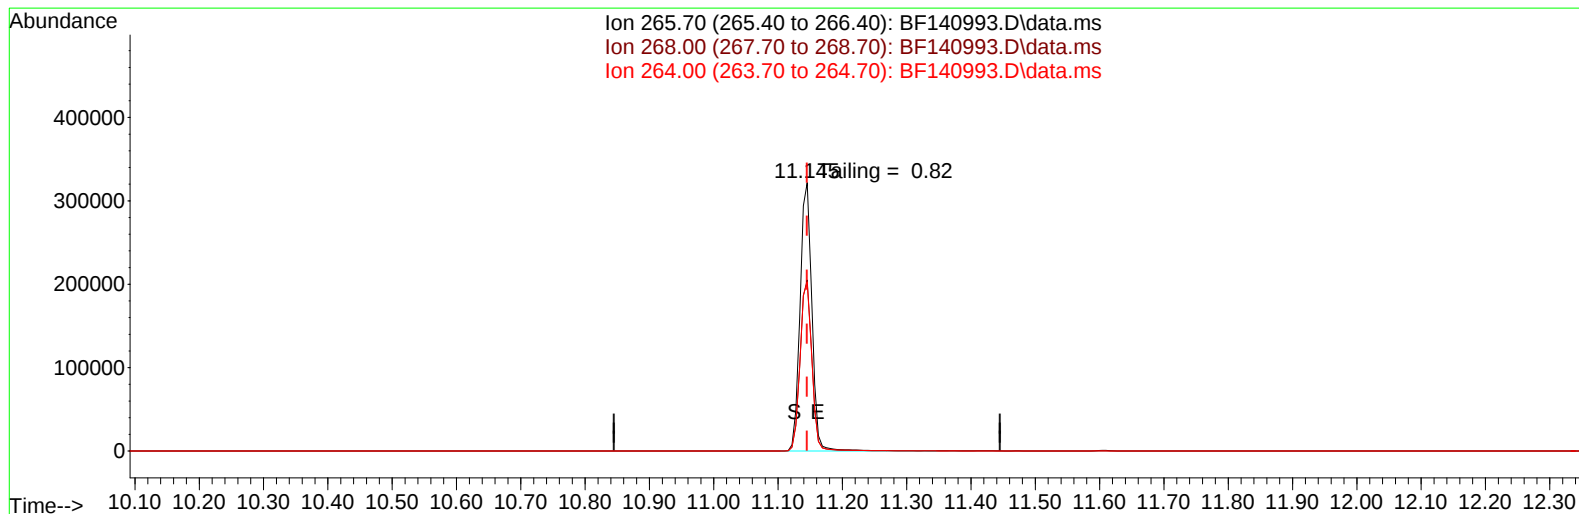

TIC: BF140993.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 33852.29 ng

response 415287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.69
264.00	62.80	63.03
0.00	0.00	0.00

