
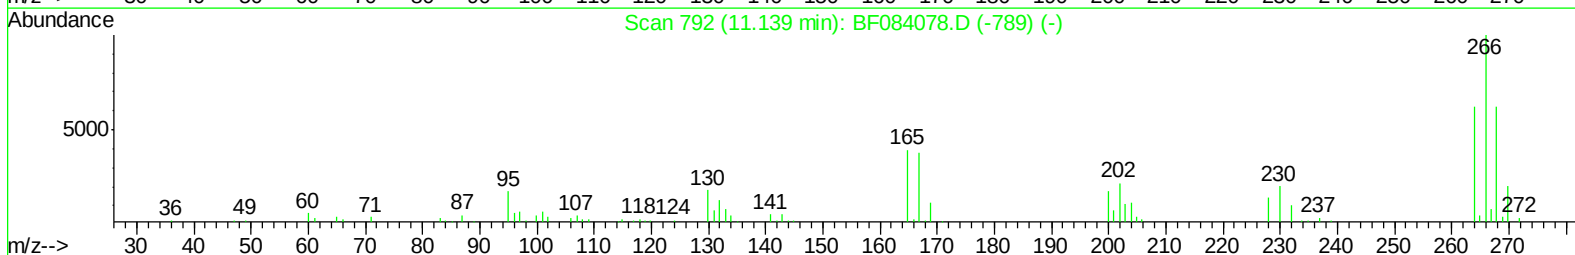
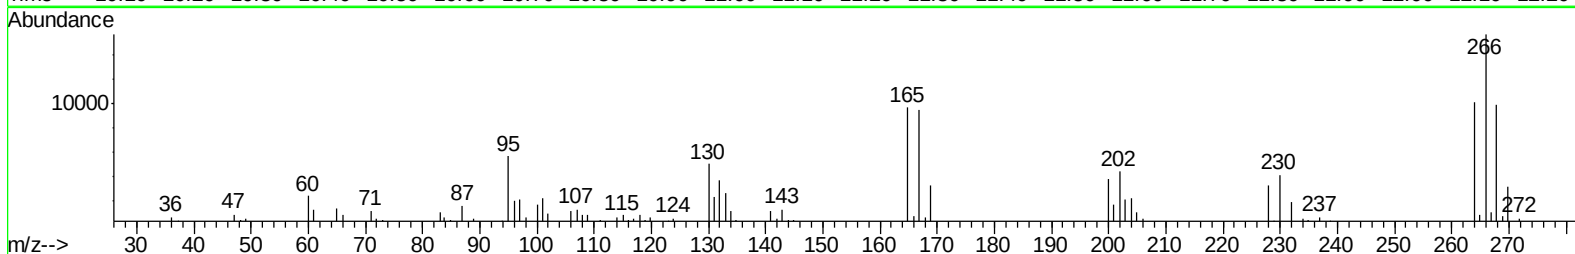


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122815\
Data File : BF084154.D
Acq On : 28 Dec 2015 11:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 06:58:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 24 16:48:39 2015
Response via : Initial Calibration

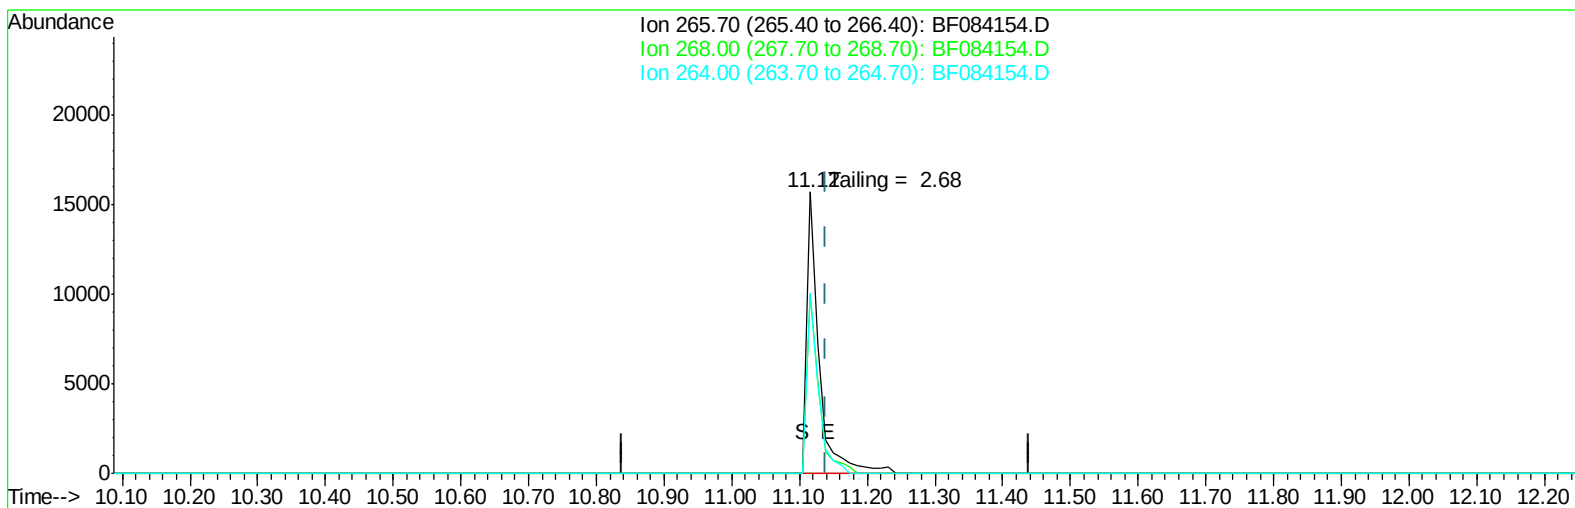

TIC: BF084154.D

(69) Pentachlorophenol (C)




11.116min (-0.023) 0.00ng

response 20049

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	63.20
264.00	62.70	64.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF122815\
 Data File : BF084154.D
 Acq On : 28 Dec 2015 11:50
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 06:58:40 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 24 16:48:39 2015
 Response via : Initial Calibration

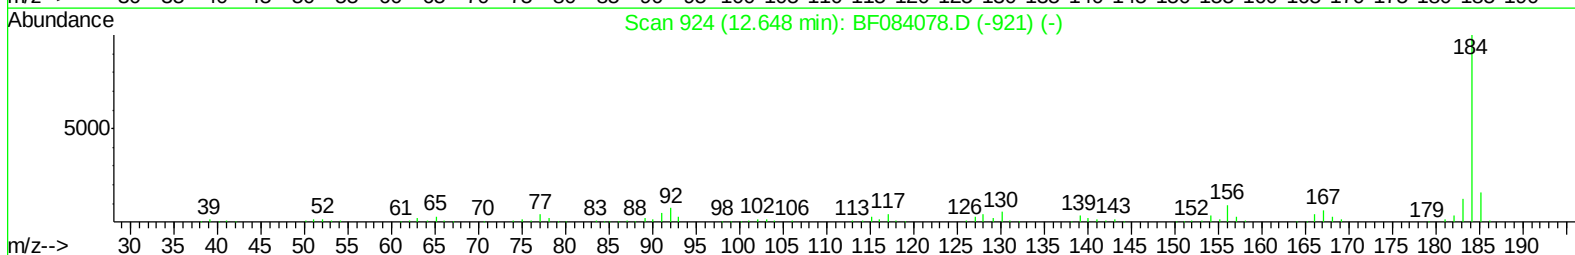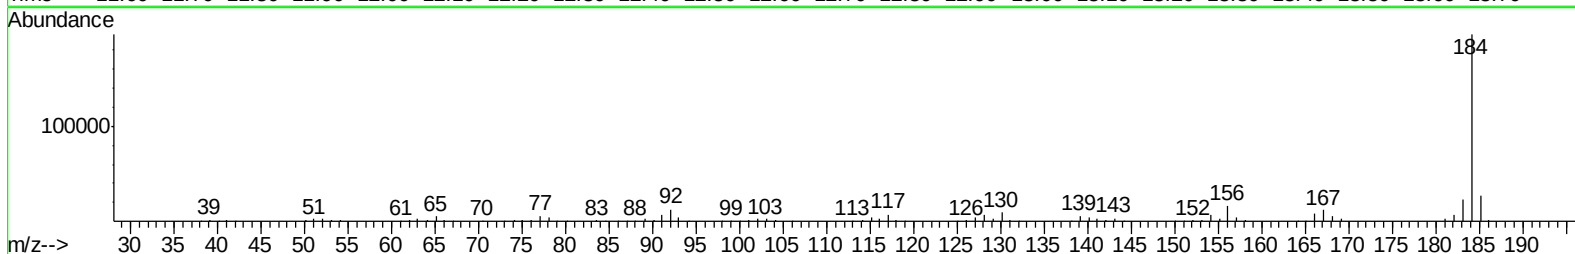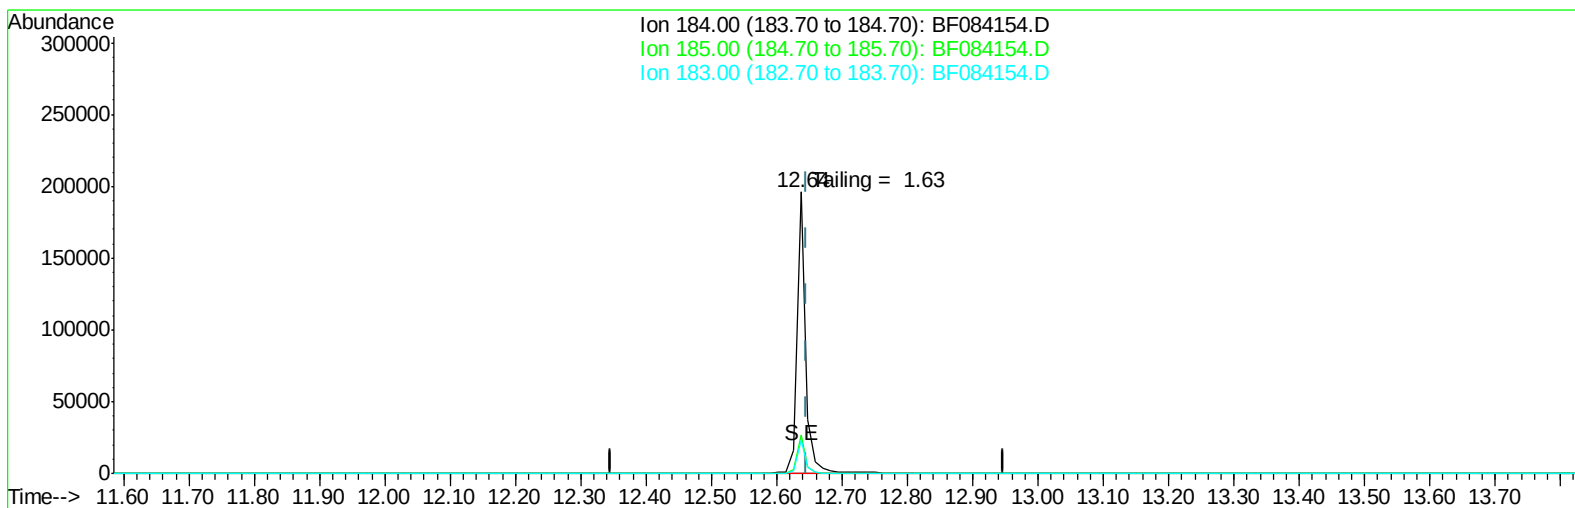

TIC: BF084154.D

(76) Benzidine

12.636min (-0.011) 24081.61ng

response 185796

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.72
183.00	12.30	11.81
0.00	0.00	0.00