


Data Path : Z:\HPCHEM1\BNA F\Data\BF122815\
 Data File : BF084154.D
 Acq On : 28 Dec 2015 11:50
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 24 16:48:39 2015

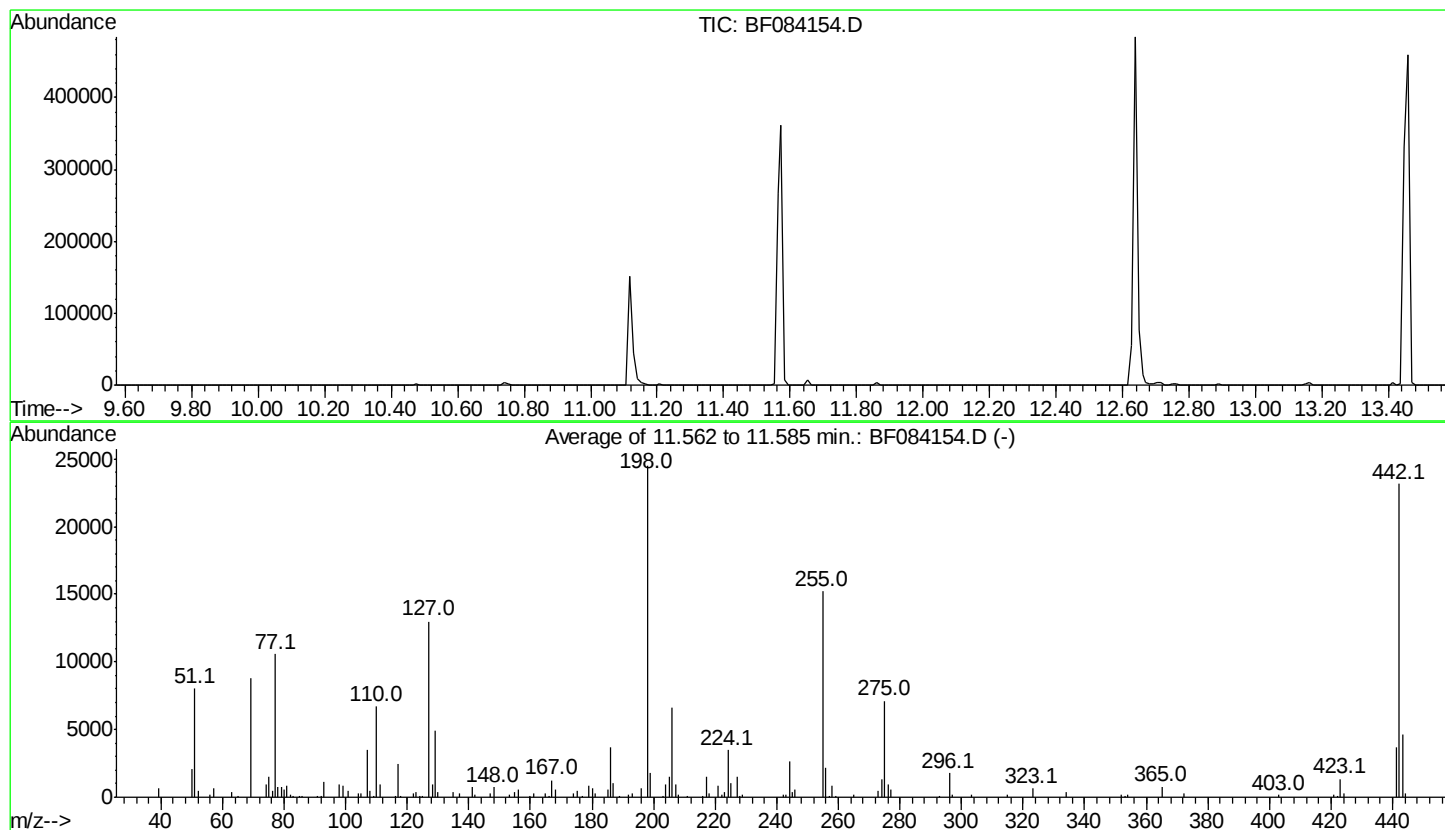

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	8015	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.8	8785	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	12980	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24509	PASS
199	198	5	9	7.5	1836	PASS
275	198	10	60	29.0	7108	PASS
365	198	1	100	3.1	759	PASS
441	442	0.01	24	15.8	3671	PASS
442	198	50	100	94.6	23179	PASS
443	442	15	24	20.0	4639	PASS