

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122816\
 Data File : BF092006.D
 Acq On : 28 Dec 2016 20:42
 Operator : UM/SJ
 Sample : H6281-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-7

Quant Time: Dec 29 00:41:31 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 17:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	214472	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	870582	20.00	ng	-0.01
38) Acenaphthene-d10	9.74	164	486413	20.00	ng	-0.01
63) Phenanthrene-d10	11.23	188	584073	20.00	ng	0.00
75) Chrysene-d12	13.86	240	199805	20.00	ng	-0.01
86) Perylene-d12	15.24	264	149057	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	877522	68.32	ng	0.00
7) Phenol-d6	6.36	99	610267	38.91	ng	-0.02
23) Nitrobenzene-d5	7.28	82	1196456	76.42	ng	-0.01
41) 2,4,6-Tribromophenol	10.54	330	570027	141.61	ng	0.00
44) 2-Fluorobiphenyl	9.07	172	1984153	83.32	ng	-0.01
78) Terphenyl-d14	12.82	244	1123072	136.32	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.48	77	29260	2.27	ng	# 70
19) n-Nitroso-di-n-propylamine	7.28	70	163984	15.72	ng	# 78
49) Dimethylphthalate	9.47	163	68908	2.21	ng	99
66) 4-Bromophenyl-phenylether	10.54	248	34764	5.72	ng	# 1
71) Anthracene	11.33	178	983	Below Cal	#	1
73) Di-n-butylphthalate	11.80	149	5886	Below Cal	#	59
74) Fluoranthene	12.44	202	599	Below Cal	#	1
76) Benzydine	12.43	184	1053	Below Cal	#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122816\  
Data File : BF092006.D  
Acq On    : 28 Dec 2016   20:42  
Operator  : UM/SJ  
Sample    : H6281-02  
Misc      :  
ALS Vial  : 15      Sample Multiplier: 1
```

Quant Time: Dec 29 00:41:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.70 min Scan# 404

Delta R.T. 0.00 min

Lab File: BF092006.D

Acq: 28 Dec 2016 20:42

Instrument :

BNA_F

ClientSampleId :

MW-7


Tgt Ion:152 Resp: 214472

Ion Ratio Lower Upper

152 100

150 154.8 124.9 187.3




115 58.7 46.0 69.0

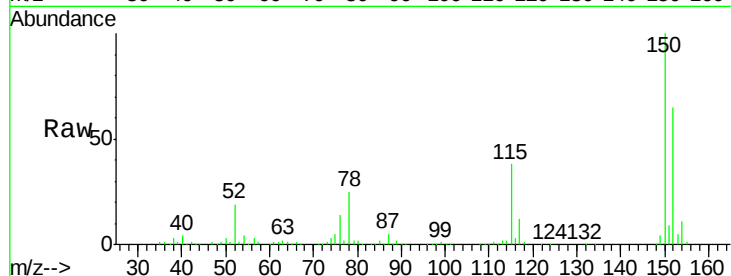

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

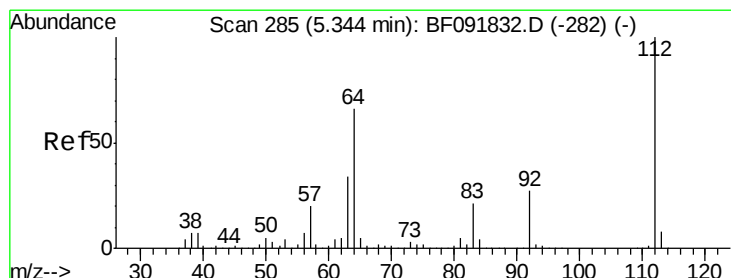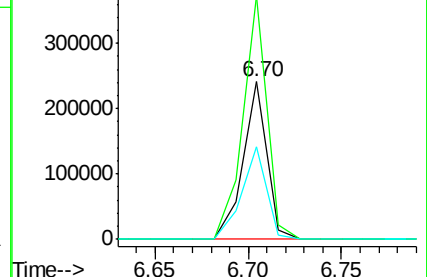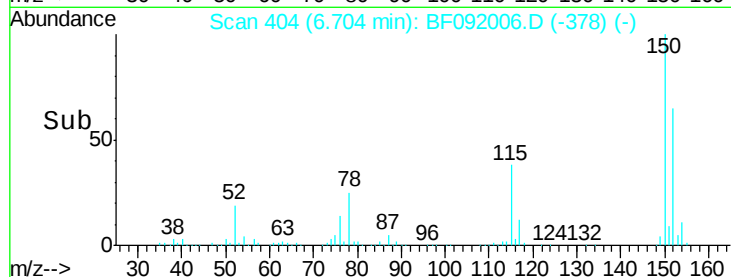

#5

2-Fluorophenol

Concen: 68.32 ng

RT: 5.32 min Scan# 283

Delta R.T. 0.00 min

Lab File: BF092006.D

Acq: 28 Dec 2016 20:42


Tgt Ion:112 Resp: 877522

Ion Ratio Lower Upper

112 100

64 51.9 46.1 69.1



63 25.6 23.8 35.6

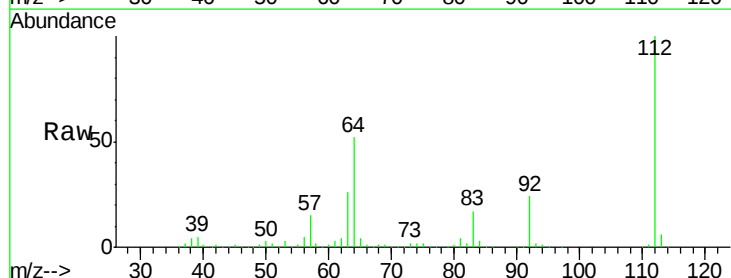

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

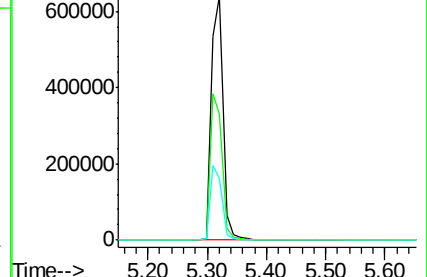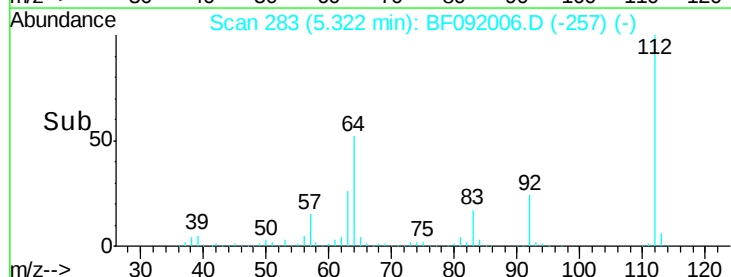



#7

Phenol-d6

Concen: 38.91 ng

RT: 6.36 min Scan# 374

Delta R.T. -0.02 min

Lab File: BF092006.D

Acq: 28 Dec 2016 20:42

Instrument :

BNA_F

ClientSampleId :

MW-7


Tgt Ion: 99 Resp: 610267

Ion Ratio Lower Upper

99 100

42 21.0 15.6 23.4




71 36.1 27.5 41.3

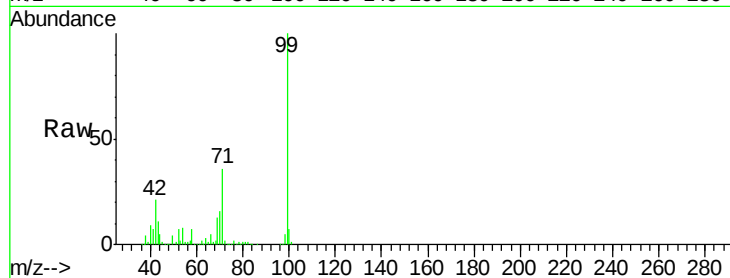

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

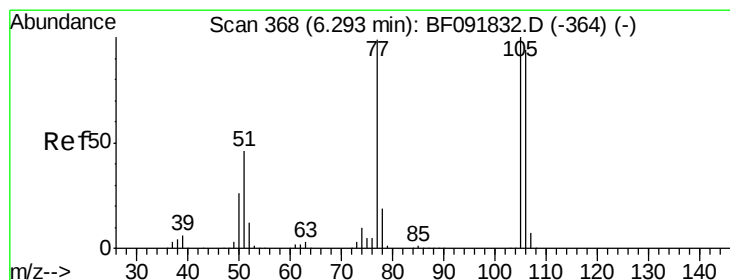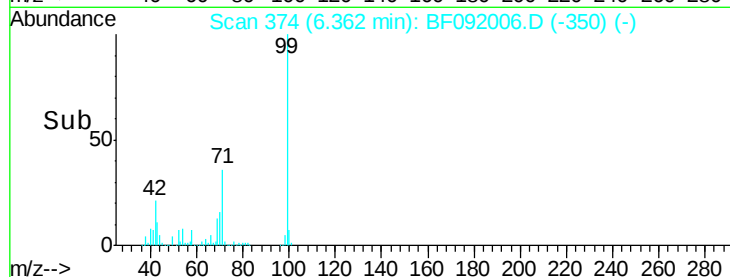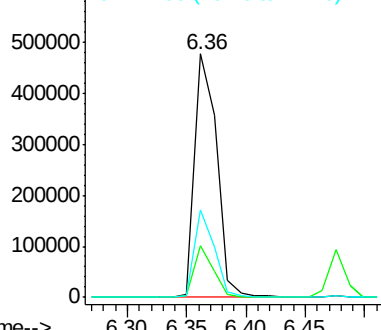

#9

Benzaldehyde

Concen: 2.27 ng

RT: 6.48 min Scan# 384

Delta R.T. 0.23 min

Lab File: BF092006.D

Acq: 28 Dec 2016 20:42


Tgt Ion: 77 Resp: 29260

Ion Ratio Lower Upper

77 100

105 76.1 83.9 123.9#



106 65.0 77.6 117.6#


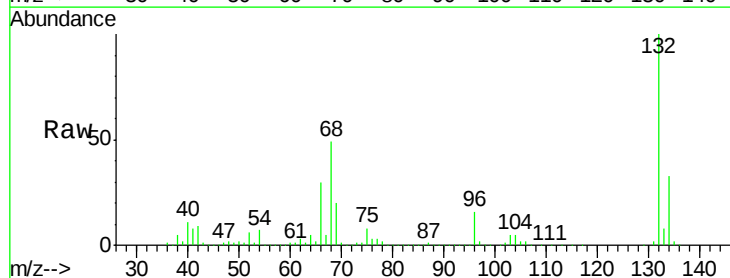


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



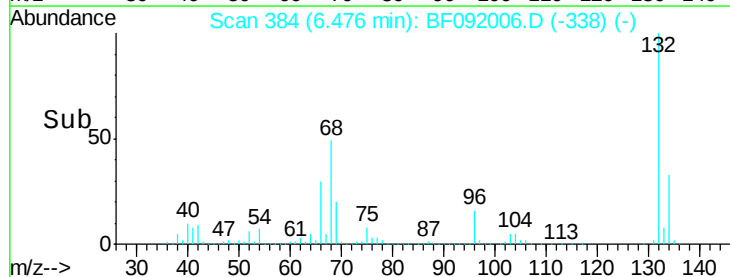
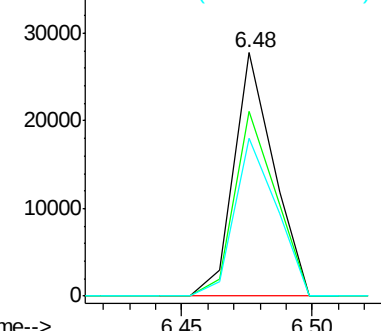


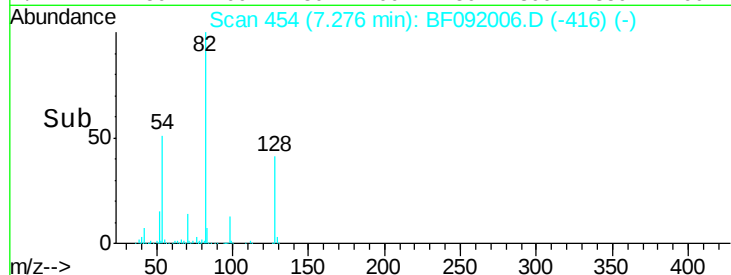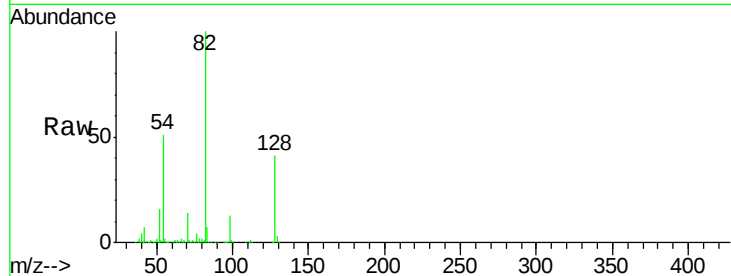

#19
n-Nitroso-di-n-propylamine
Concen: 15.72 ng
RT: 7.28 min Scan# 454
Delta R.T. 0.14 min
Lab File: BF092006.D
Acq: 28 Dec 2016 20:42


Instrument :
BNA_F
ClientSampleId :
MW-7

Tgt Ion:	70	Resp:	163984
Ion	Ratio	Lower	Upper
70	100		
42	48.2	49.4	74.0#
101	0.0	7.4	11.2#
130	1.9	14.2	21.4#

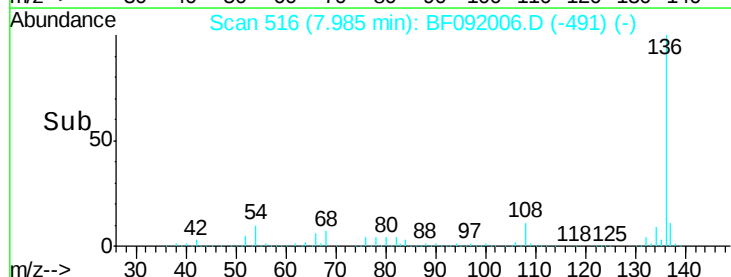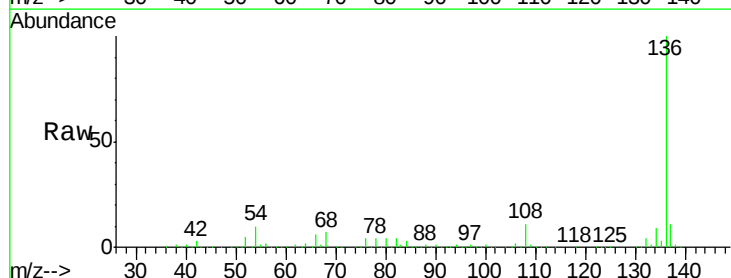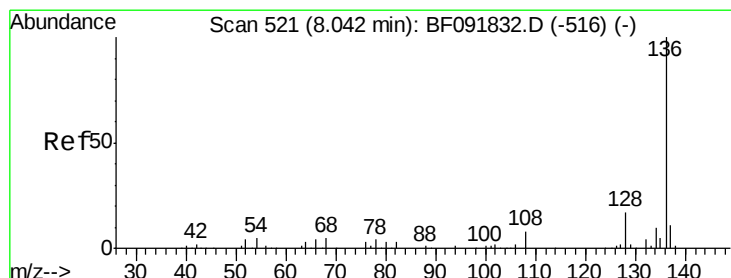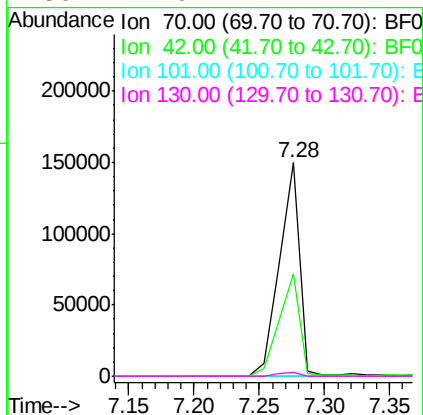

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.98 min Scan# 516
Delta R.T. -0.01 min
Lab File: BF092006.D
Acq: 28 Dec 2016 20:42

Tgt Ion:	136	Resp:	870582
Ion	Ratio	Lower	Upper
136	100		
137	11.5	8.4	12.6
54	9.5	4.5	6.7#
68	7.4	3.6	5.4#




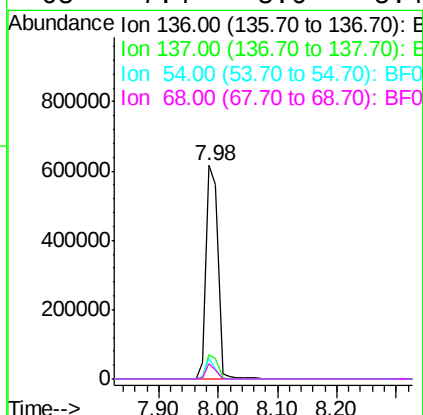




#23
 Nitrobenzene-d5
 Concen: 76.42 ng
 RT: 7.28 min Scan# 454
 Delta R.T. -0.01 min
 Lab File: BF092006.D
 Acq: 28 Dec 2016 20:42




Instrument :
 BNA_F
 ClientSampleId :
 MW-7


Tgt Ion: 82 Resp: 1196456
 Ion Ratio Lower Upper
 82 100
 128 41.1 34.6 52.0
 54 50.9 39.5 59.3

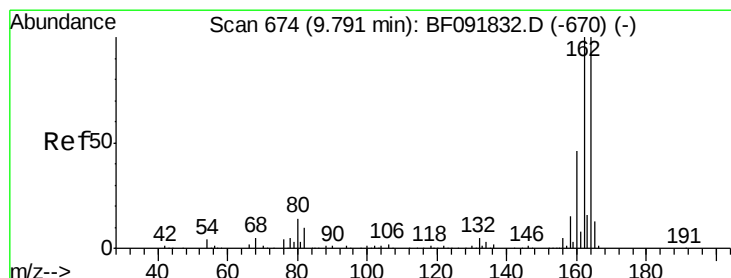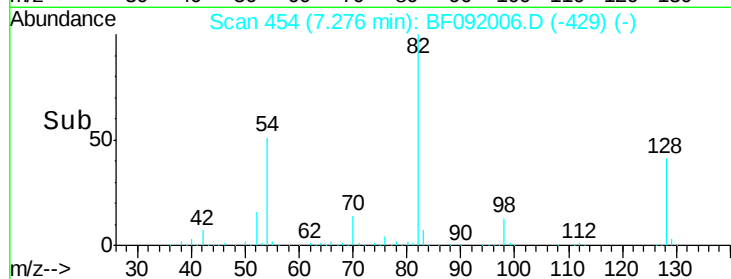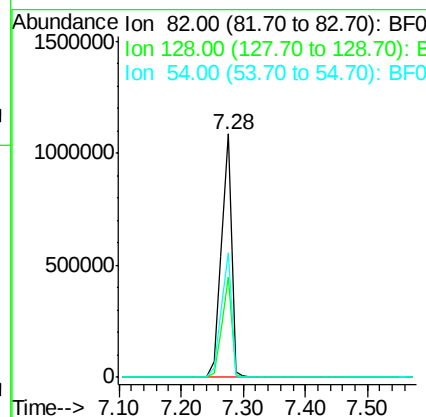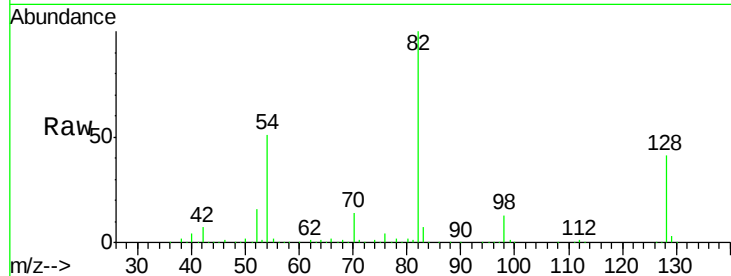

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.74 min Scan# 670
 Delta R.T. -0.01 min
 Lab File: BF092006.D
 Acq: 28 Dec 2016 20:42

Tgt Ion: 164 Resp: 486413
 Ion Ratio Lower Upper
 164 100
 162 100.5 80.2 120.2
 160 44.4 36.9 55.3


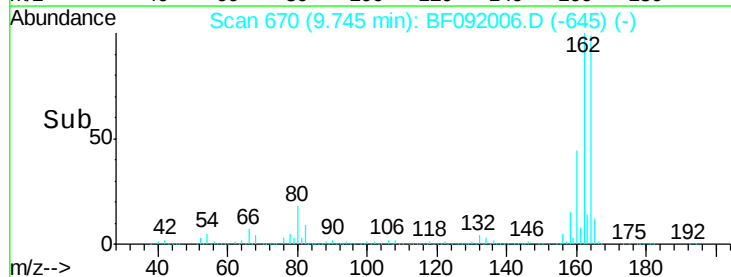
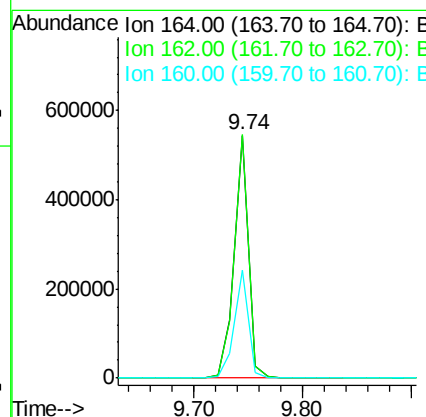
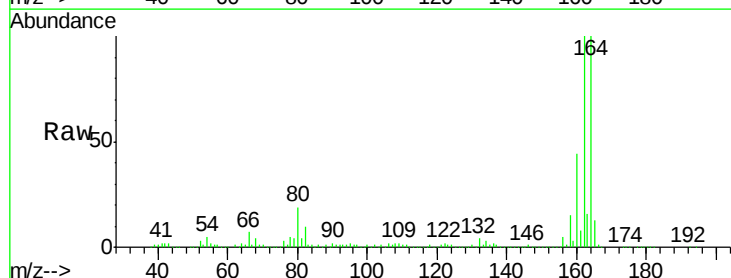


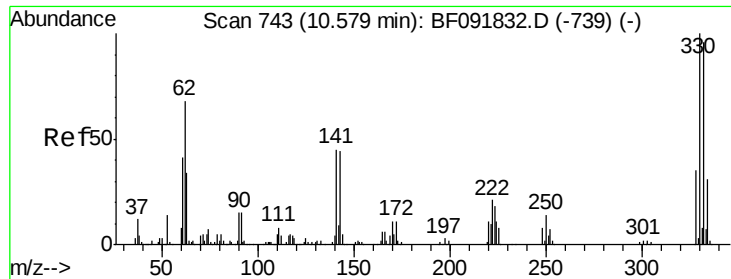

#41
 2,4,6-Tribromophenol
 Concen: 141.61 ng
 RT: 10.54 min Scan# 740
 Delta R.T. 0.00 min
 Lab File: BF092006.D
 Acq: 28 Dec 2016 20:42




Instrument :
 BNA_F
 ClientSampleId :
 MW-7


Tgt Ion:330 Resp: 570027
 Ion Ratio Lower Upper
 330 100
 332 95.6 77.4 116.2
 141 33.1 34.1 51.1#

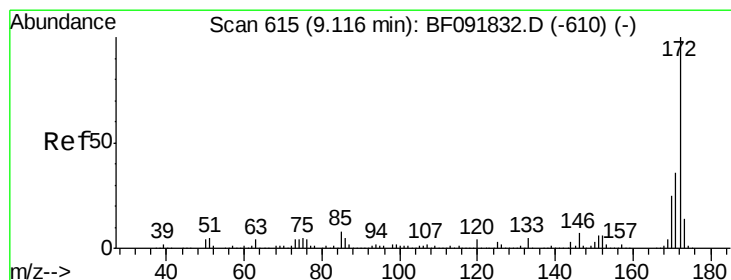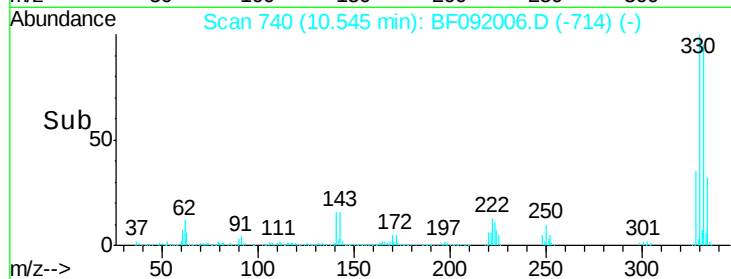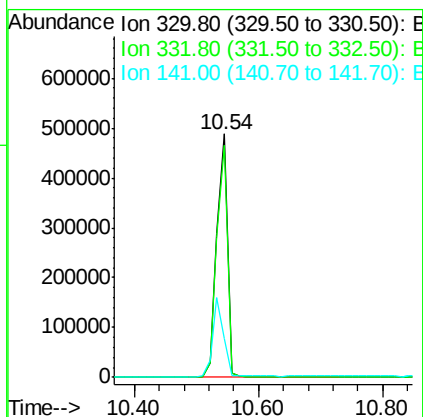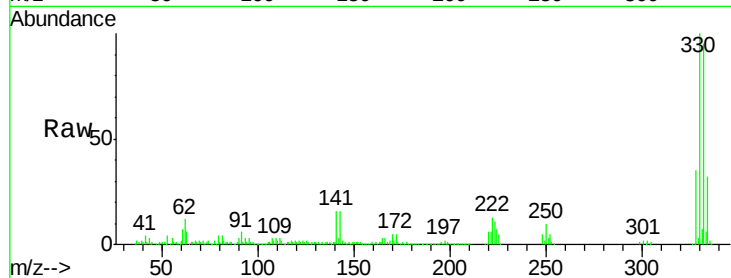

#44
 2-Fluorobiphenyl
 Concen: 83.32 ng
 RT: 9.07 min Scan# 611
 Delta R.T. -0.01 min
 Lab File: BF092006.D
 Acq: 28 Dec 2016 20:42

Tgt Ion:172 Resp: 1984153
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.4 44.0
 170 24.6 20.2 30.4

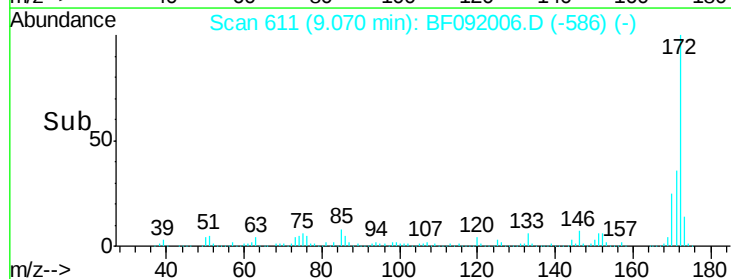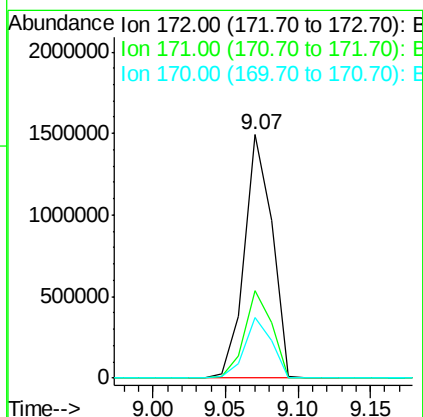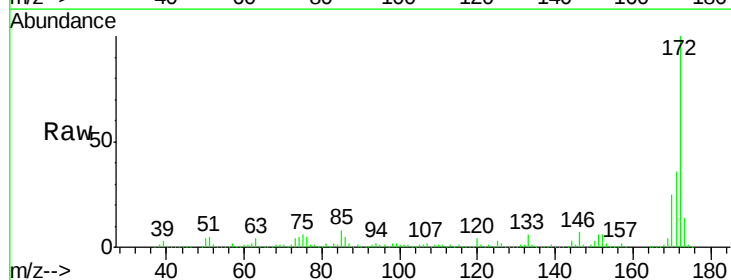


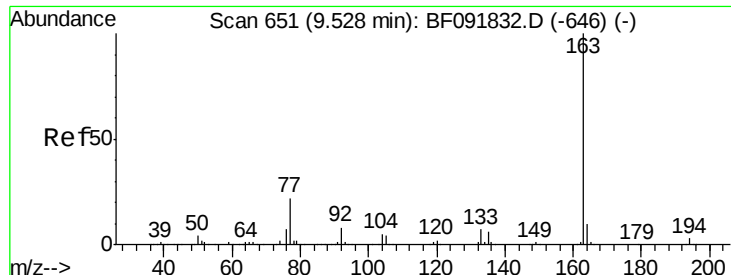




#49
Dimethylphthalate
Concen: 2.21 ng
RT: 9.47 min Scan# 646
Delta R.T. -0.02 min
Lab File: BF092006.D
Acq: 28 Dec 2016 20:42

Instrument :
BNA_F
ClientSampleId :
MW-7

Tgt Ion:163 Resp: 68908
Ion Ratio Lower Upper
163 100
194 4.0 3.0 4.4
164 9.8 8.0 12.0

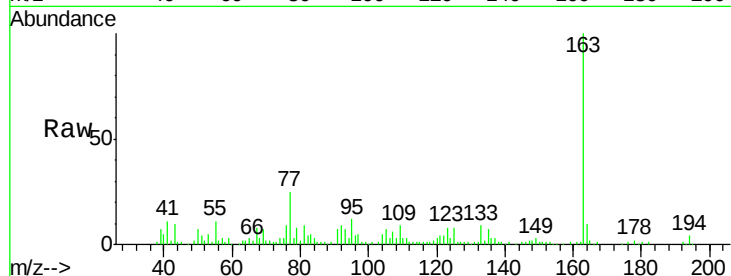


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

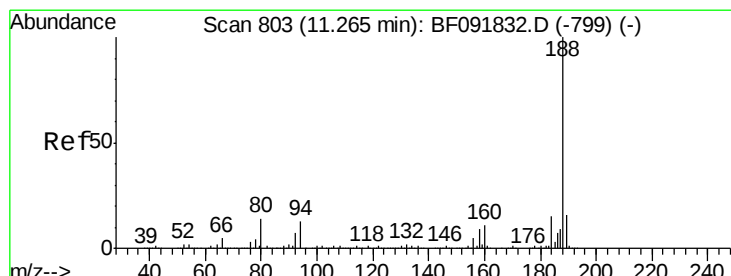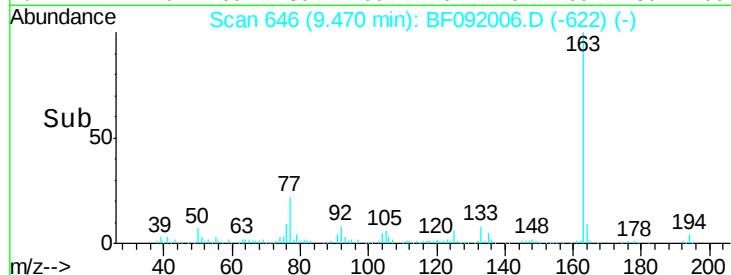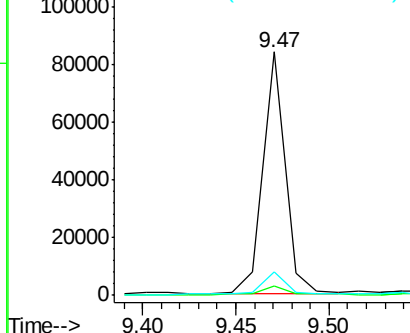

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.23 min Scan# 800
Delta R.T. 0.00 min
Lab File: BF092006.D
Acq: 28 Dec 2016 20:42

Tgt Ion:188 Resp: 584073
Ion Ratio Lower Upper
188 100
94 7.5 10.0 15.0#
80 7.2 11.2 16.8#

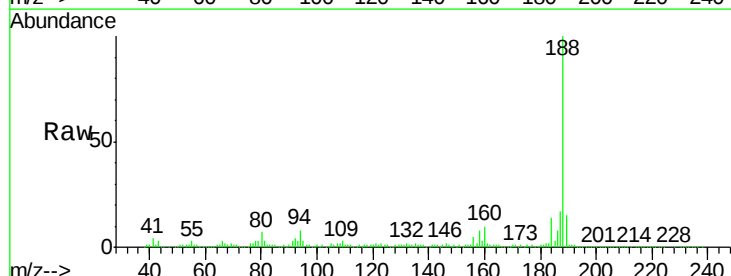

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

