
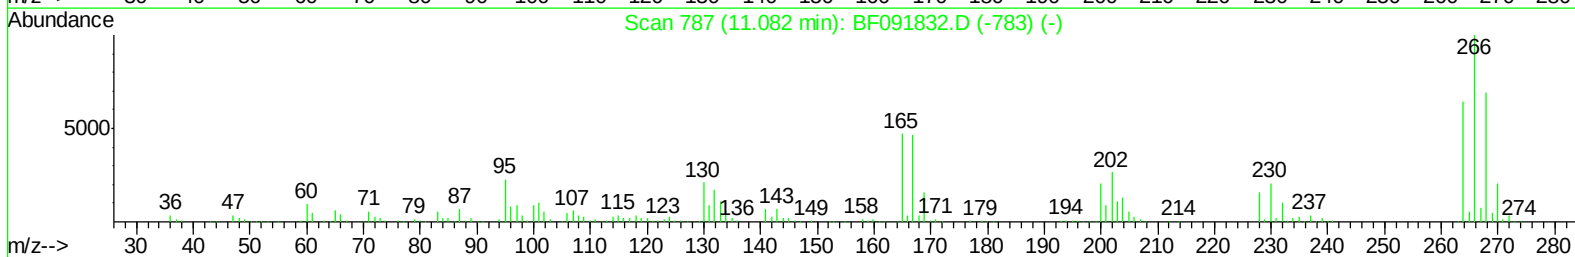
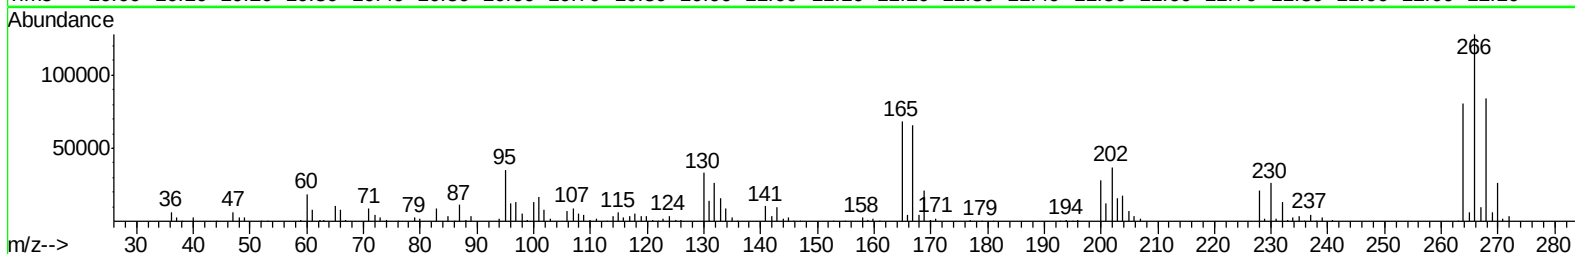


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122816\
Data File : BF091992.D
Acq On : 28 Dec 2016 12:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 06:52:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

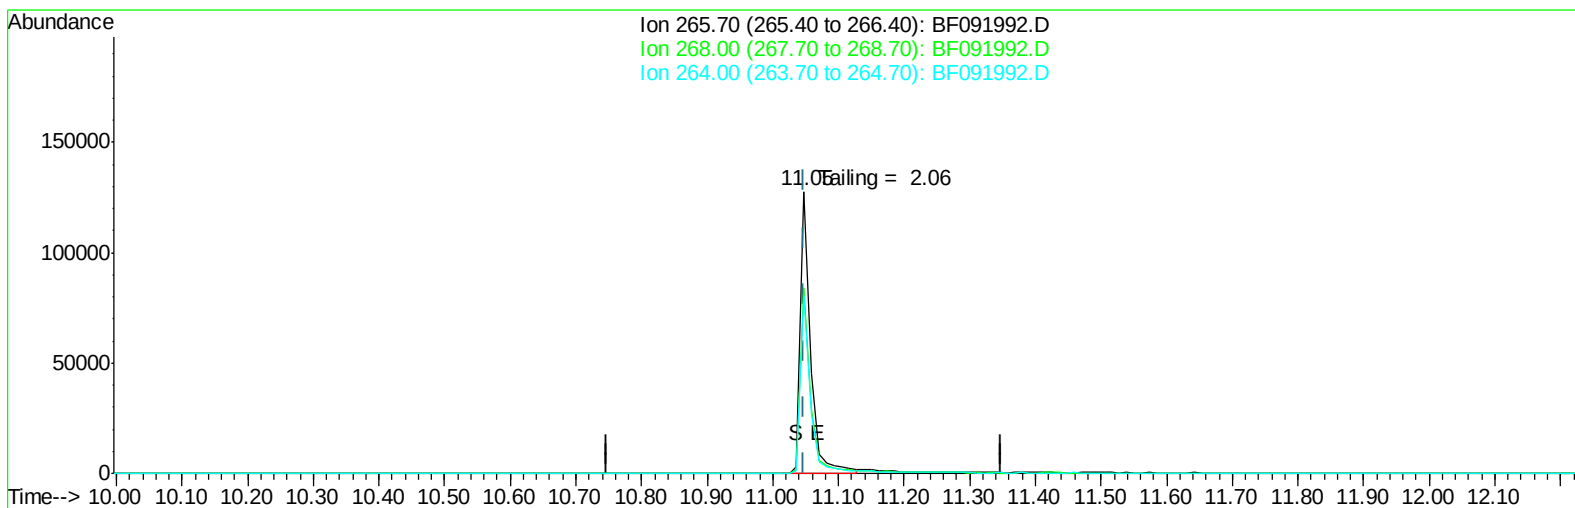

TIC: BF091992.D

(69) Pentachlorophenol (C)




11.048min (-0.000) 0.00ng

response 143405

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.14
264.00	62.90	63.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122816\
 Data File : BF091992.D
 Acq On : 28 Dec 2016 12:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 06:52:18 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 17:32:10 2016
 Response via : Initial Calibration

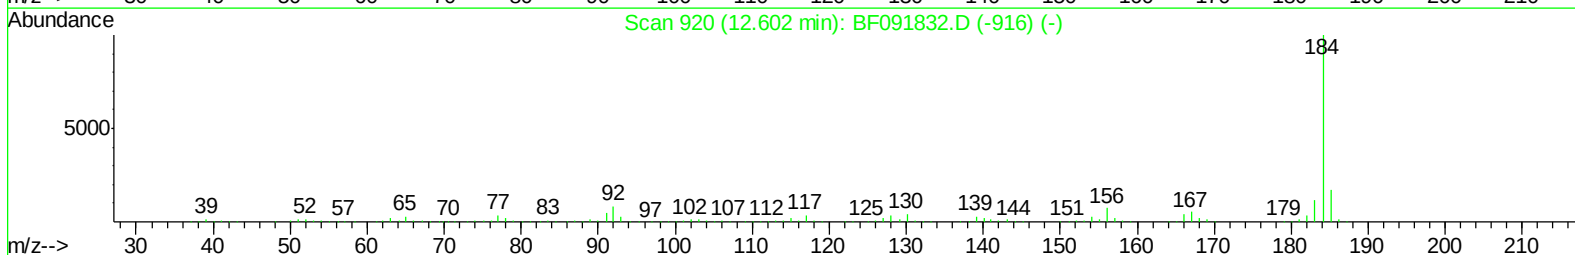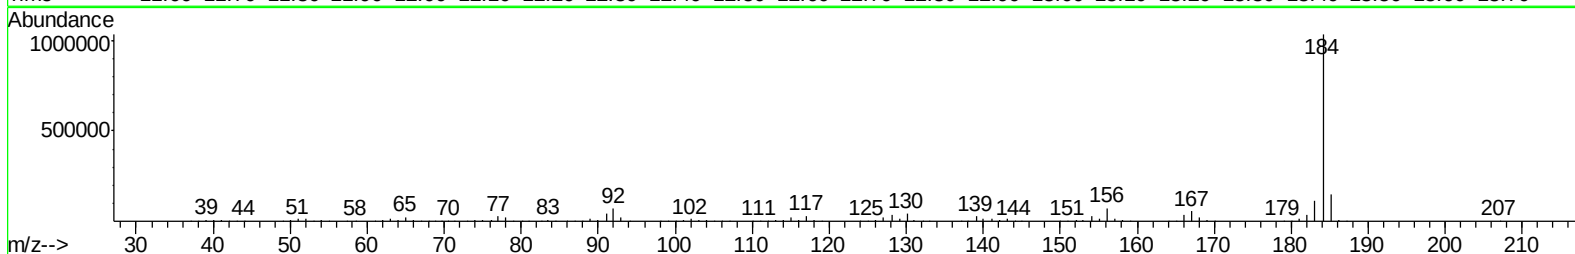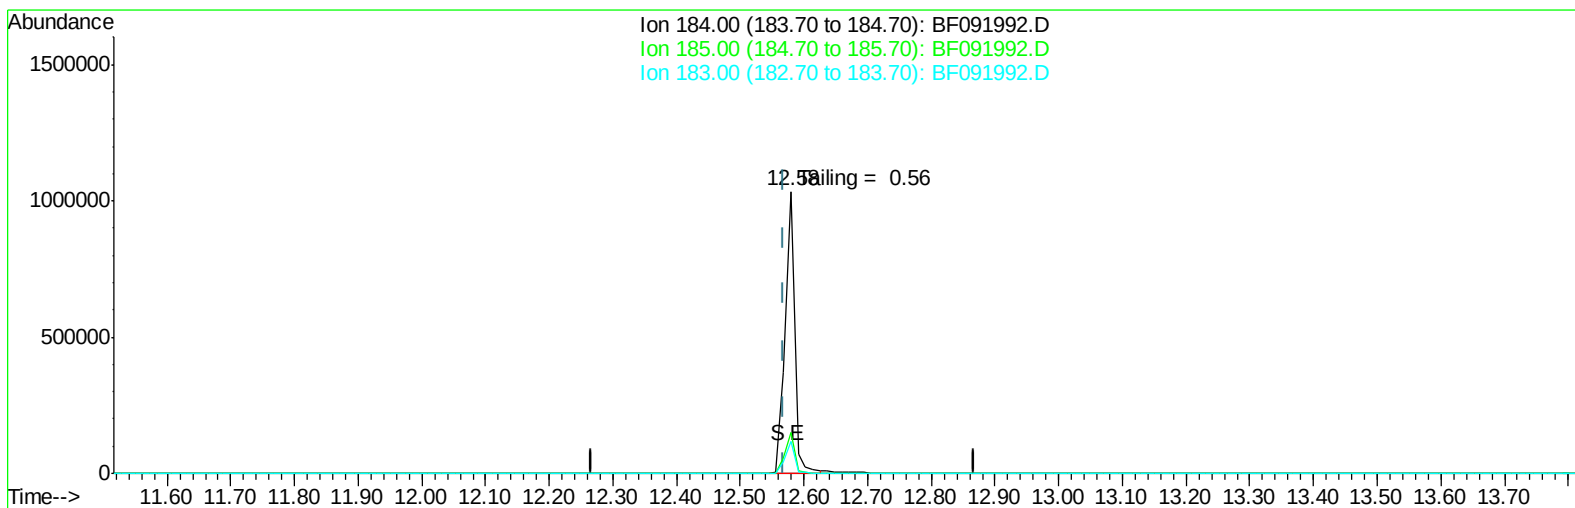

TIC: BF091992.D

(76) Benzidine

12.579min (+0.011) 0.00ng

response 1082206

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.38
183.00	11.50	11.17
0.00	0.00	0.00