


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122816\
 Data File : BF091992.D
 Acq On : 28 Dec 2016 12:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 17:32:10 2016

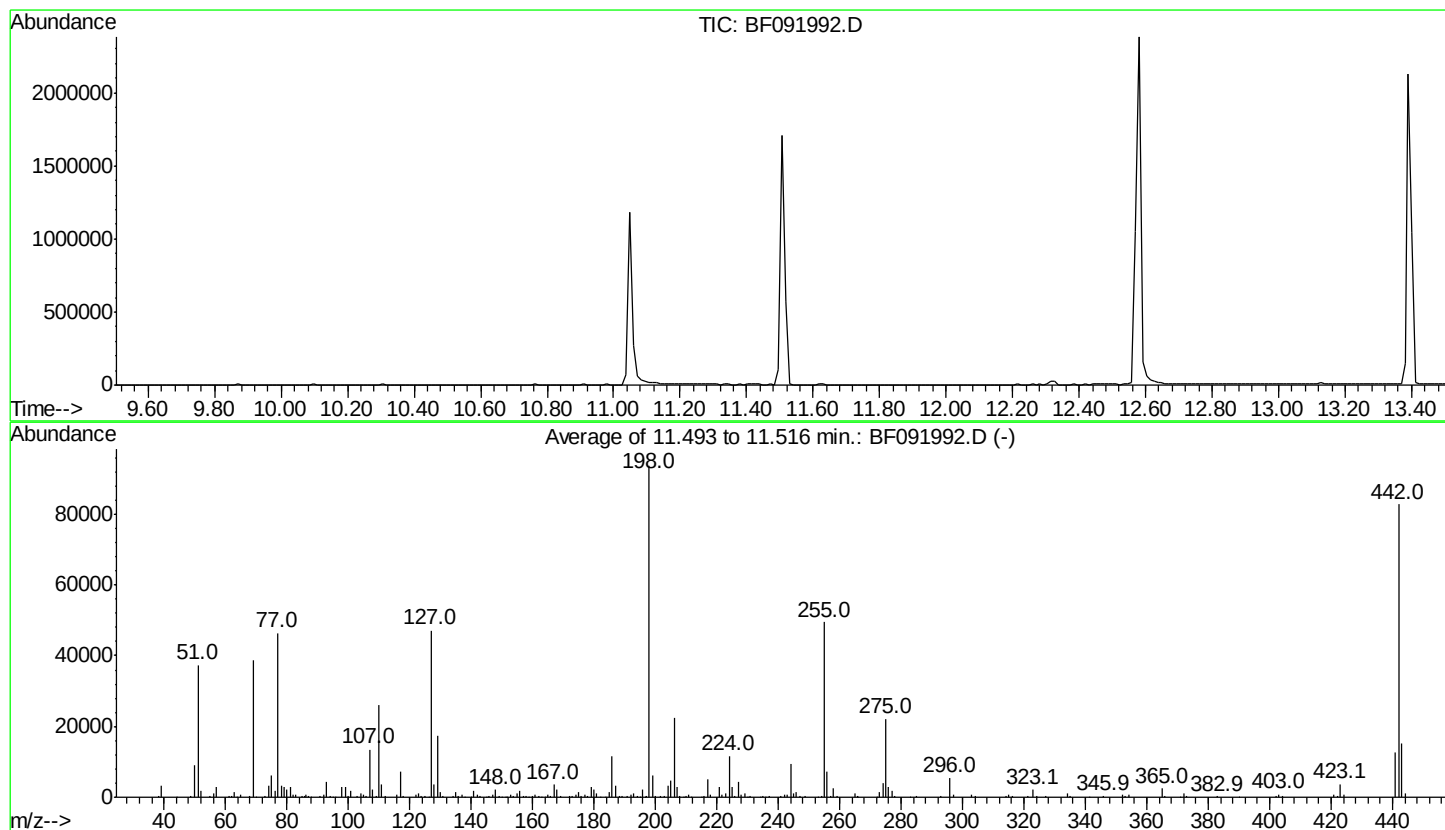

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	37454	PASS
68	69	0.00	2	1.3	512	PASS
69	198	0.00	100	41.3	38709	PASS
70	69	0.00	2	0.4	158	PASS
127	198	10	80	50.3	47143	PASS
197	198	0.00	2	0.5	423	PASS
198	198	100	100	100.0	93725	PASS
199	198	5	9	6.5	6130	PASS
275	198	10	60	23.6	22149	PASS
365	198	1	100	2.6	2420	PASS
441	442	0.01	24	15.5	12847	PASS
442	198	50	100	88.2	82687	PASS
443	442	15	24	18.5	15263	PASS