
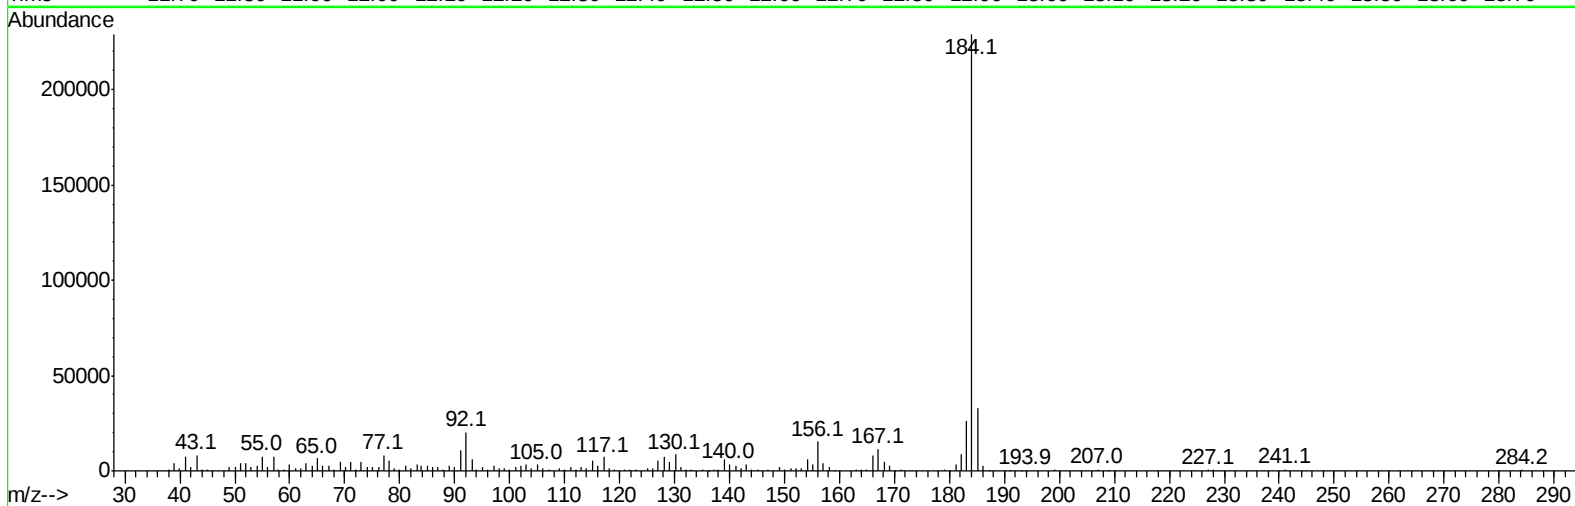


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122817\
Data File : BF101794.D
Acq On : 28 Dec 2017 11:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 05:59:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

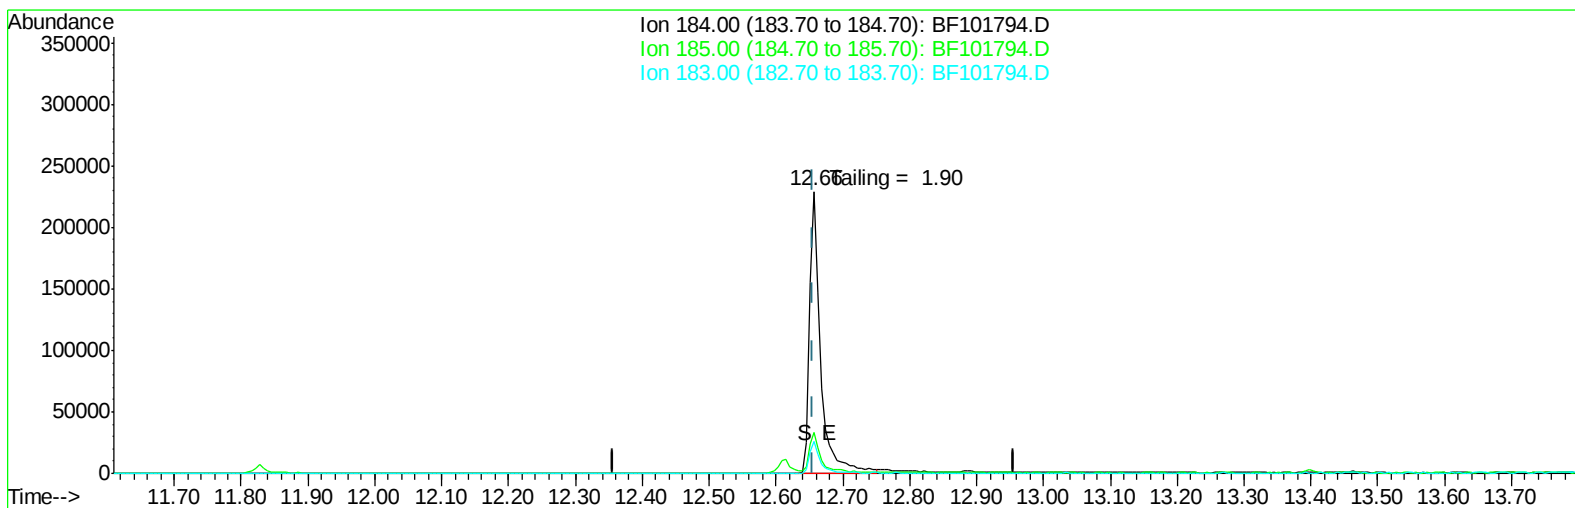

TIC: BF101794.D

(76) Benzidine



12.657min (-0.000) 126.43ng

response 275890

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.48
183.00	11.60	11.57
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122817\
Data File : BF101794.D
Acq On : 28 Dec 2017 11:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 05:59:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

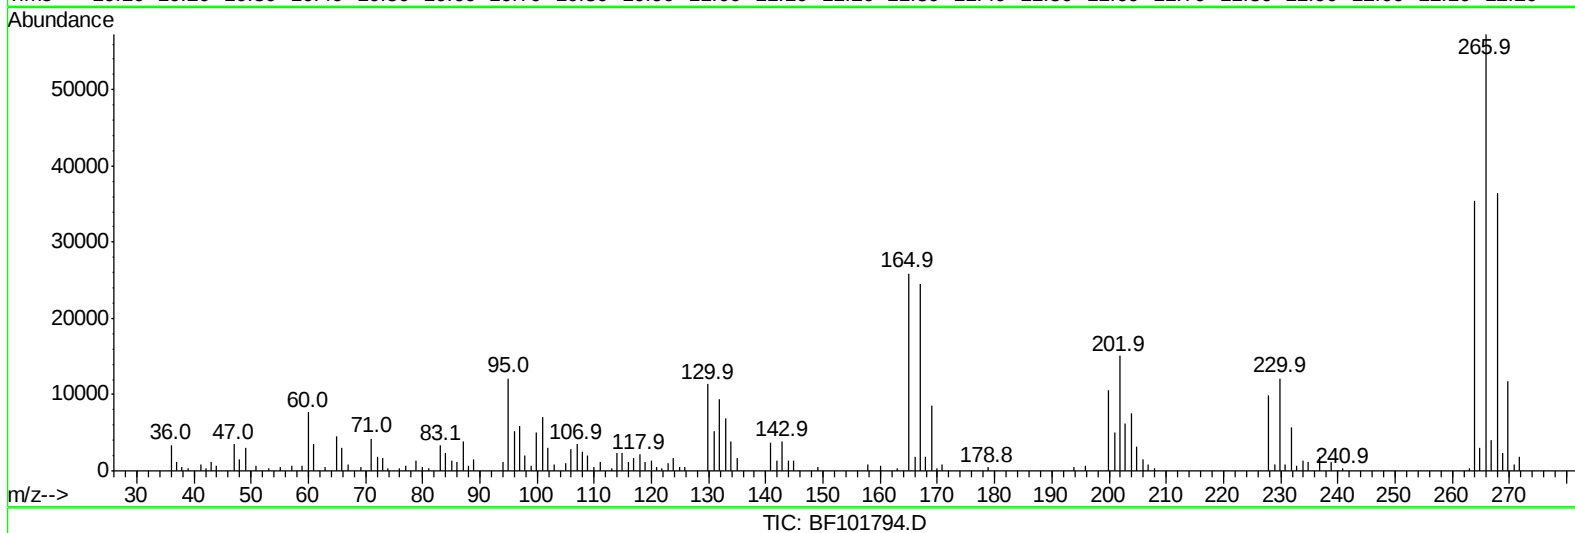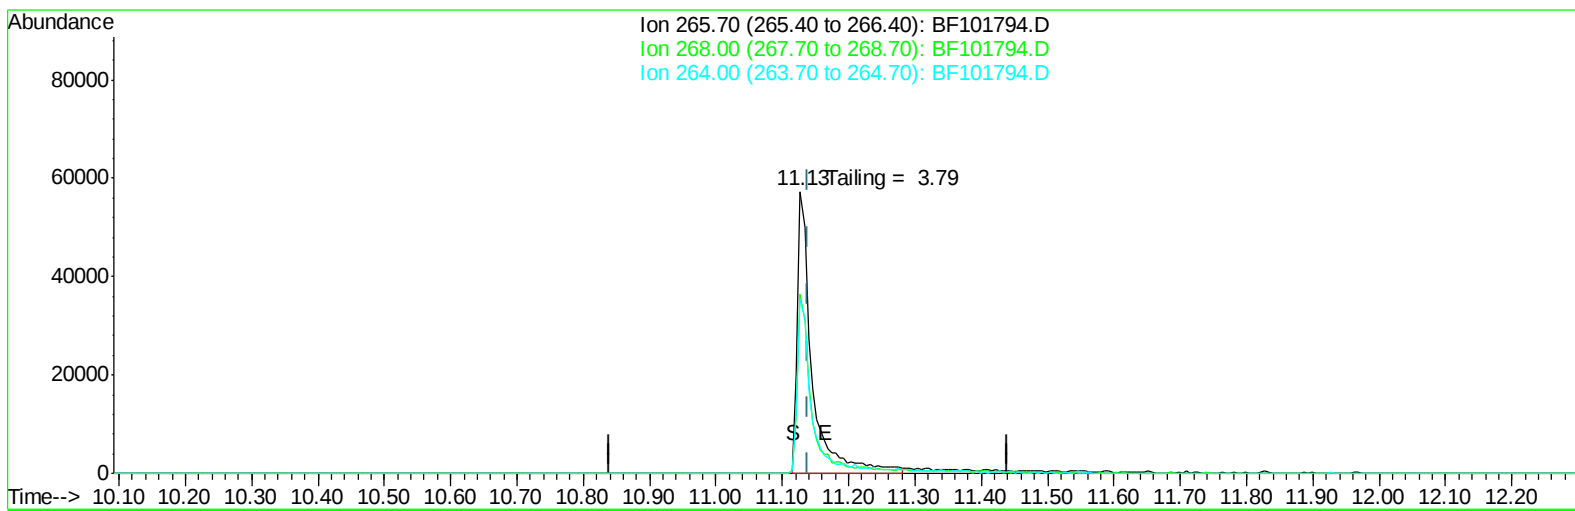

(69) Pentachlorophenol (C)

11.127min (-0.012) 35500.10ng m

response 85107

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.66
264.00	61.90	61.86
0.00	0.00	0.00