


Data Path : Z:\HPCHEM1\BNA F\Data\BF122817\
 Data File : BF101794.D
 Acq On : 28 Dec 2017 11:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 26 10:48:01 2017

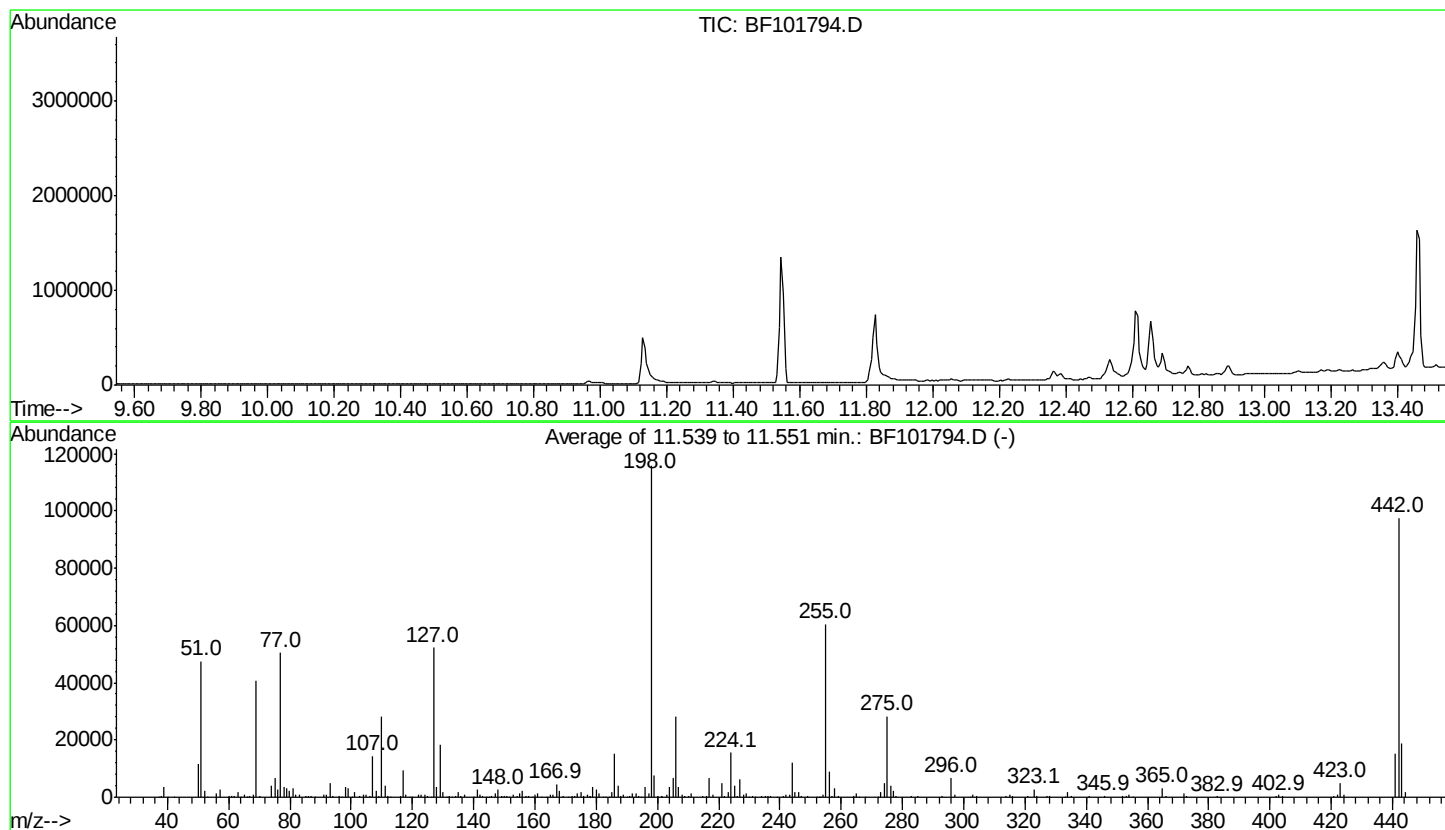

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	47539	PASS
68	69	0.00	2	1.8	723	PASS
69	198	0.00	100	35.1	40627	PASS
70	69	0.00	2	1.3	529	PASS
127	198	10	80	45.0	52114	PASS
197	198	0.00	2	1.0	1203	PASS
198	198	100	100	100.0	115784	PASS
199	198	5	9	6.7	7808	PASS
275	198	10	60	24.4	28245	PASS
365	198	1	100	2.9	3310	PASS
441	443	0.01	100	81.3	15233	PASS
442	198	50	100	84.2	97514	PASS
443	442	15	24	19.2	18737	PASS