
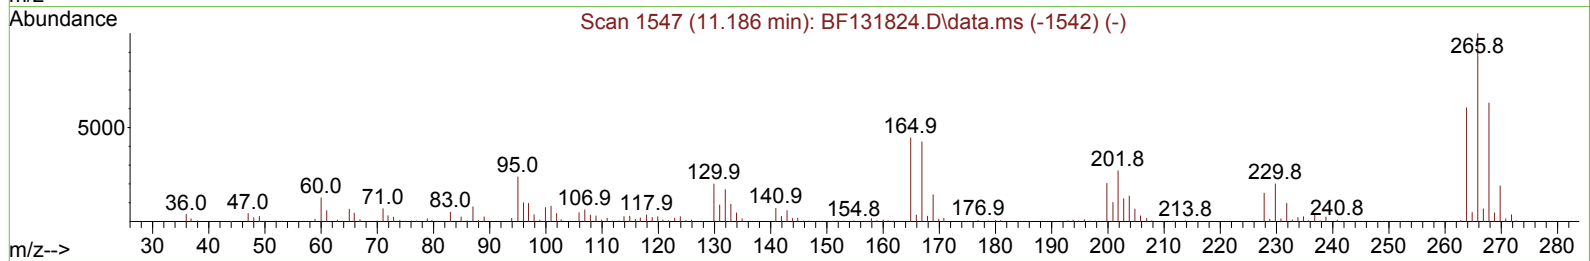
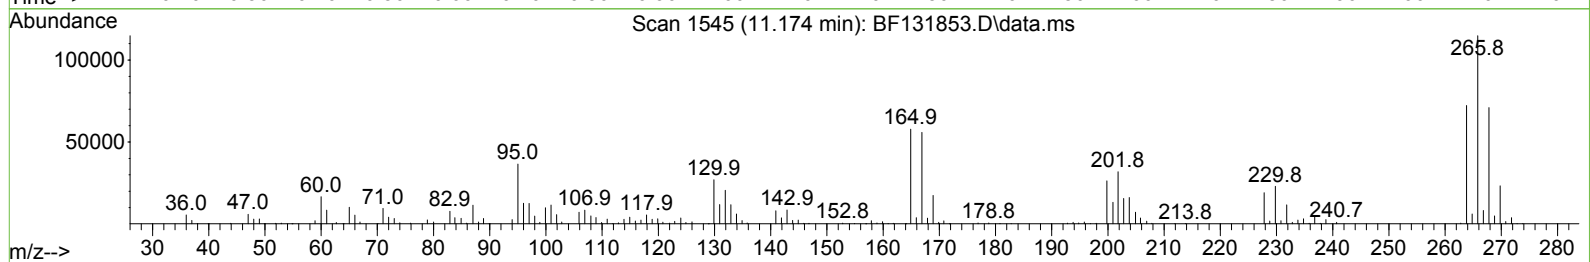


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
Data File : BF131853.D
Acq On : 28 Dec 2022 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 08:34:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

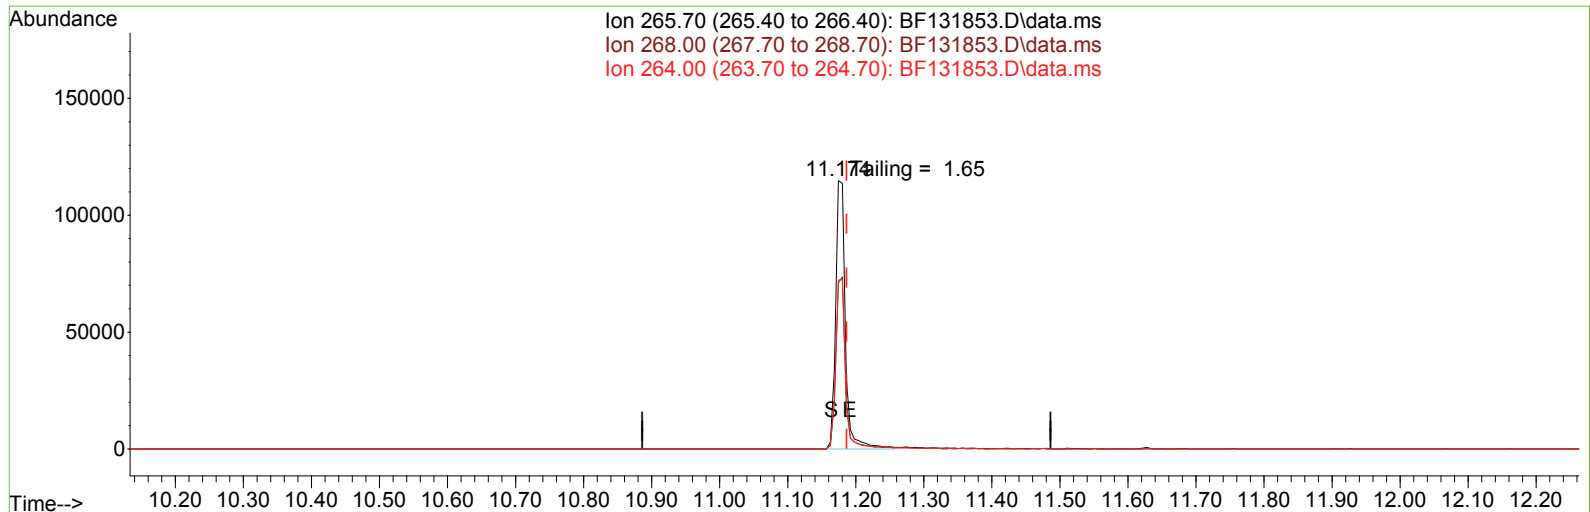

TIC: BF131853.D\data.ms

(70) Pentachlorophenol (C)




11.174min (-0.012) 33559.61 ng

response 114805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.88
264.00	60.40	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122822\
Data File : BF131853.D
Acq On : 28 Dec 2022 10:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 08:34:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

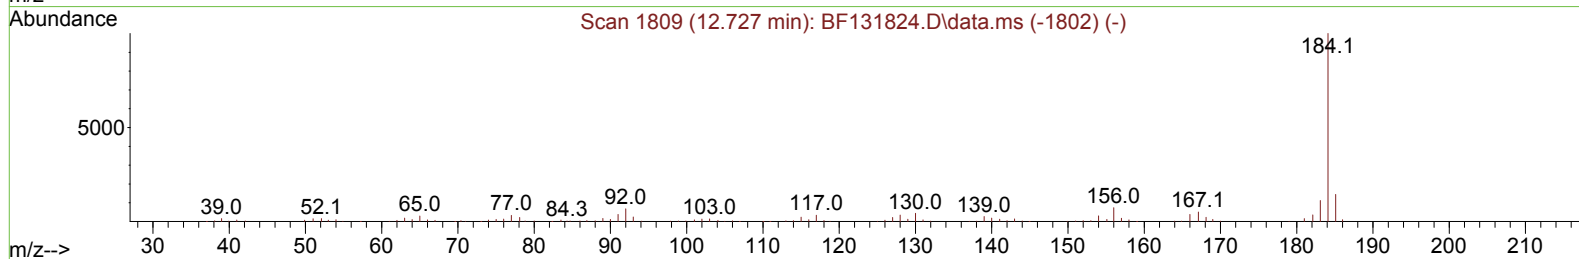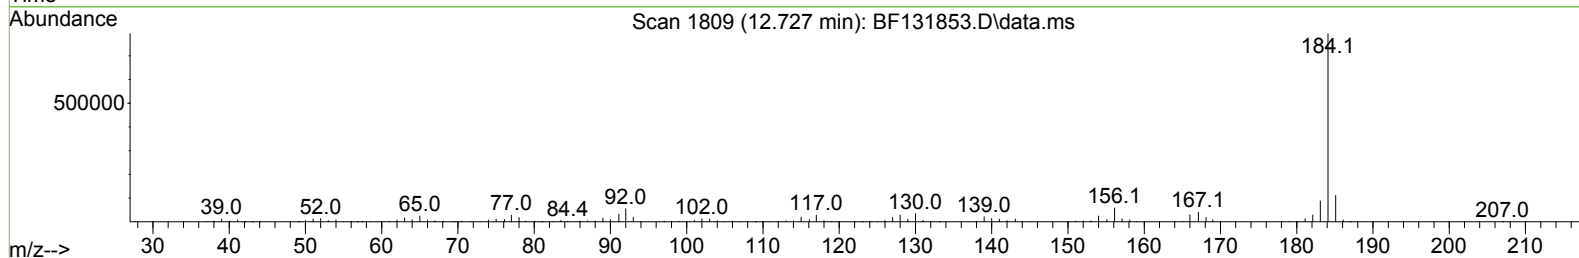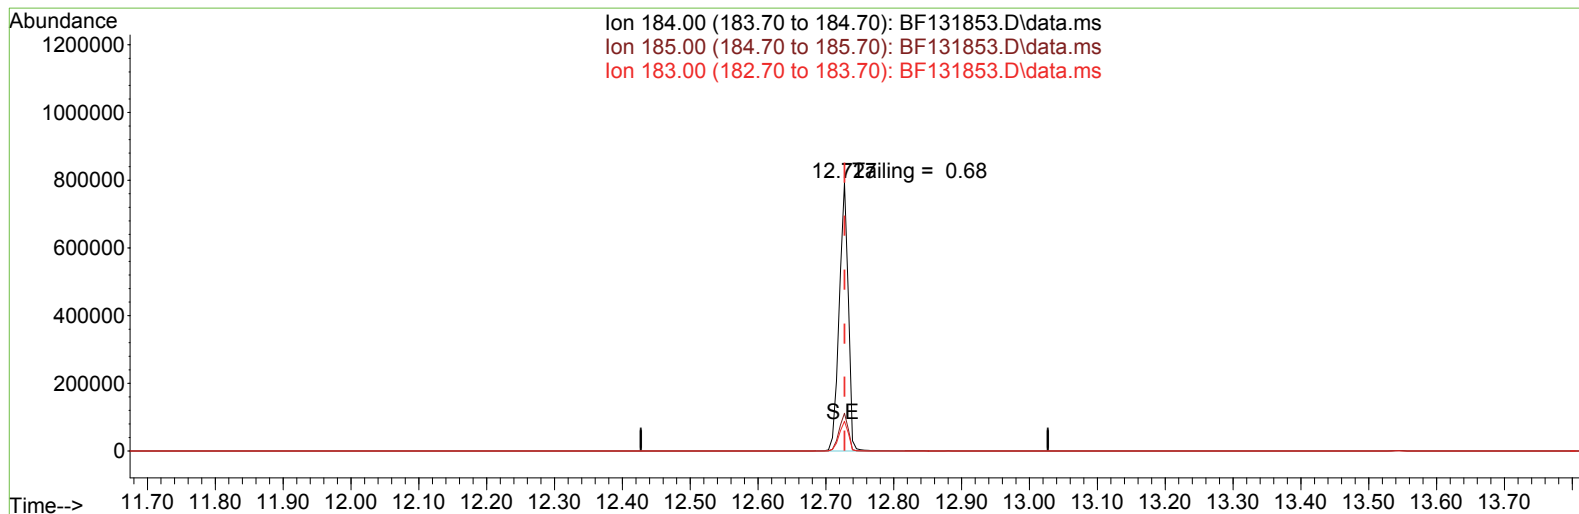

TIC: BF131853.D\data.ms

(77) Benzidine

12.727min (-0.000) 0.00 ng

response 732244

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.10
183.00	11.20	11.10
0.00	0.00	0.00